


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111723\
Data File : VX038893.D
Acq On : 17 Nov 2023 21:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Title : SW846 8260
Last Update : Thu Nov 16 22:59:22 2023

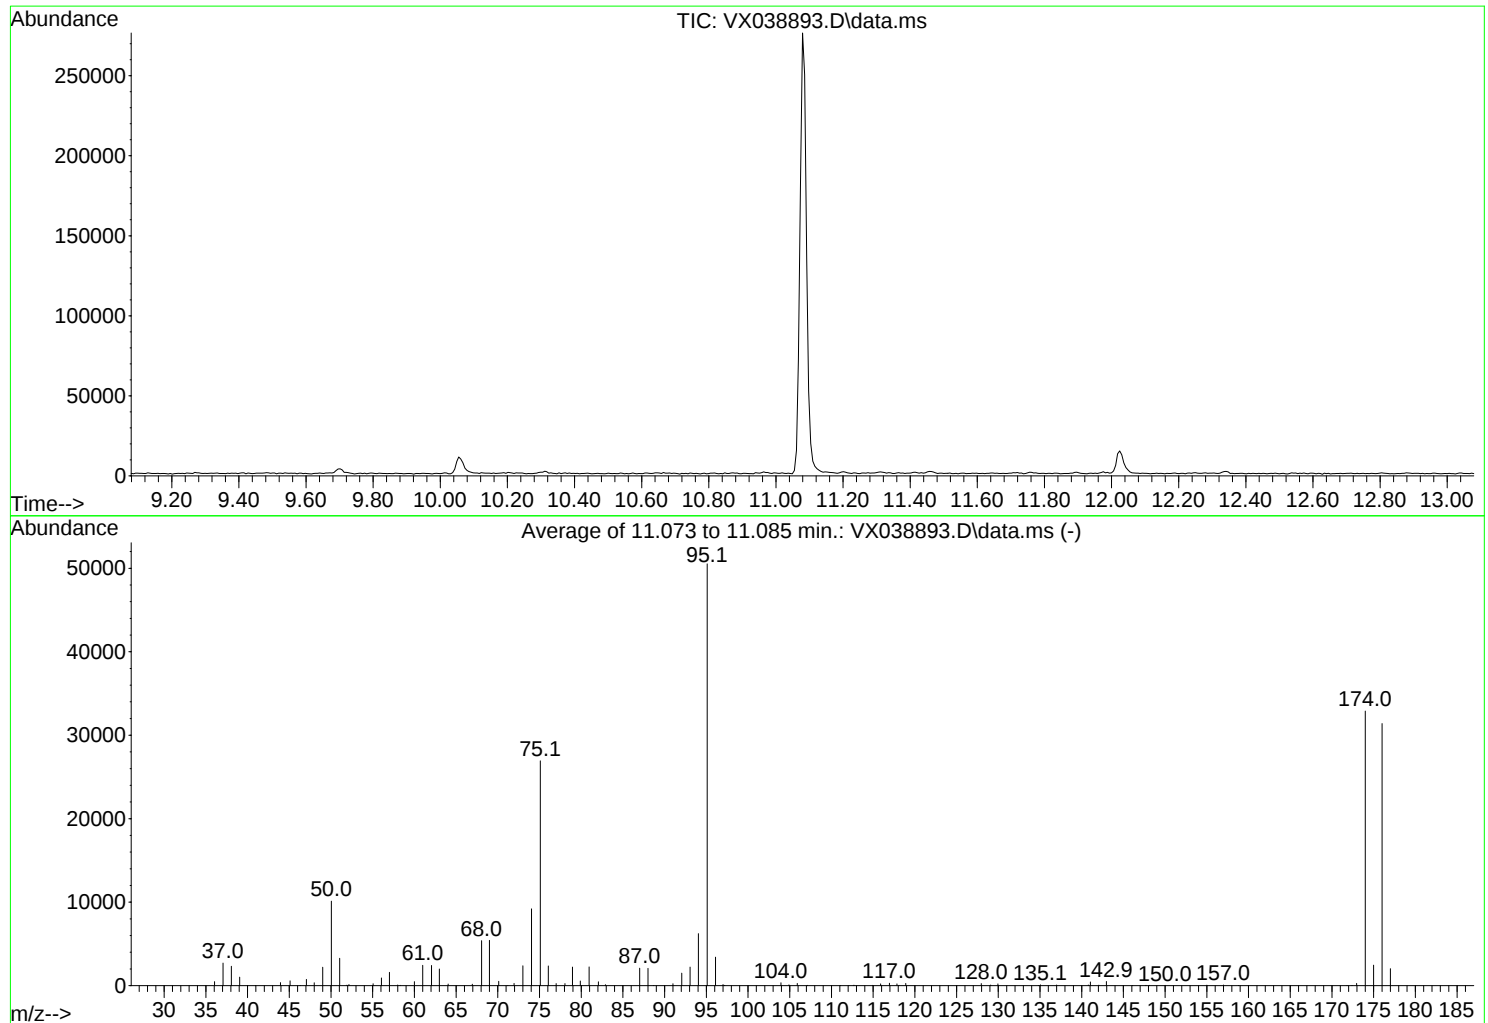

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	10125	PASS
75	95	30	60	53.3	26939	PASS
95	95	100	100	100.0	50536	PASS
96	95	5	9	6.8	3416	PASS
173	174	0.00	2	0.8	278	PASS
174	95	50	100	65.1	32893	PASS
175	174	5	9	7.5	2460	PASS
176	174	95	101	95.5	31400	PASS
177	176	5	9	6.5	2043	PASS