

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX111820\
 Data File : VX019449.D
 Acq On : 18 Nov 2020 12:25
 Operator : JC/MD
 Sample : VSTDCCC0.5EC
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD0.5214

Quant Time: Nov 19 12:14:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 18 17:44:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.82	114	16736	0.50	ug/L	0.00
5) Chlorobenzene-d5	10.09	117	14212	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	12.06	152	8191	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.39	65	8347	0.47	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	94.00%
4) 1,2-Dichloroethane-d4	6.01	65	7268	0.46	ug/L	-0.02
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.00%
7) 1,2-Dichloropropane-d6	7.35	67	7501	0.58	ug/L	-0.02
Spiked Amount	0.500	Range	60 - 140	Recovery	=	116.00%
8) Toluene-d8	8.68	98	19443	0.54	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.00%
10) 1,1,2,2-Tetrachloroethane-	11.22	84	4306	0.47	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	94.00%

Target Compounds


					Qvalue
3) Vinyl chloride	1.39	62	7045	0.433	ug/L 96
6) Trichloroethene	7.18	95	6037	0.514	ug/L 95
9) 1,2-Dibromoethane	9.66	107	3058	0.442	ug/L 99
12) 1,2,3-Trichloropropane	11.27	75	3007	0.371	ug/L 95
13) 1,2-Dibromo-3-chloropropan	12.97	75	473	0.340	ug/L 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX111820\
Data File : VX019449.D
Acq On : 18 Nov 2020 12:25
Operator : JC/MD
Sample : VSTDCCC0.5EC
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTD0.5214

Quant Time: Nov 19 12:14:06 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 18 17:44:43 2020
Response via : Initial Calibration

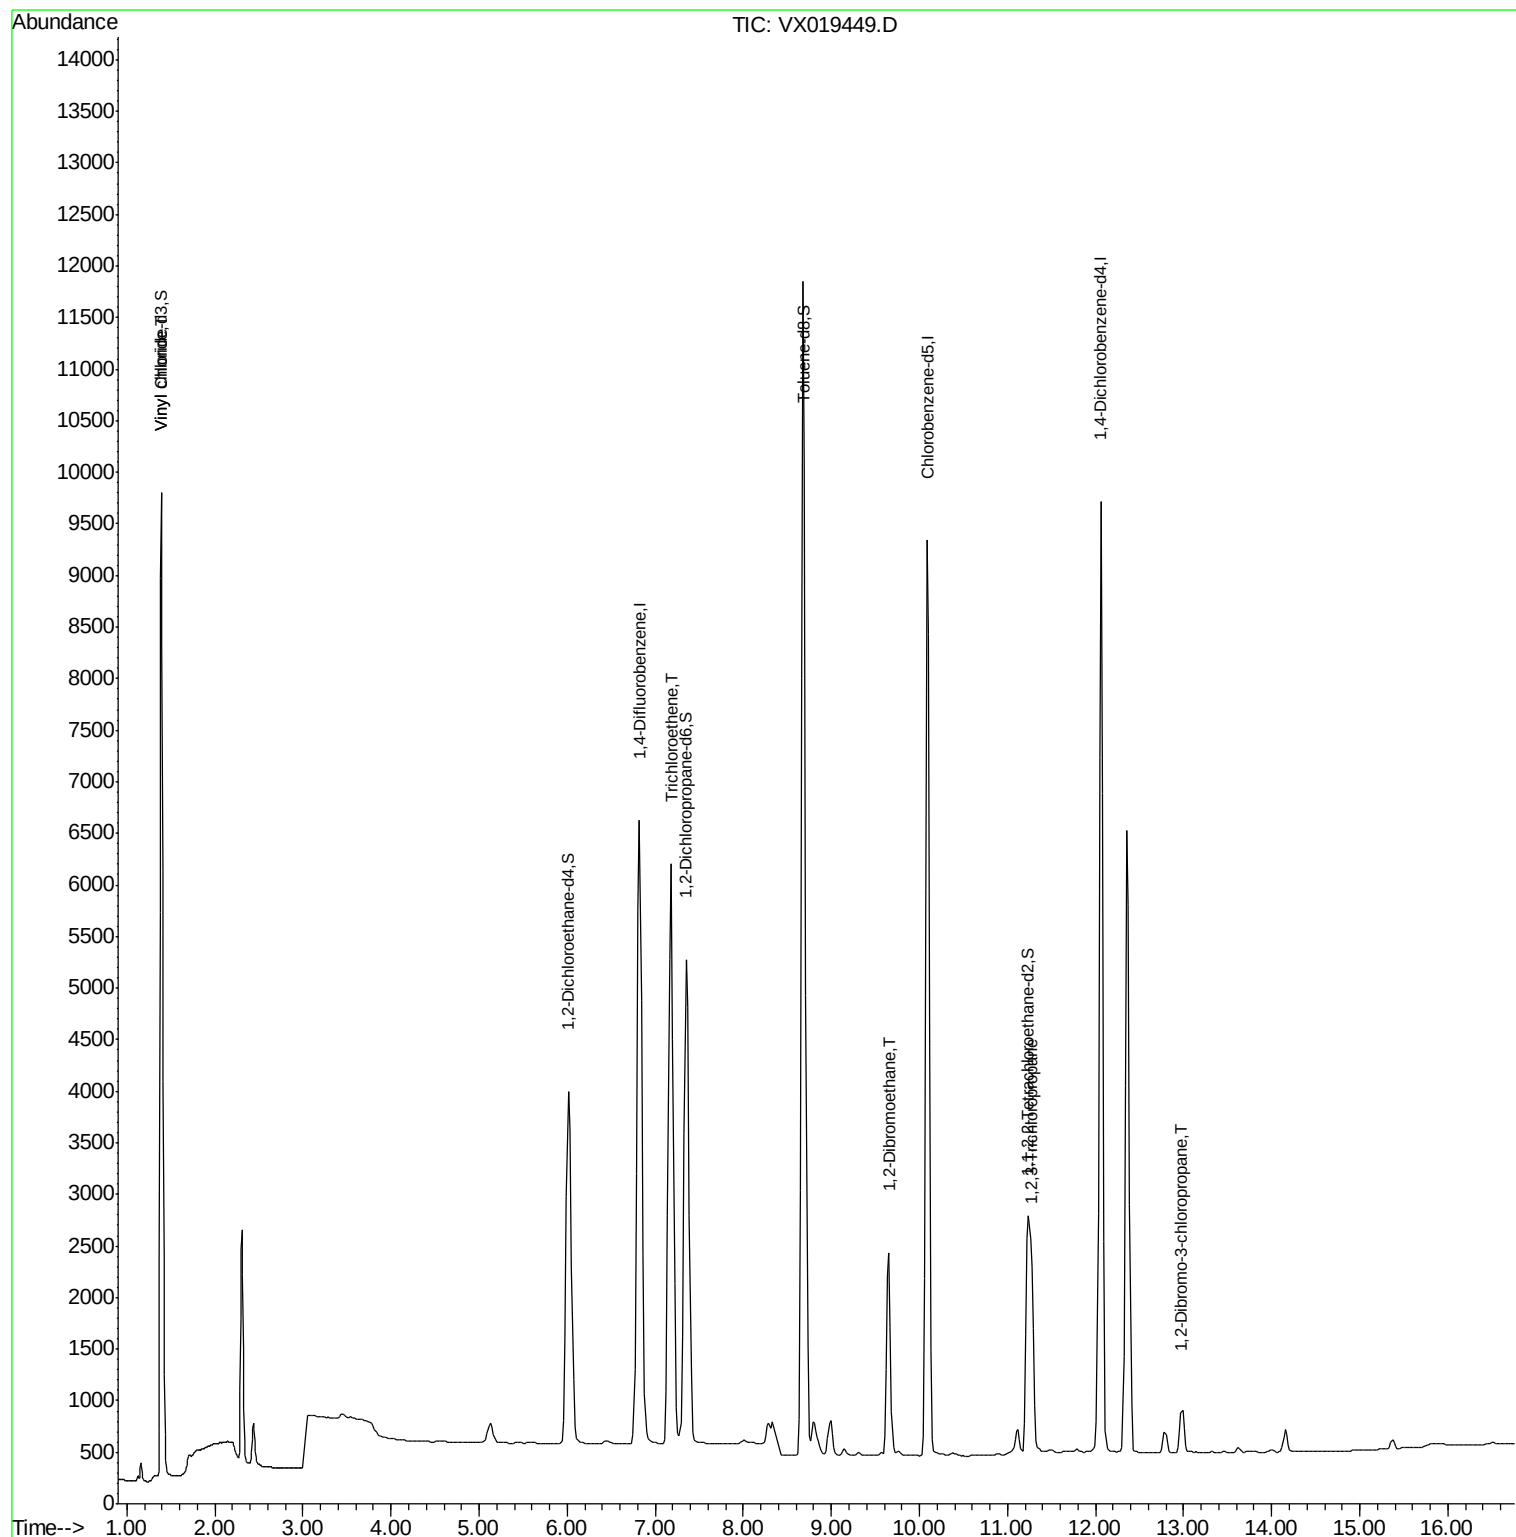

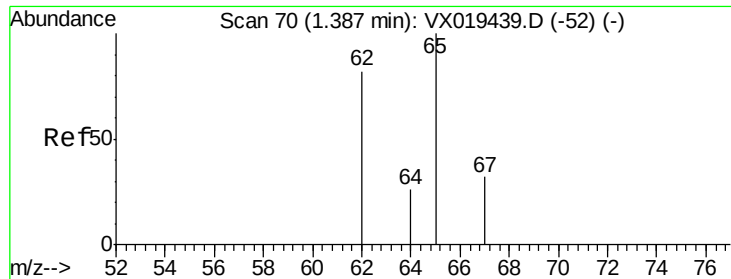

#3

Vinyl chloride

Concen: 0.433 ug/L

RT: 1.39 min Scan# 71

Delta R.T. 0.01 min

Lab File: VX019449.D

Acq: 18 Nov 2020 12:25

Instrument :

MSVOA_X

ClientSampleId :





VSTD0.5214

Tot Ion: 62 Resp: 7045

Ion Ratio Lower Upper

62 100

64 34.4 22.5 41.7

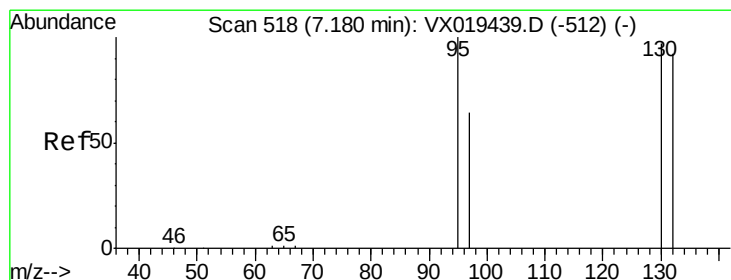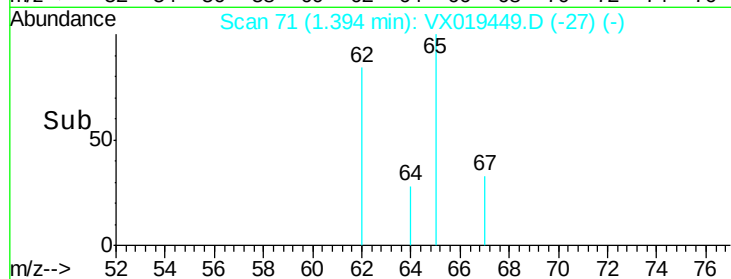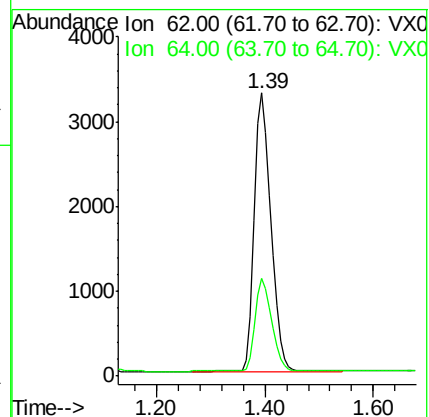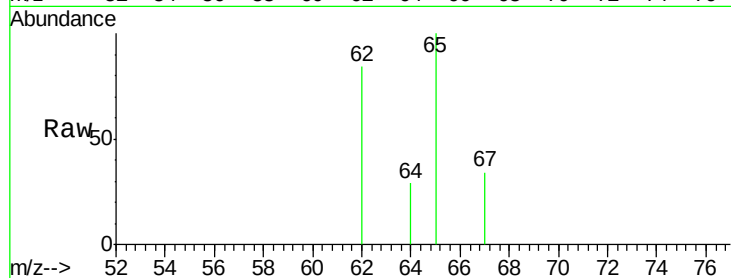

#6

Trichloroethene

Concen: 0.514 ug/L

RT: 7.18 min Scan# 518

Delta R.T. -0.00 min

Lab File: VX019449.D

Acq: 18 Nov 2020 12:25

Tgt Ion: 95 Resp: 6037




Ion Ratio Lower Upper


95 100

97 66.2 45.2 84.0

132 94.6 61.0 113.4

130 98.7 65.6 121.8

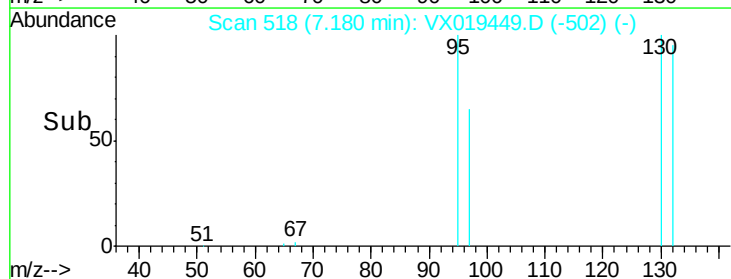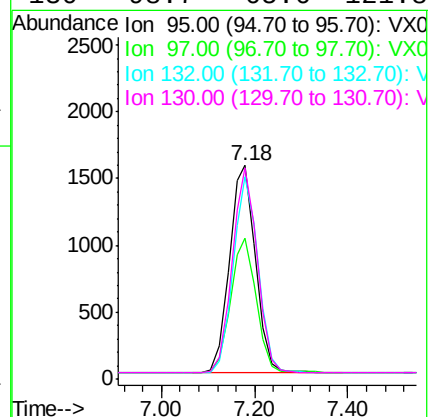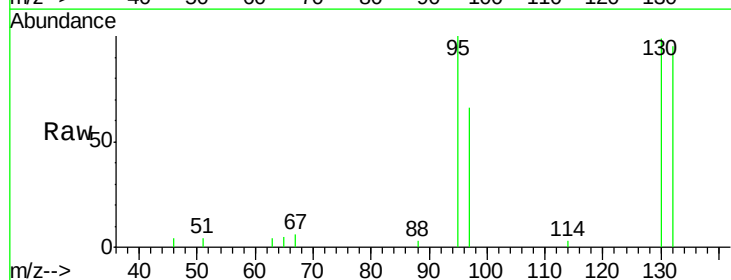

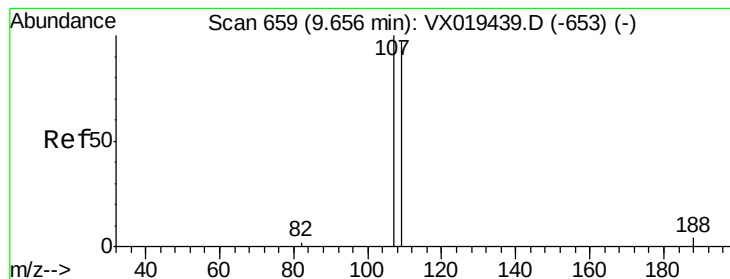

#9

1,2-Dibromoethane

Concen: 0.442 ug/L

RT: 9.66 min Scan# 659

Delta R.T. -0.00 min

Lab File: VX019449.D

Acq: 18 Nov 2020 12:25

Instrument :

MSVOA_X

ClientSampled :

VSTD0.5214


Tot Ion:107 Resp: 3058

Ion Ratio Lower Upper

107 100

109 95.7 67.5 125.3




188 7.7 5.5 8.3

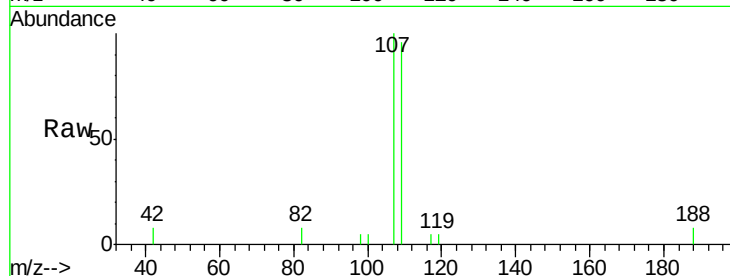

Abundance Ion 107.00 (106.70 to 107.70): V

Ion 109.00 (108.70 to 109.70): V

Ion 188.00 (187.70 to 188.70): V

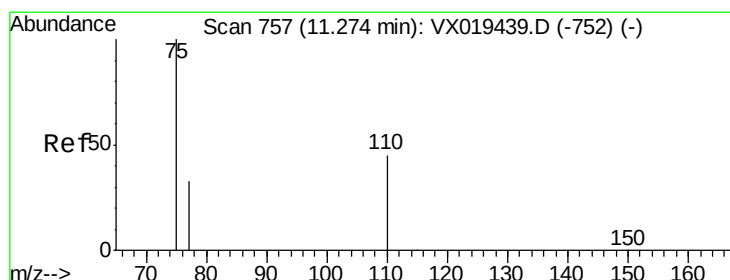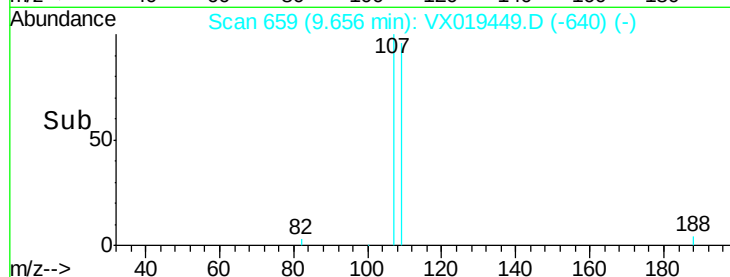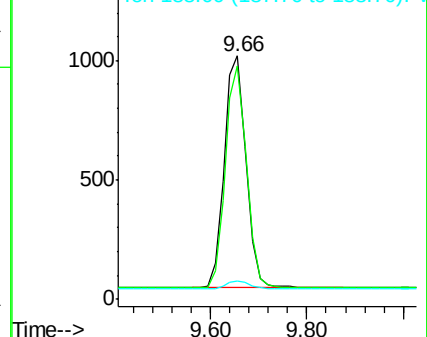

#12

1,2,3-Trichloropropane

Concen: 0.371 ug/L

RT: 11.27 min Scan# 757

Delta R.T. -0.00 min

Lab File: VX019449.D

Acq: 18 Nov 2020 12:25


Tgt Ion: 75 Resp: 3007

Ion Ratio Lower Upper

75 100

110 38.2 33.0 49.4



77 35.7 26.6 39.8



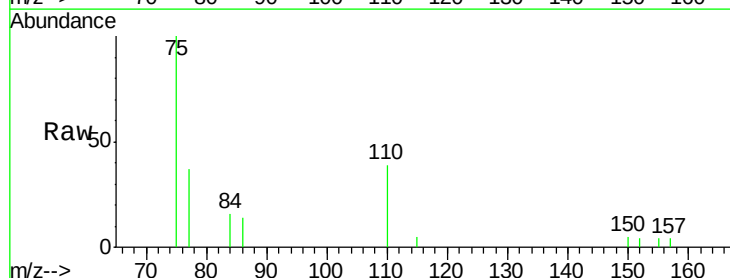


Abundance Ion 75.00 (74.70 to 75.70): VX0

Ion 110.00 (109.70 to 110.70): V

Ion 77.00 (76.70 to 77.70): VX0

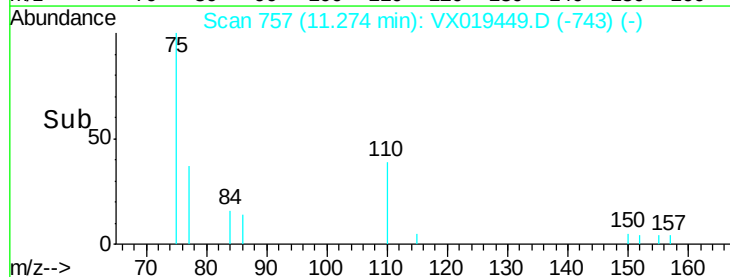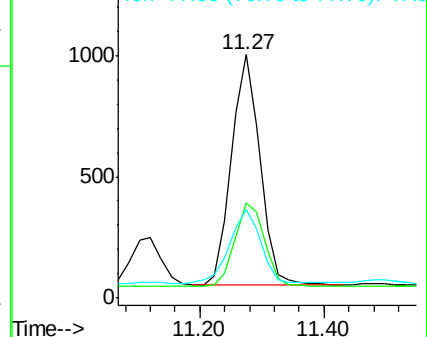

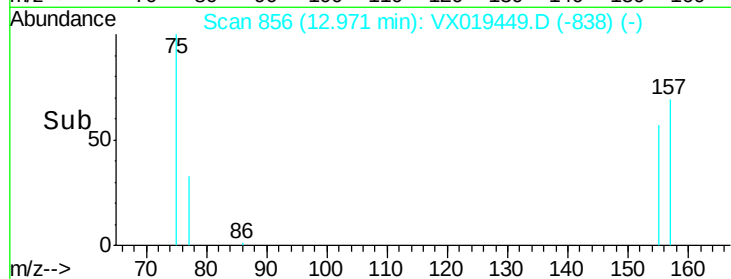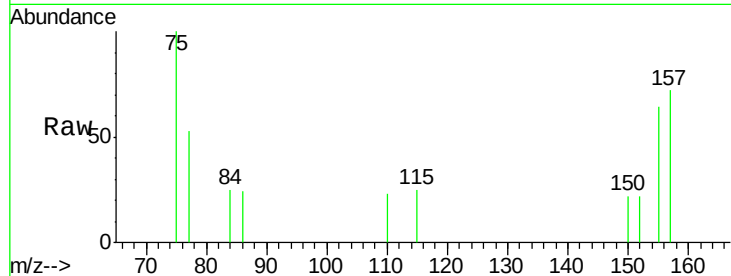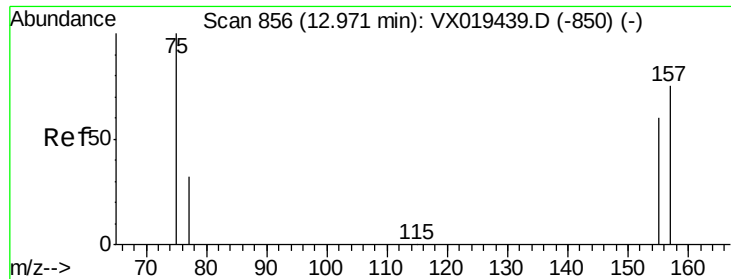

#13

1,2-Dibromo-3-chloropropane

Concen: 0.340 ug/L

RT: 12.97 min Scan# 856

Delta R.T. -0.00 min

Lab File: VX019449.D

Acq: 18 Nov 2020 12:25

Instrument :

MSVOA_X

ClientSampleId :

VSTD0.5214

Tot Ion: 75 Resp: 473

Ion Ratio Lower Upper

75 100

157 71.8 59.6 89.4

155 63.6 50.6 76.0

