


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX111820\
Data File : VX019445.D
Acq On : 18 Nov 2020 08:55
Operator : JC/MD
Sample : BFB06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
Title : TRACE VOA SOM01.0
Last Update : Wed Nov 18 17:44:43 2020

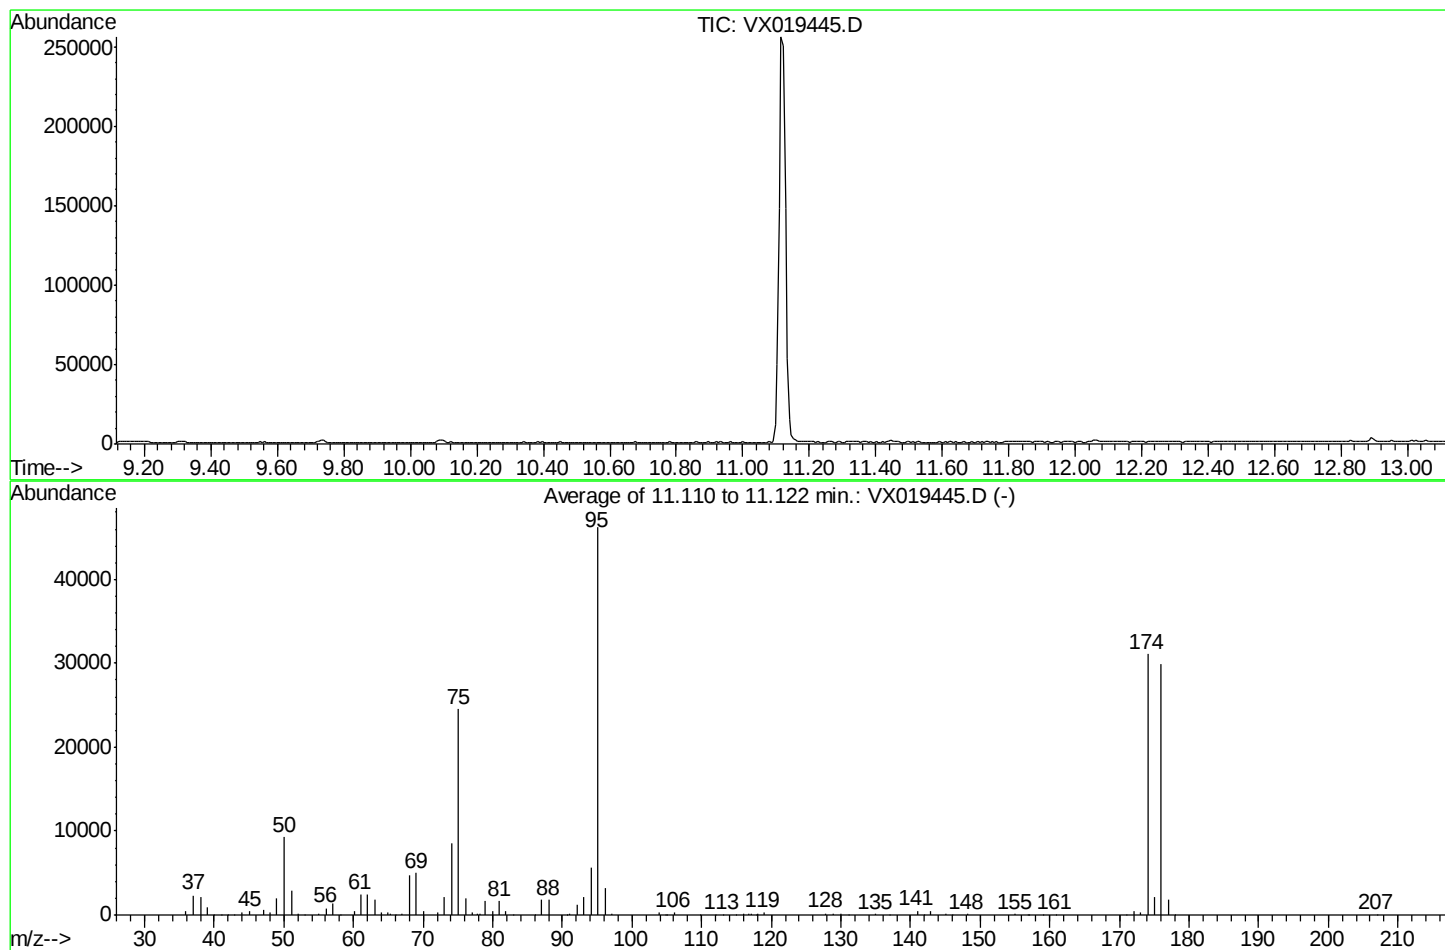

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	9294	PASS
75	95	30	80	53.1	24533	PASS
95	95	100	100	100.0	46205	PASS
96	95	5	9	6.8	3149	PASS
173	174	0.00	2	1.0	305	PASS
174	95	50	120	67.2	31064	PASS
175	174	5	9	6.9	2156	PASS
176	174	95	101	96.4	29936	PASS
177	176	5	9	6.3	1877	PASS

m/z	Abundance
36.00	347.0
37.00	1906.0
38.00	1590.0
39.00	719.0
40.00	240.0
42.80	57.0
44.00	685.0
45.20	332.0
47.20	456.0
47.90	218.0
49.00	1611.0
50.00	7440.0
51.10	2059.0
52.00	151.0
55.00	129.0
56.00	582.0
57.10	1092.0
58.00	63.0
60.20	312.0
61.00	1898.0
62.10	1813.0
63.10	1536.0
64.10	249.0
64.90	368.0
66.90	129.0
68.00	3371.0
69.00	3666.0
70.00	409.0
72.00	216.0
73.00	1513.0
74.00	6141.0
75.00	17920.0
76.00	1577.0
77.00	297.0
78.10	163.0
78.90	1203.0
79.90	319.0
81.00	1274.0
81.90	302.0
87.10	1264.0
88.00	1209.0
90.70	90.0
91.10	114.0
92.10	907.0
93.10	1479.0
94.10	3851.0
95.10	31728.0
96.10	2338.0
97.20	136.0
104.00	159.0
105.20	66.0
106.10	162.0
116.00	151.0
117.10	162.0
117.80	105.0
118.20	92.0
119.00	202.0
127.90	111.0
128.70	53.0
130.00	111.0
135.00	73.0
141.00	284.0
142.90	256.0
145.10	56.0
155.00	57.0
156.90	63.0
172.10	250.0
174.10	17688.0
175.00	1134.0
176.00	18336.0
177.10	975.0
206.90	67.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

m/z	Abundance
35.90	492.0
37.10	2702.0
38.00	2740.0
39.10	1294.0
40.00	230.0
40.90	59.0
41.90	75.0
42.90	111.0
44.00	915.0
45.10	558.0
47.10	517.0
48.00	432.0
49.00	2107.0
50.00	10722.0
51.00	3642.0
52.10	202.0
53.10	80.0
54.90	195.0
56.10	864.0
57.10	1630.0
58.10	83.0
60.10	553.0
61.00	2945.0
62.00	2667.0
63.00	2173.0
64.10	255.0
65.20	402.0
66.10	79.0
67.00	214.0
68.00	5971.0
69.00	5752.0
70.00	491.0
72.10	394.0
73.00	2705.0
74.00	9759.0
75.10	28664.0
76.10	2473.0
77.10	384.0
77.80	352.0
79.00	1840.0
79.90	567.0
81.00	1854.0
81.90	498.0
83.00	65.0
86.00	80.0
87.00	2190.0
88.00	2263.0
90.90	209.0
92.00	1542.0
93.00	2642.0
94.10	6734.0
95.10	54936.0
96.10	3623.0
97.10	99.0
103.80	293.0
104.80	140.0
106.00	339.0
109.80	55.0
113.00	80.0
114.90	73.0
115.90	165.0
116.80	357.0
118.00	230.0
119.00	332.0
127.90	184.0
128.80	158.0
130.00	158.0
131.10	91.0
135.00	140.0
137.00	79.0
140.90	518.0
142.00	52.0
142.90	524.0
145.10	138.0
146.10	85.0
148.10	122.0
155.00	150.0
157.10	111.0
159.00	66.0
160.80	86.0
171.10	58.0
172.00	515.0
173.00	414.0
174.00	35024.0
175.00	2622.0
176.00	35464.0
177.00	2244.0
178.00	66.0
207.00	71.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

m/z	Abundance
36.00	462.0
37.10	2293.0
38.10	2039.0
39.10	1077.0
40.00	258.0
41.10	67.0
41.90	82.0
43.10	70.0
43.90	991.0
45.00	455.0
47.10	729.0
47.90	337.0
49.00	2161.0
50.10	9722.0
51.10	2890.0
52.10	164.0
53.00	93.0
55.00	176.0
56.00	1026.0
57.10	1557.0
58.00	98.0
60.00	486.0
61.00	2371.0
62.00	2651.0
63.00	2017.0
64.00	326.0
65.00	559.0
65.90	82.0
67.00	186.0
68.10	4909.0
69.00	5482.0
70.10	393.0
72.00	276.0
73.00	2260.0
74.10	9673.0
75.00	27016.0
76.10	2081.0
77.00	376.0
78.10	228.0
79.00	1842.0
80.00	606.0
80.90	1721.0
81.80	532.0
83.00	79.0
86.00	116.0
86.90	1962.0
88.10	1950.0
90.90	259.0
92.00	1405.0
93.00	2149.0
94.10	6153.0
95.00	51952.0
96.10	3487.0
97.10	101.0
104.00	280.0
105.00	139.0
106.00	297.0
111.90	56.0
113.00	64.0
115.90	204.0
117.00	377.0
118.00	266.0
118.90	258.0
127.70	218.0
128.90	103.0
130.00	232.0
131.00	62.0
135.00	106.0
136.90	108.0
140.90	637.0
142.00	103.0
143.00	595.0
144.90	130.0
146.00	106.0
148.20	155.0
155.00	135.0
156.90	114.0
159.10	56.0
160.90	76.0
171.00	62.0
172.10	567.0
173.10	501.0
174.00	40480.0
175.00	2713.0
176.00	36008.0
177.00	2412.0
178.00	80.0
207.30	82.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06

Scan 1638 (11.073 min): VX019445.D
BFB06

m/z	Abundance
39.10	61.0
40.00	215.0
40.90	71.0
43.10	71.0
44.10	543.0
73.00	63.0
207.20	87.0

Instrument :
MSVOA_X
ClientSampleId :
BFB06