

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
 Data File : VX032930.D
 Acq On : 18 Nov 2022 17:14
 Operator : JC/MD
 Sample : N5671-13 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP04-20221115DL

Quant Time: Nov 19 03:08:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	115617	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	194810	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	178567	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	82405	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	83010	51.672	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.340%
35) Dibromofluoromethane	5.385	113	67187	48.350	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.700%
50) Toluene-d8	8.647	98	241539	49.988	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.980%
62) 4-Bromofluorobenzene	11.079	95	92280	48.891	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.780%
Target Compounds						
					Qvalue	
9) 1,1,2-Trichlorotrifluo...	2.337	101	1015	0.818	ug/l	92
20) Methylene Chloride	2.788	84	829	0.619	ug/l #	74
44) Trichloroethene	7.123	130	8950	5.806	ug/l	93
64) Tetrachloroethene	9.275	164	1111	0.850	ug/l #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
Data File : VX032930.D
Acq On : 18 Nov 2022 17:14
Operator : JC/MD
Sample : N5671-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20221115DL

Quant Time: Nov 19 03:08:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration




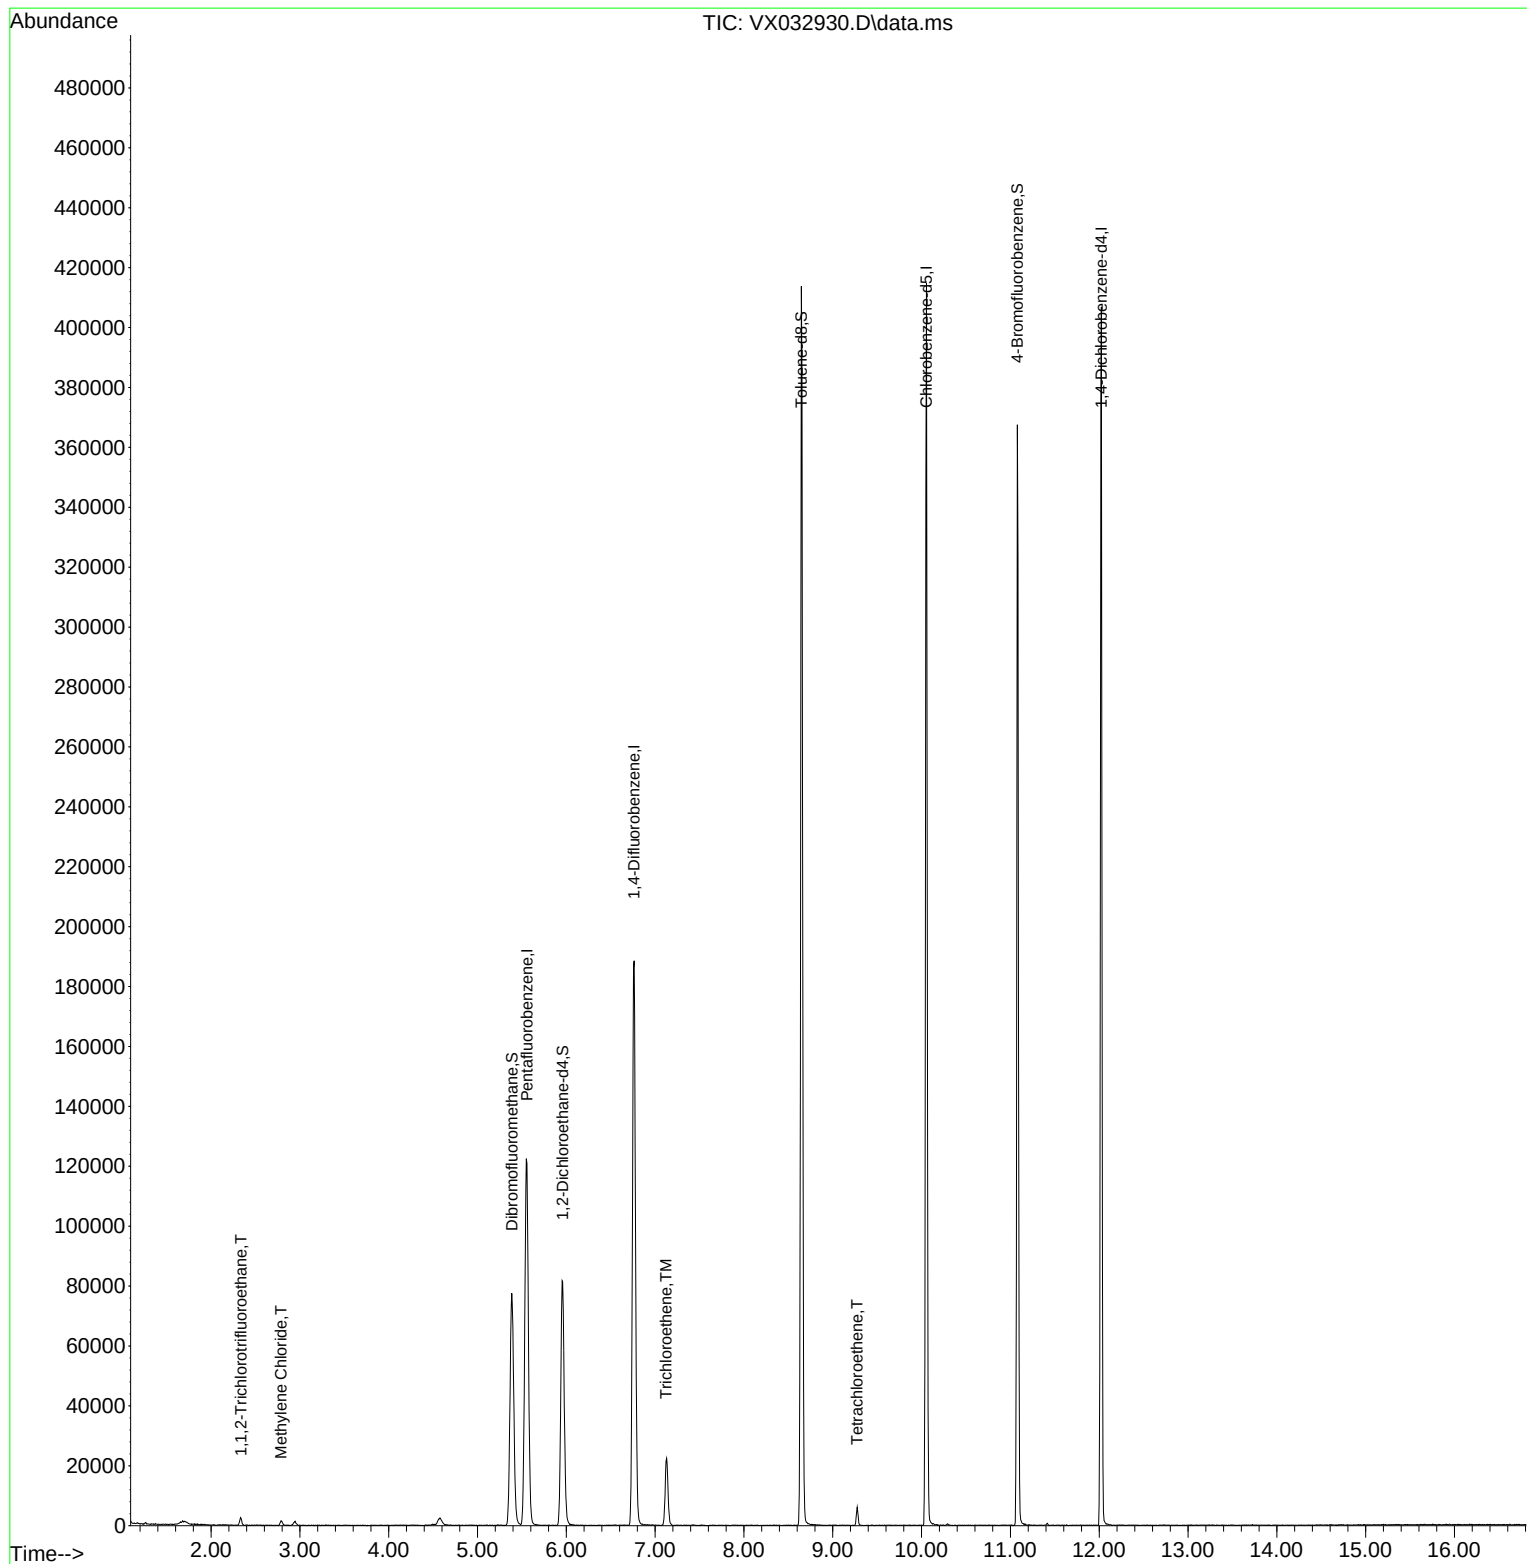


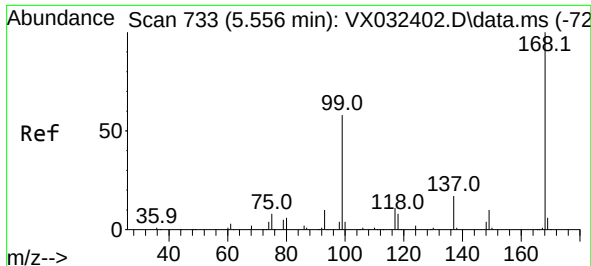

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20221115DL


Tgt Ion:168 Resp: 115617
Ion Ratio Lower Upper
168 100
99 56.6 46.1 69.1

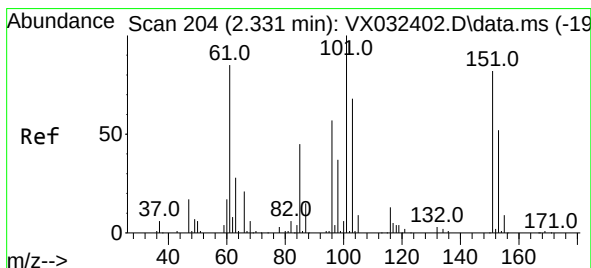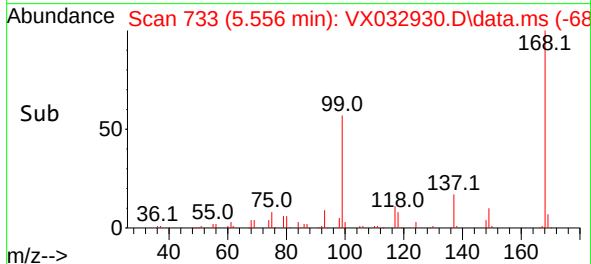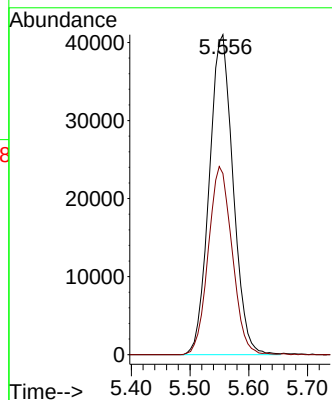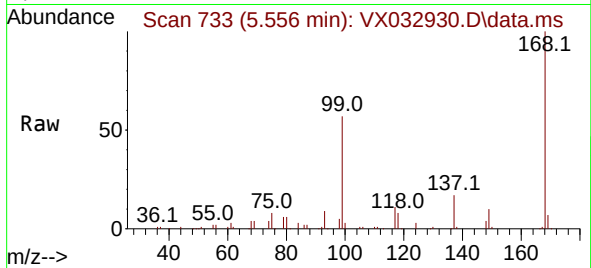

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.818 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.006 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14

Tgt Ion:101 Resp: 1015
Ion Ratio Lower Upper
101 100
85 53.2 37.0 55.4
151 86.0 64.4 96.6

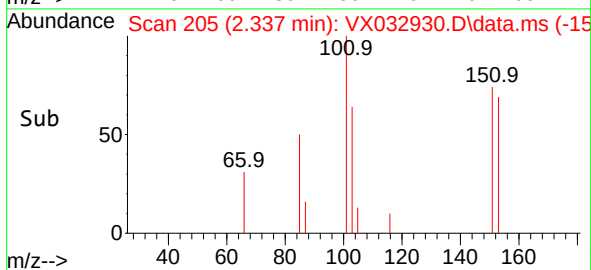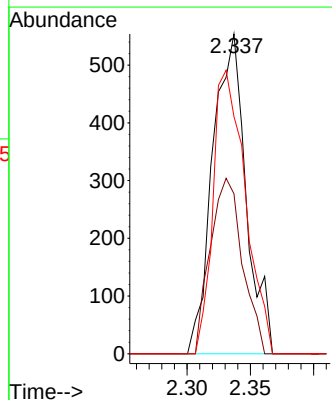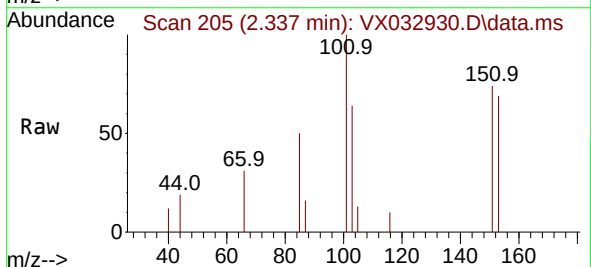

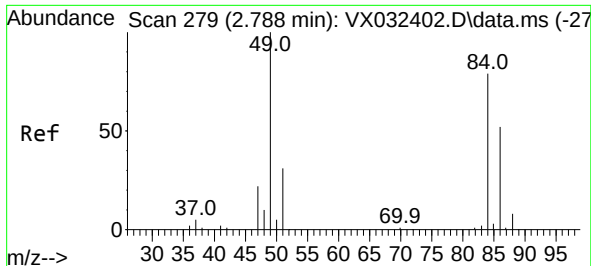

#20

Methylene Chloride

Concen: 0.619 ug/l

RT: 2.788 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX032930.D


Acq: 18 Nov 2022 17:14

Instrument :

MSVOA_X

ClientSampleId :

DUP04-20221115DL

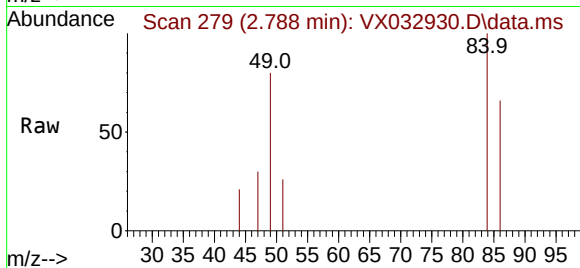

Tgt Ion: 84 Resp: 829




Ion Ratio Lower Upper

84 100

49 80.2 101.0 151.6#

51 26.3 31.1 46.7#

86 65.9 52.3 78.5

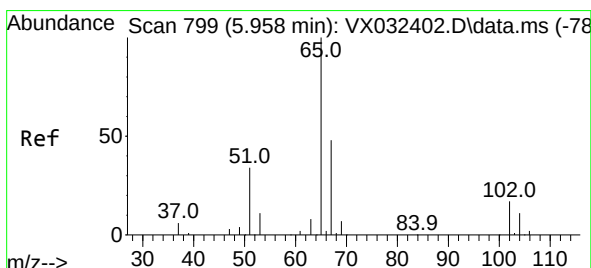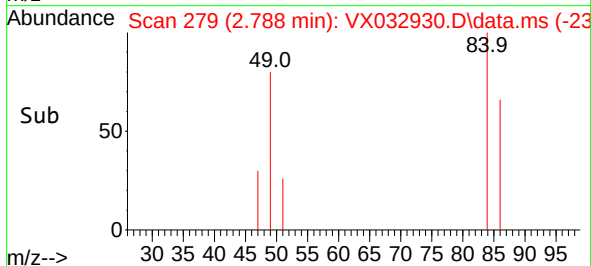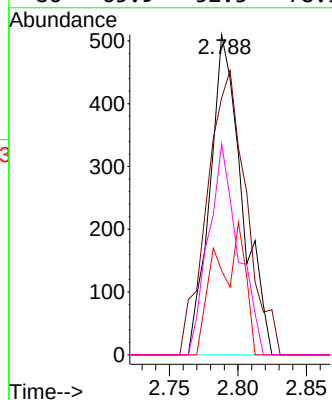

#33

1,2-Dichloroethane-d4

Concen: 51.672 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX032930.D




Acq: 18 Nov 2022 17:14


Tgt Ion: 65 Resp: 83010

Ion Ratio Lower Upper

65 100

67 50.9 0.0 101.8


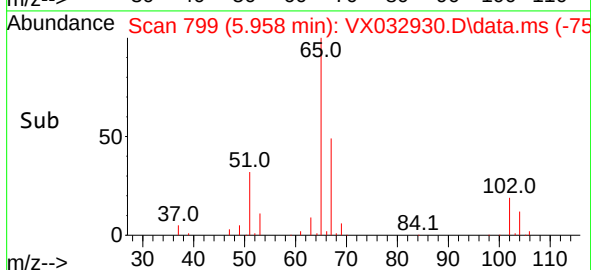
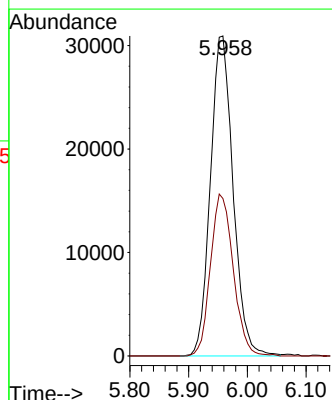
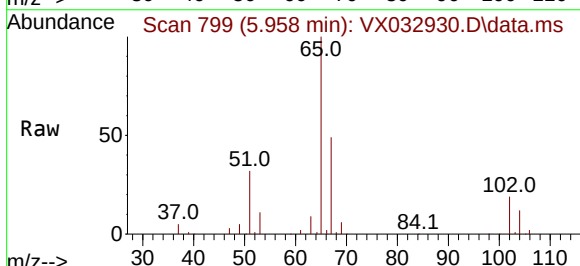


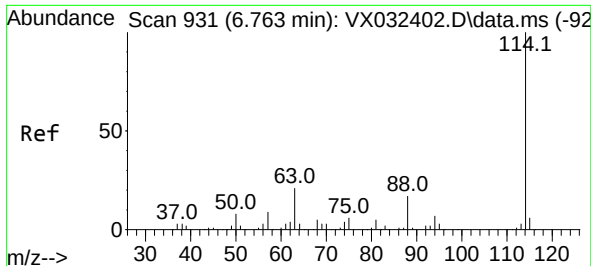

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20221115DL


Tgt Ion:114 Resp: 194810
Ion Ratio Lower Upper
114 100
63 19.7 0.0 41.6
88 15.4 0.0 33.4

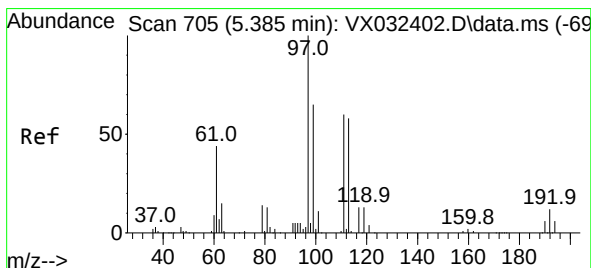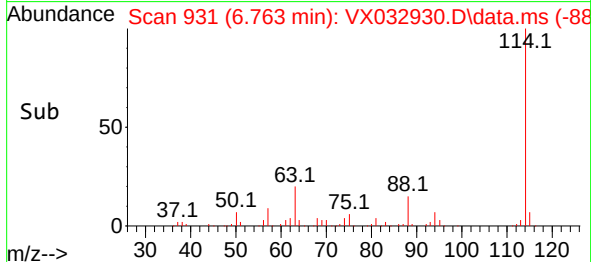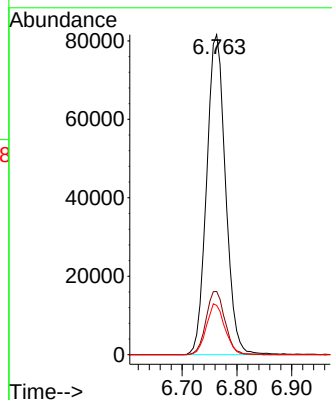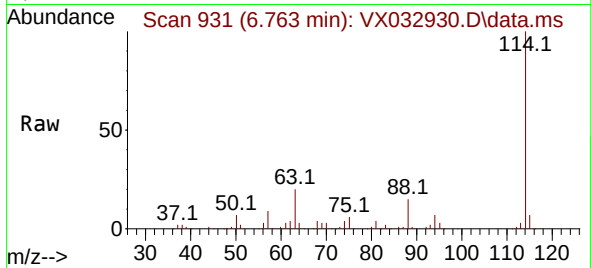

#35
Dibromofluoromethane
Concen: 48.350 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14

Tgt Ion:113 Resp: 67187
Ion Ratio Lower Upper
113 100
111 103.5 82.4 123.6
192 19.5 15.4 23.2


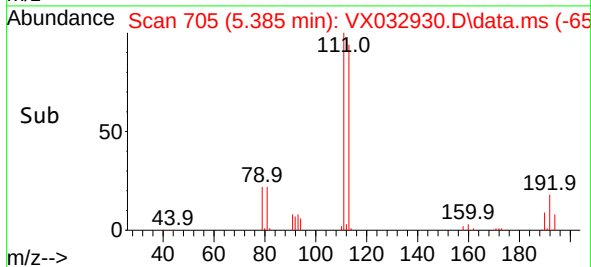
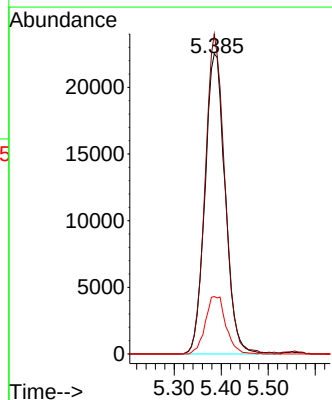
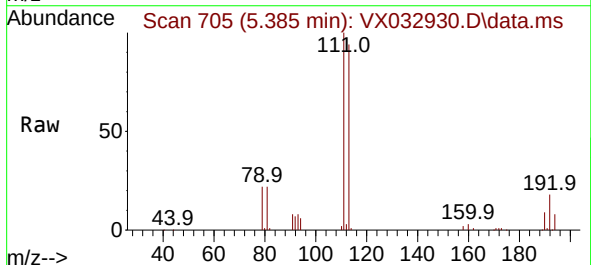


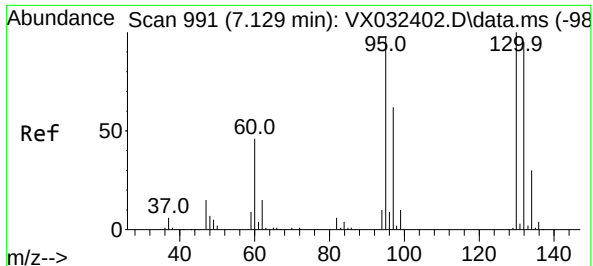

#44
Trichloroethene
Concen: 5.806 ug/l
RT: 7.123 min Scan# 991
Delta R.T. -0.006 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20221115DL


Tgt Ion:130 Resp: 8950
Ion Ratio Lower Upper
130 100
95 90.2 0.0 195.2

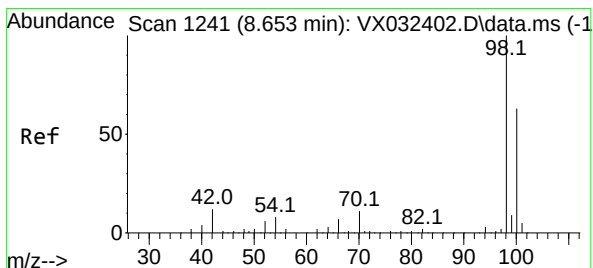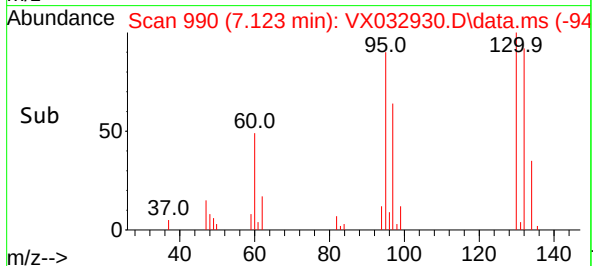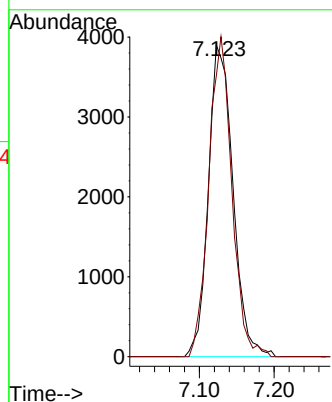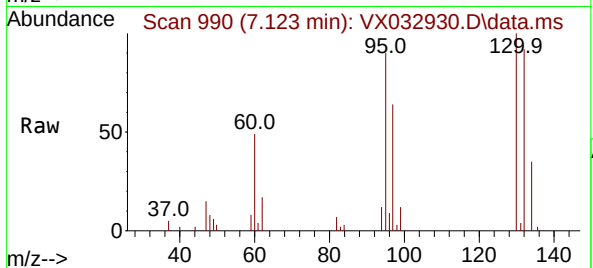

#50
Toluene-d8
Concen: 49.988 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14

Tgt Ion: 98 Resp: 241539
Ion Ratio Lower Upper
98 100
100 64.0 50.9 76.3


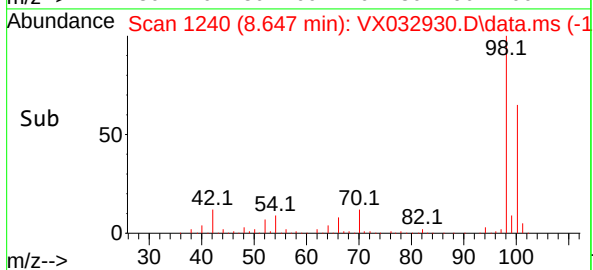
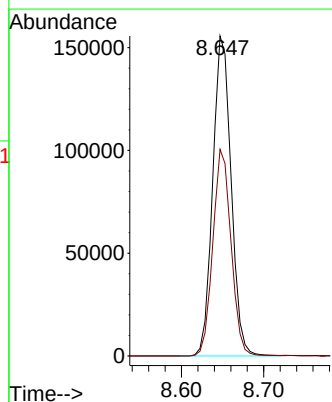
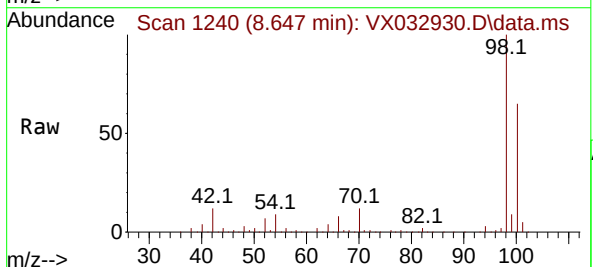


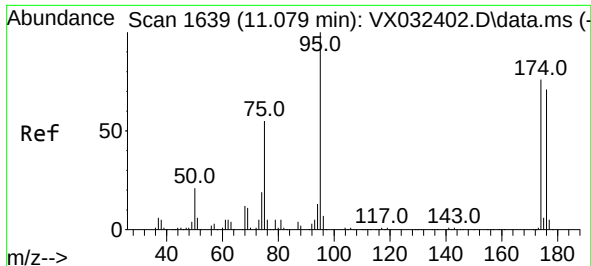

#62
4-Bromofluorobenzene
Concen: 48.891 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14




Instrument :
MSVOA_X
ClientSampleId :
DUP04-20221115DL


Tgt Ion: 95 Resp: 92280
Ion Ratio Lower Upper
95 100
174 82.5 0.0 164.0
176 79.4 0.0 154.4

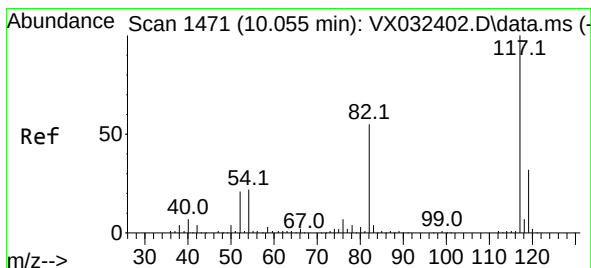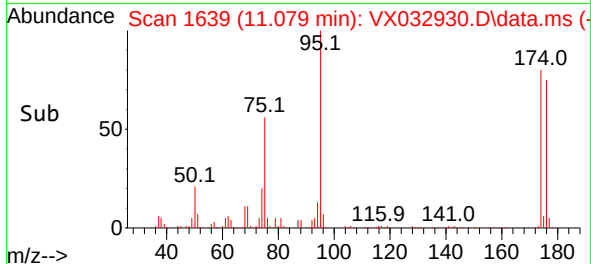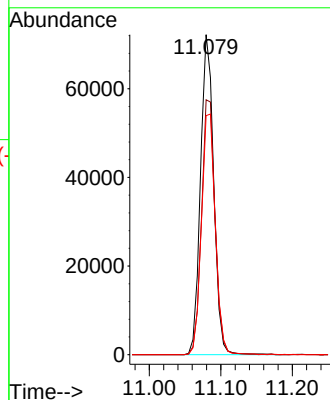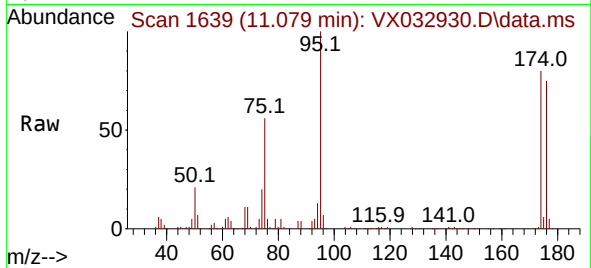

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14

Tgt Ion: 117 Resp: 178567
Ion Ratio Lower Upper
117 100
82 53.6 44.3 66.5
119 32.0 25.7 38.5


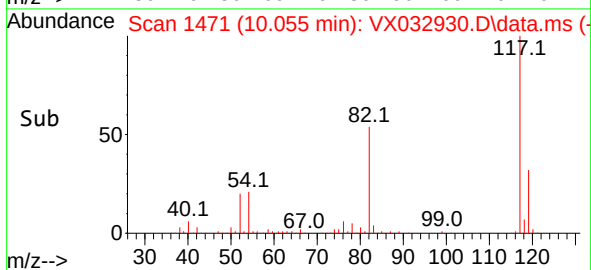
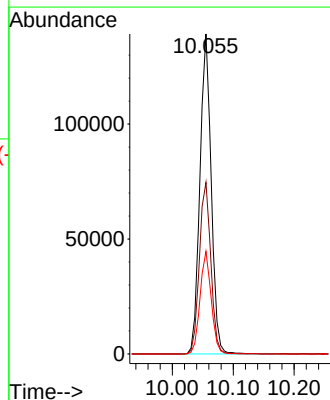
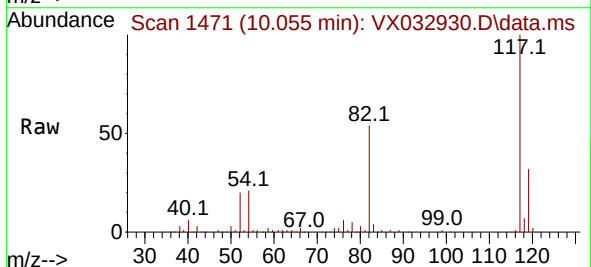


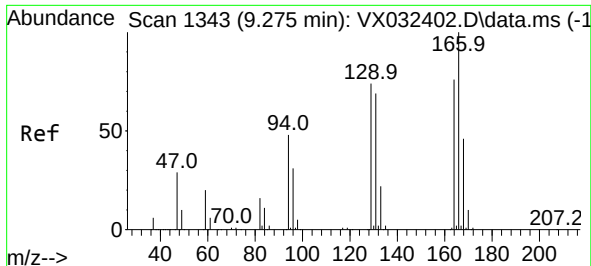

#64
Tetrachloroethene
Concen: 0.850 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20221115DL

Tgt Ion:164 Resp: 1111
Ion Ratio Lower Upper
164 100
166 108.0 105.4 158.2
129 88.0 78.2 117.2
131 69.9 72.5 108.7#

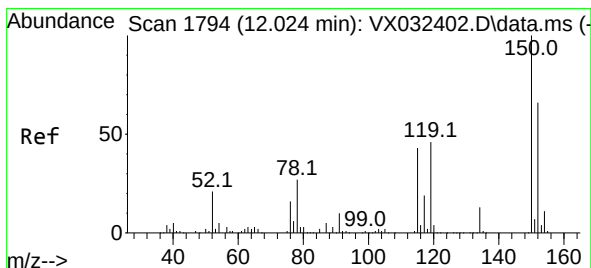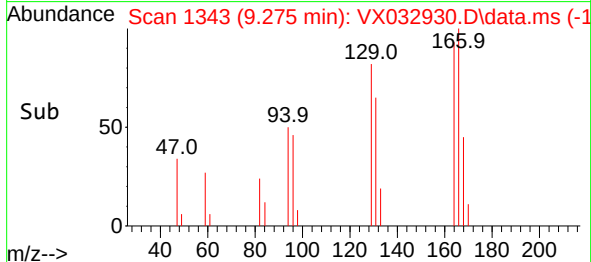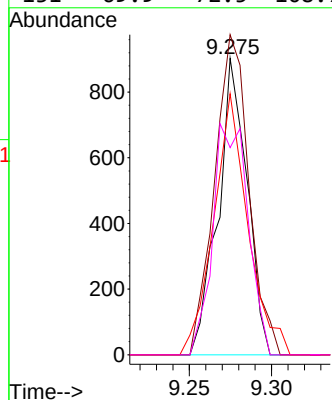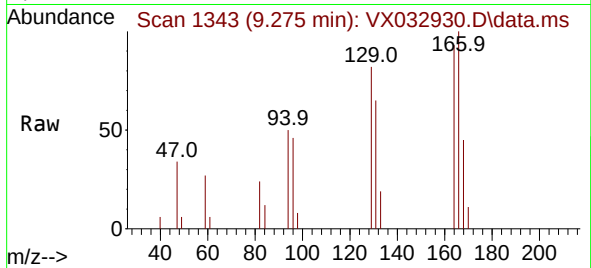

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032930.D
Acq: 18 Nov 2022 17:14

Tgt Ion:152 Resp: 82405
Ion Ratio Lower Upper
152 100
115 60.4 44.0 132.0
150 157.4 0.0 351.8

