

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
 Data File : VX032934.D
 Acq On : 18 Nov 2022 18:46
 Operator : JC/MD
 Sample : N5671-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D3-20221116

Quant Time: Nov 19 03:10:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	110108	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	184560	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	167960	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	77660	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	79901	52.225	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 104.460%	
35) Dibromofluoromethane	5.385	113	63458	48.203	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.400%	
50) Toluene-d8	8.647	98	232348	50.756	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 101.520%	
62) 4-Bromofluorobenzene	11.079	95	88423	49.449	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 98.900%	
Target Compounds						
44) Trichloroethene	7.129	130	2965	2.030	ug/l	94
52) Toluene	8.720	92	1936	0.572	ug/l	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
Data File : VX032934.D
Acq On : 18 Nov 2022 18:46
Operator : JC/MD
Sample : N5671-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20221116

Quant Time: Nov 19 03:10:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration




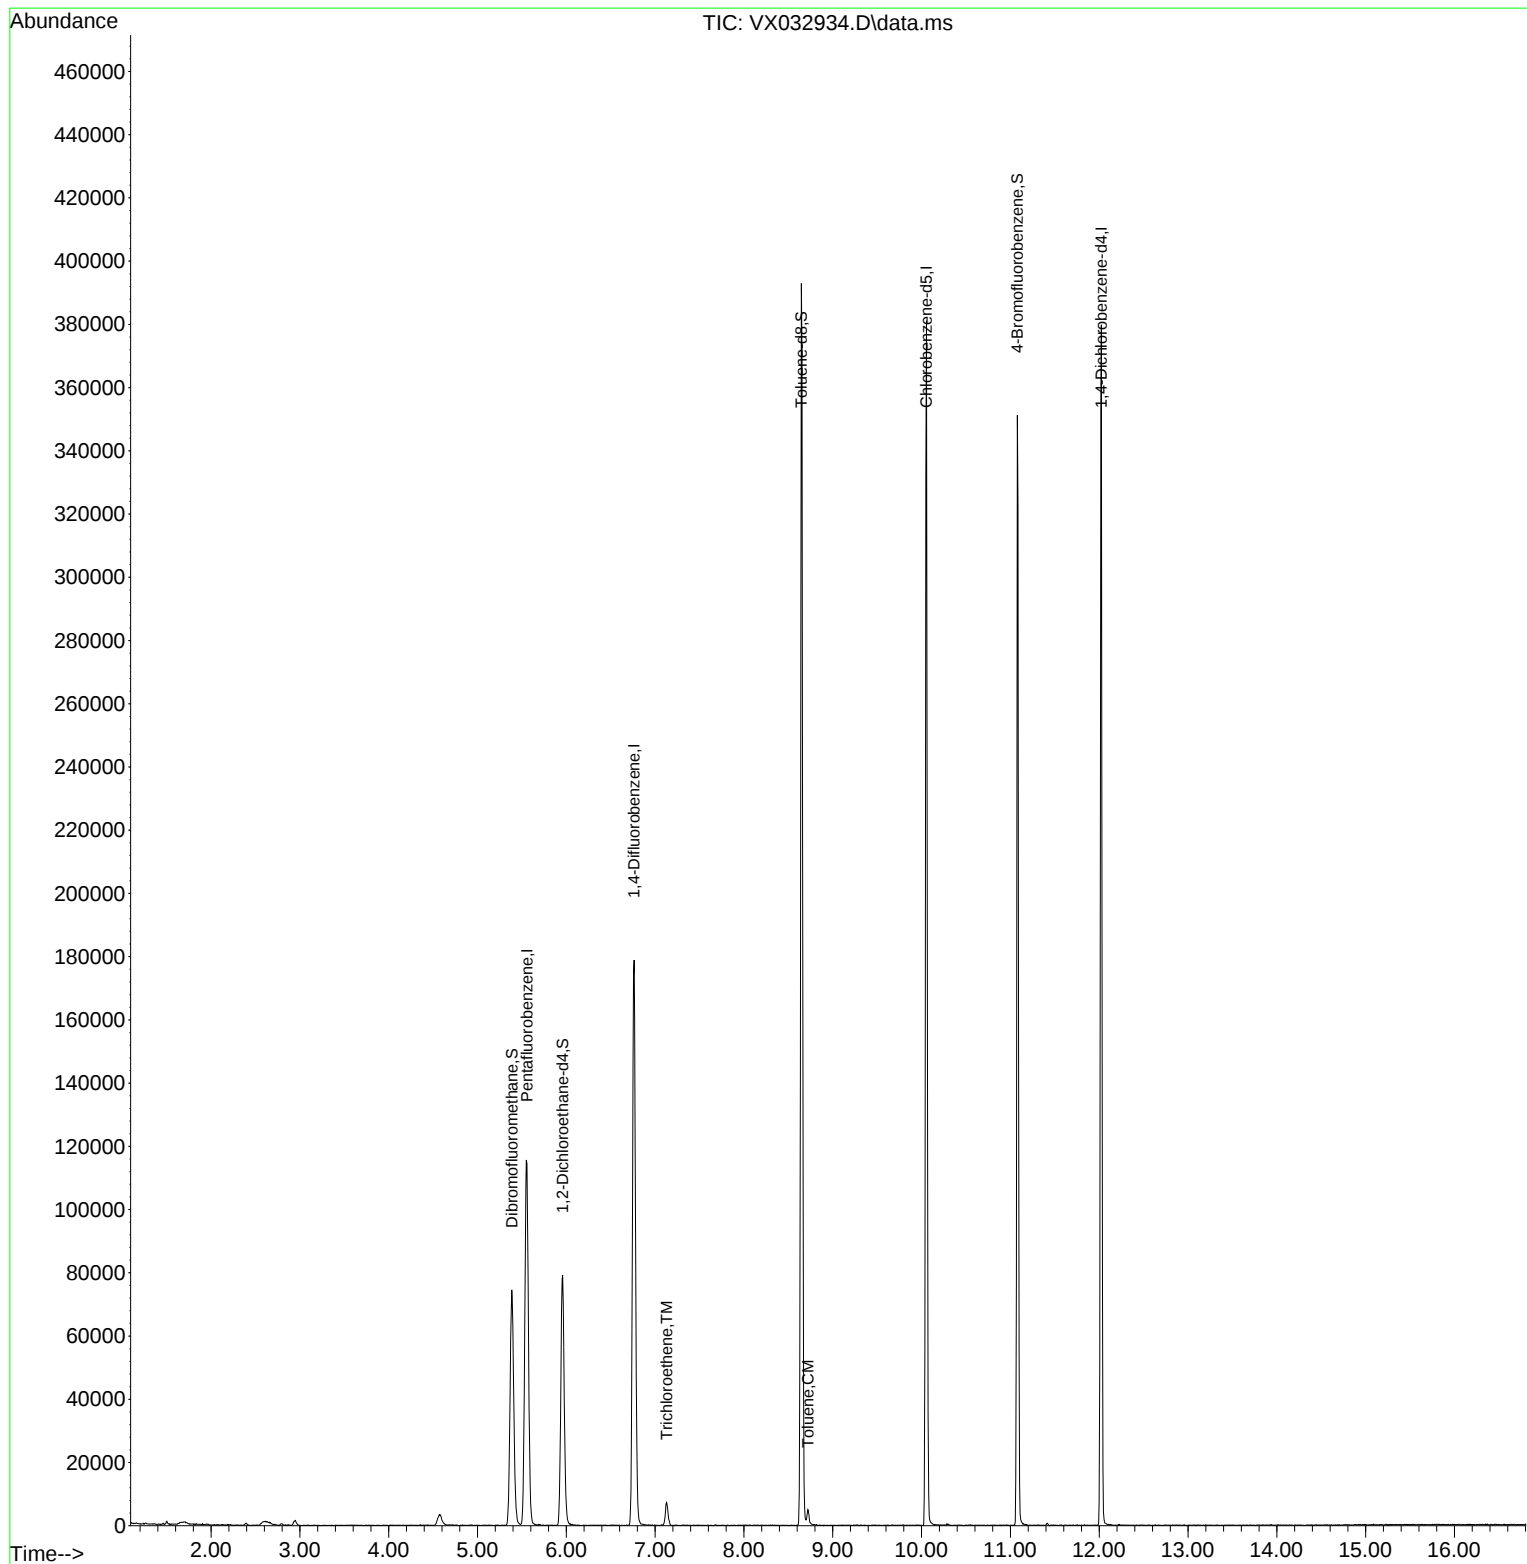




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20221116


Tgt Ion:168 Resp: 110108
Ion Ratio Lower Upper
168 100
99 55.3 46.1 69.1

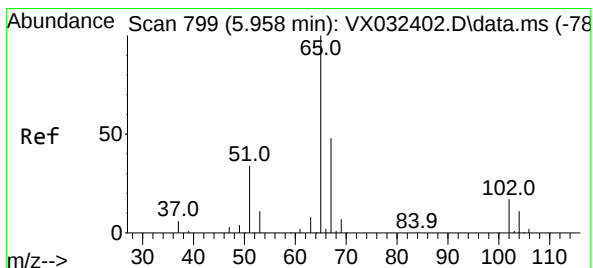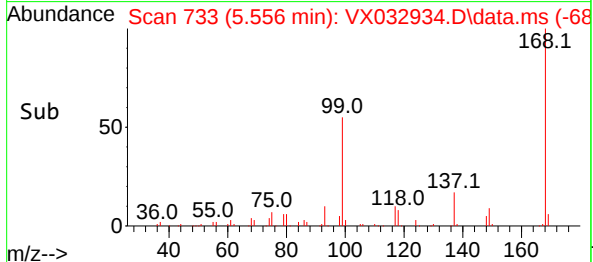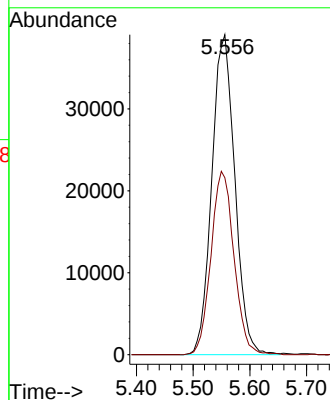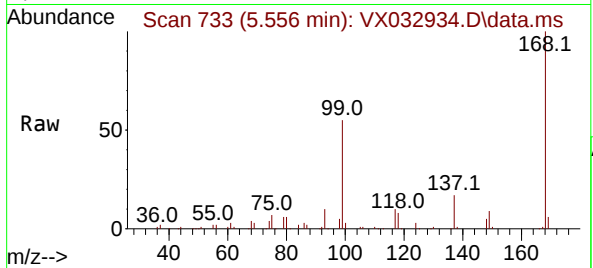

#33
1,2-Dichloroethane-d4
Concen: 52.225 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46

Tgt Ion: 65 Resp: 79901
Ion Ratio Lower Upper
65 100
67 49.2 0.0 101.8

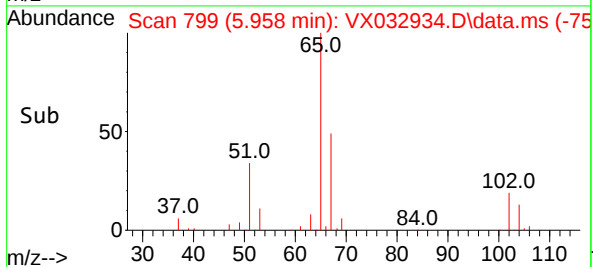
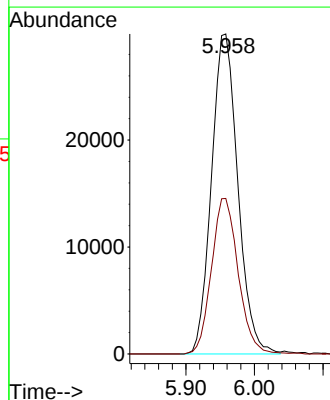
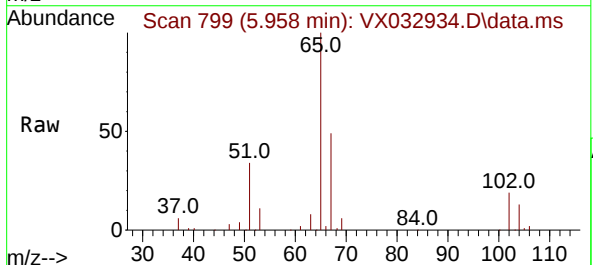


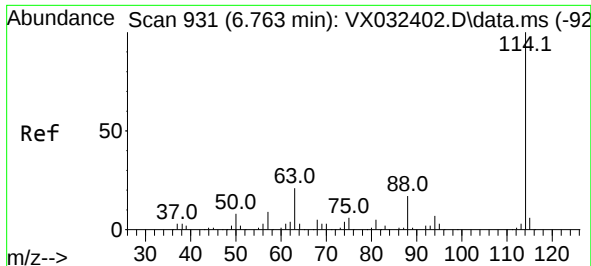

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20221116


Tgt Ion:114 Resp: 184560
Ion Ratio Lower Upper
114 100
63 18.5 0.0 41.6
88 15.3 0.0 33.4

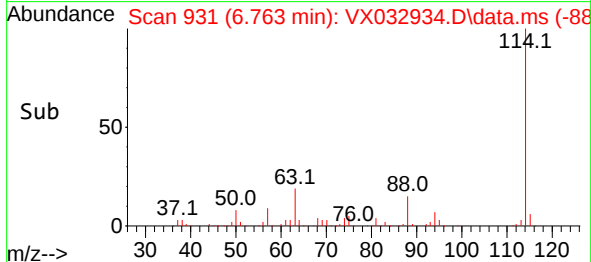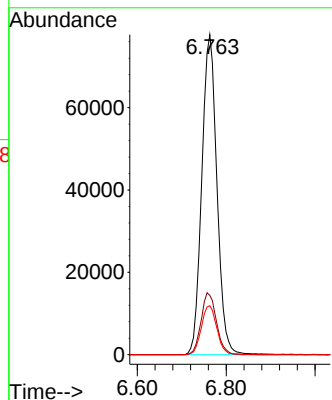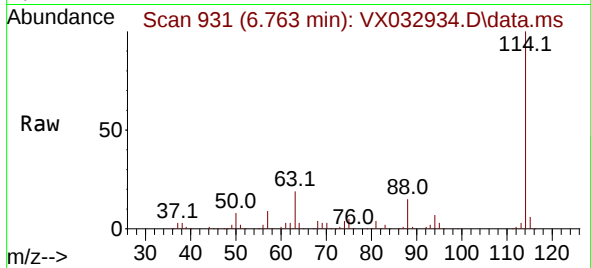

#35
Dibromofluoromethane
Concen: 48.203 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46


Tgt Ion:113 Resp: 63458
Ion Ratio Lower Upper
113 100
111 103.3 82.4 123.6
192 19.2 15.4 23.2

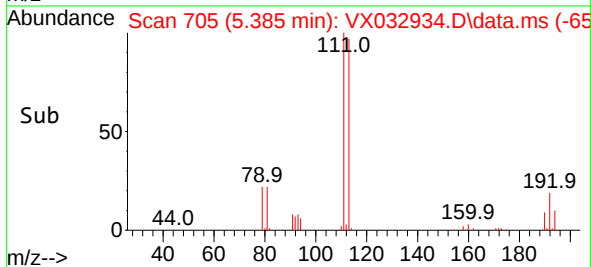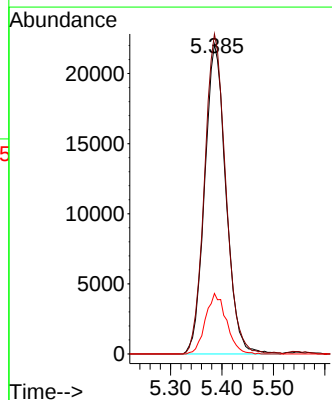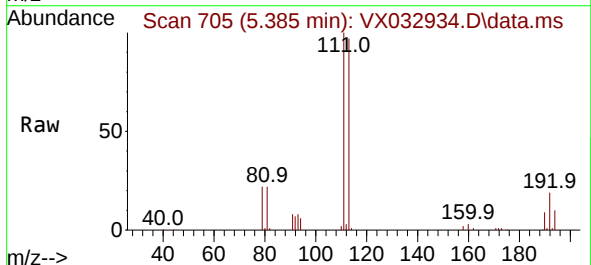



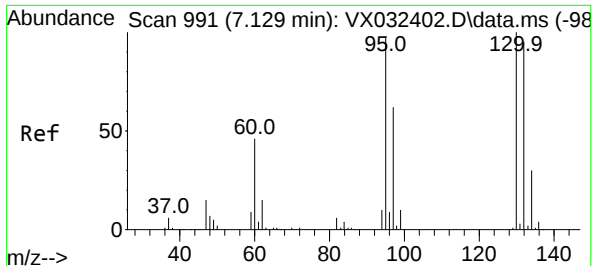


#44
 Trichloroethene
 Concen: 2.030 ug/l
 RT: 7.129 min Scan# 991
 Delta R.T. -0.000 min
 Lab File: VX032934.D
 Acq: 18 Nov 2022 18:46

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D3-20221116



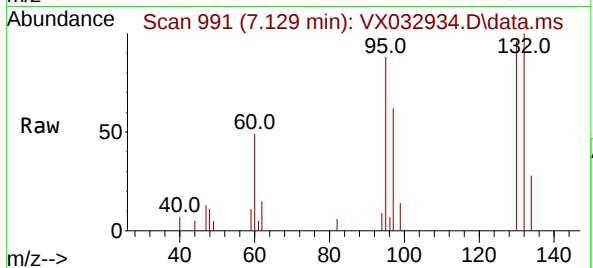



Tgt Ion:130 Resp: 2965
 Ion Ratio Lower Upper
 130 100
 95 91.8 0.0 195.2

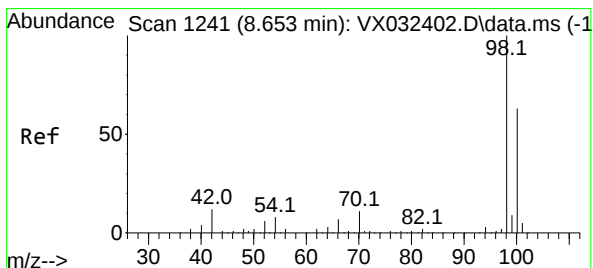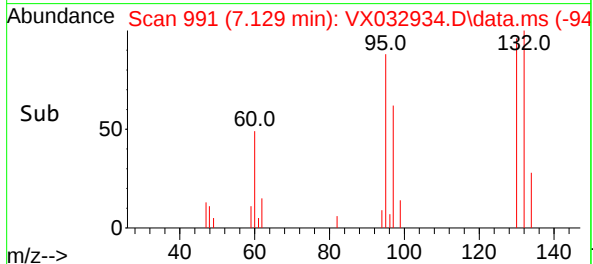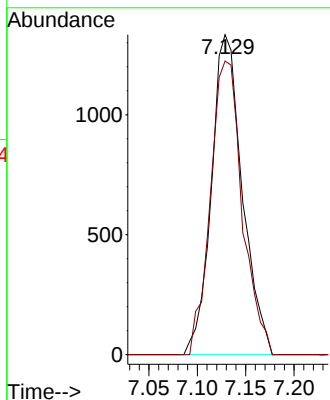

#50
 Toluene-d8
 Concen: 50.756 ug/l
 RT: 8.647 min Scan# 1240
 Delta R.T. -0.006 min
 Lab File: VX032934.D
 Acq: 18 Nov 2022 18:46

Tgt Ion: 98 Resp: 232348
 Ion Ratio Lower Upper
 98 100
 100 62.8 50.9 76.3


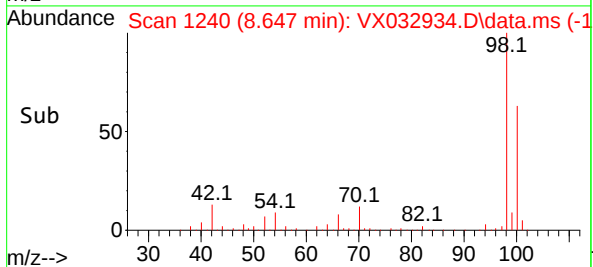
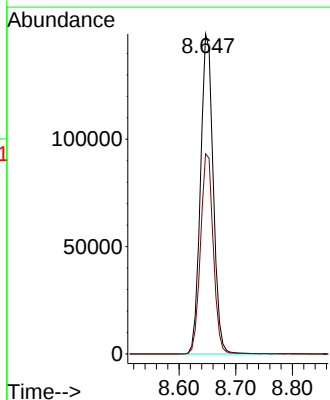
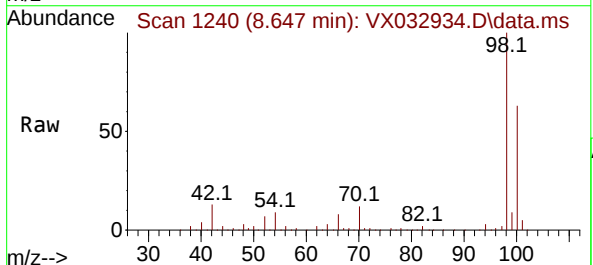


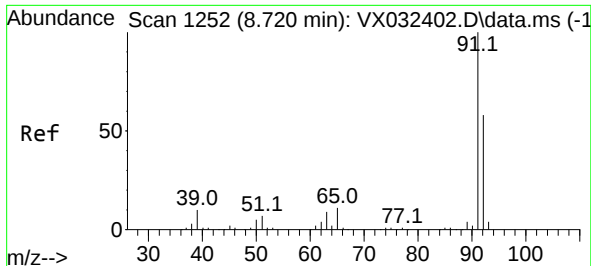

#52
Toluene
Concen: 0.572 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46




Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20221116


Tgt Ion: 92 Resp: 1936
Ion Ratio Lower Upper
92 100
91 176.7 138.3 207.5

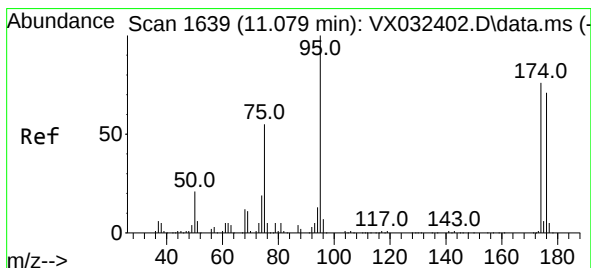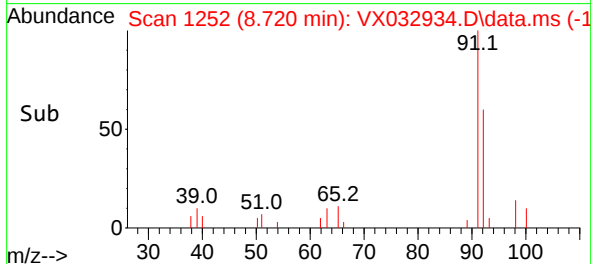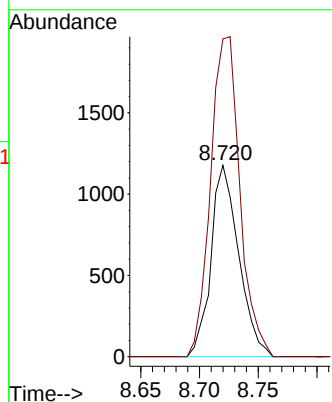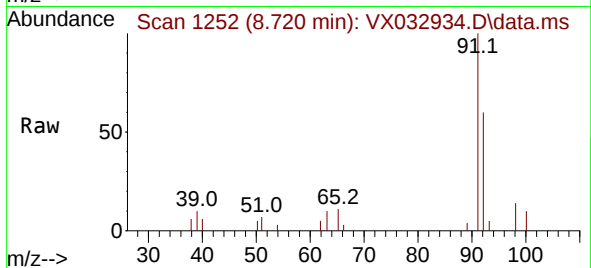

#62
4-Bromofluorobenzene
Concen: 49.449 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46

Tgt Ion: 95 Resp: 88423
Ion Ratio Lower Upper
95 100
174 81.5 0.0 164.0
176 79.9 0.0 154.4


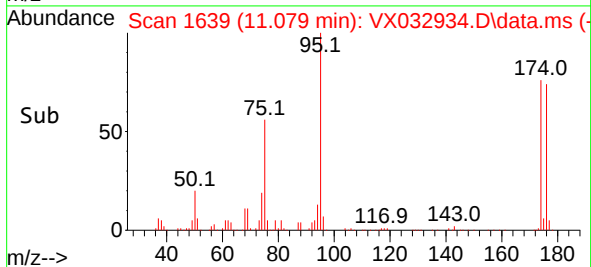
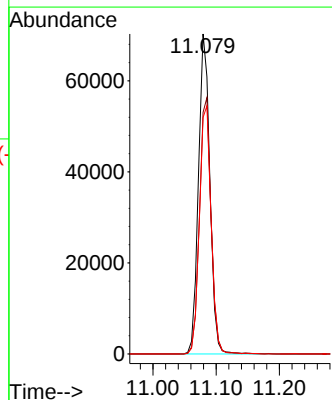
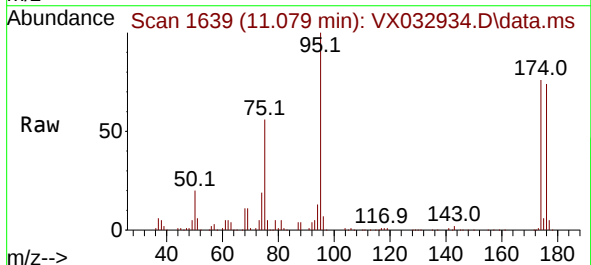


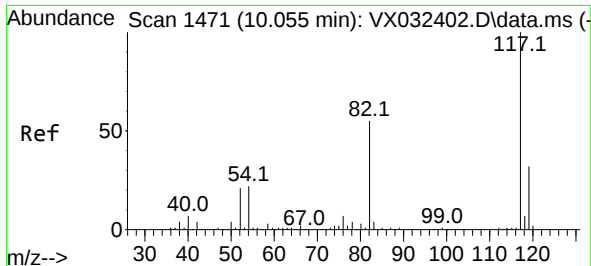

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46

Instrument :
MSVOA_X
ClientSampleId :
RE122D3-20221116

Tgt Ion:117 Resp: 167960
Ion Ratio Lower Upper
117 100
82 54.9 44.3 66.5
119 31.5 25.7 38.5

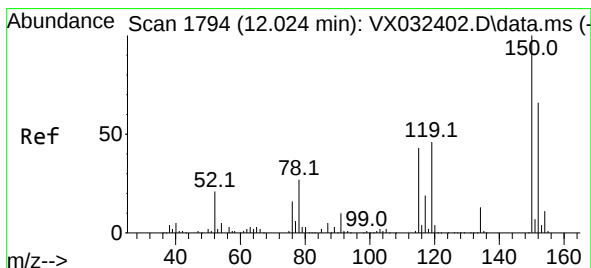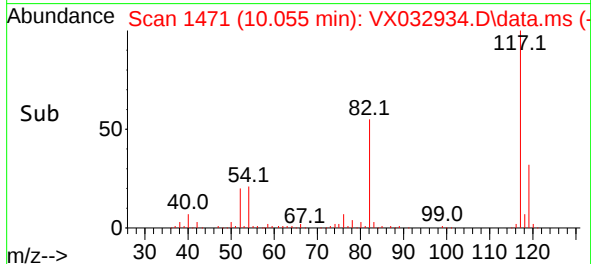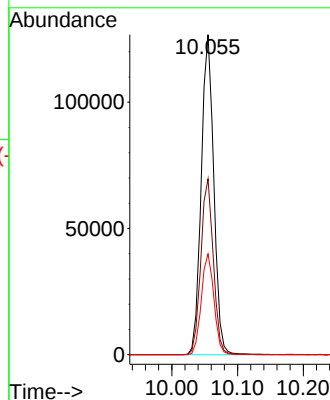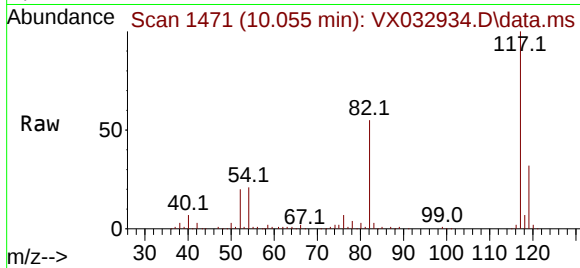

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX032934.D
Acq: 18 Nov 2022 18:46

Tgt Ion:152 Resp: 77660
Ion Ratio Lower Upper
152 100
115 59.5 44.0 132.0
150 157.2 0.0 351.8

