

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
 Data File : VX032935.D
 Acq On : 18 Nov 2022 19:10
 Operator : JC/MD
 Sample : N5672-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D2-20221116

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032935.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	197	204	212	rBV2	76200	145326	3.21%	1.811%
2	5.385	694	705	722	rBV	75924	220681	4.87%	2.750%
3	5.550	722	732	747	rVV2	119657	336296	7.42%	4.190%
4	5.958	787	799	817	rBV	81129	214755	4.74%	2.676%
5	6.763	922	931	945	rBV	186764	440590	9.72%	5.490%
6	7.129	980	991	1013	rBV	2098922	4530535	100.00%	56.450%
7	8.647	1234	1240	1248	rBV	404908	628599	13.87%	7.832%
8	9.275	1338	1343	1352	rVB	39956	57751	1.27%	0.720%
9	10.055	1465	1471	1489	rBV	383112	522555	11.53%	6.511%
10	11.079	1634	1639	1651	rBV	358201	453254	10.00%	5.647%
11	12.024	1788	1794	1806	rBV	375349	475449	10.49%	5.924%




Sum of corrected areas: 8025791

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
Data File : VX032935.D
Acq On : 18 Nov 2022 19:10
Operator : JC/MD
Sample : N5672-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20221116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

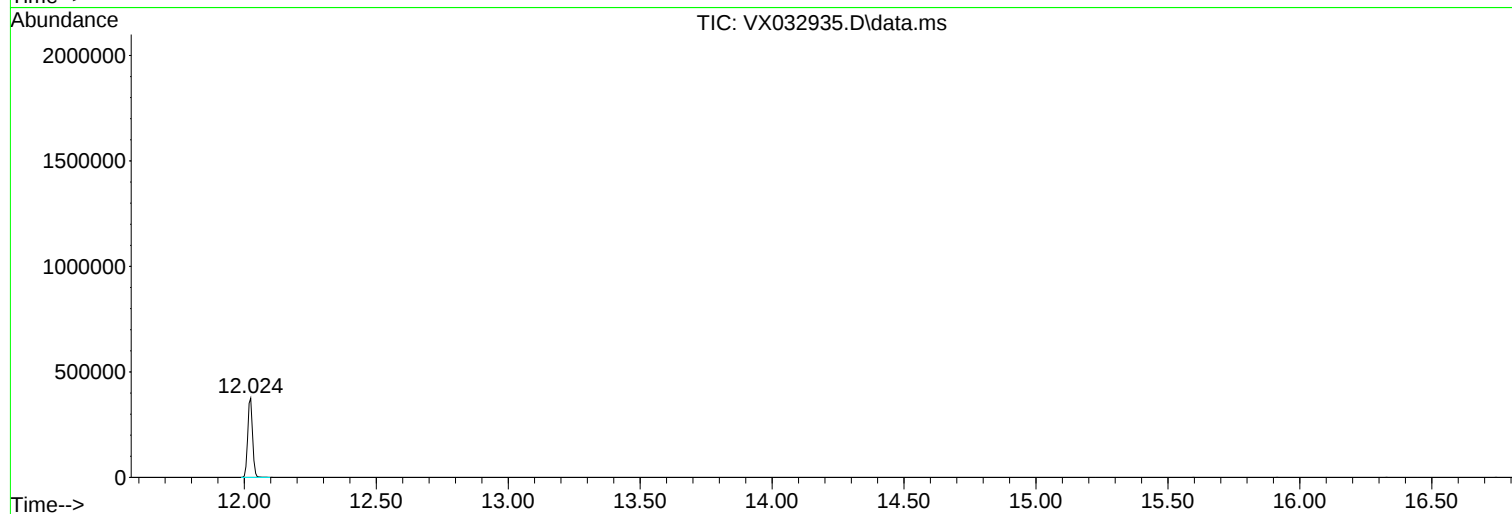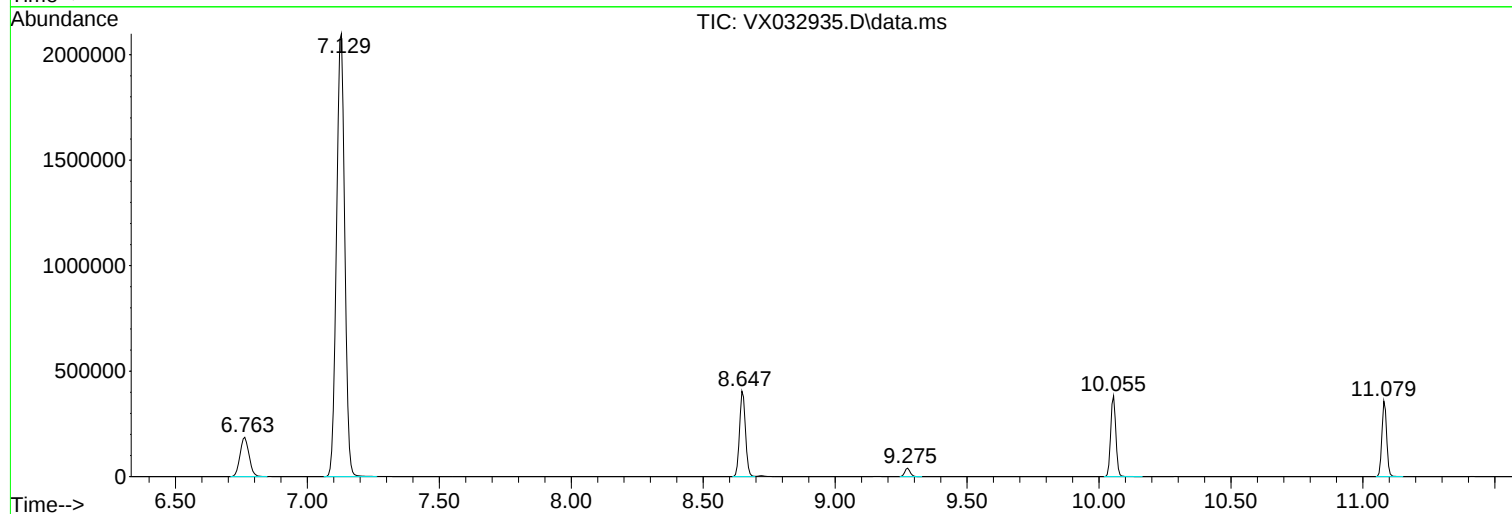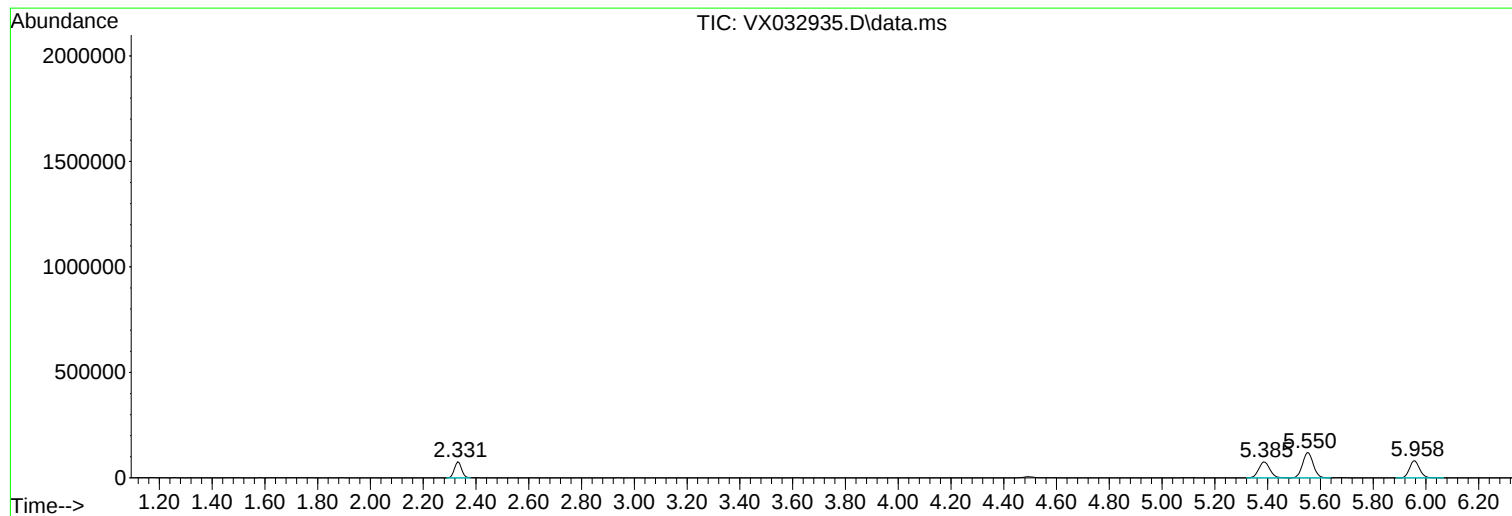

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
Data File : VX032935.D
Acq On : 18 Nov 2022 19:10
Operator : JC/MD
Sample : N5672-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20221116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111822\
Data File : VX032935.D
Acq On : 18 Nov 2022 19:10
Operator : JC/MD
Sample : N5672-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20221116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------