


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX111918\
 Data File : VX006078.D
 Acq On : 19 Nov 2018 09:04
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
 Title : SW846 8260
 Last Update : Wed Nov 07 14:40:53 2018

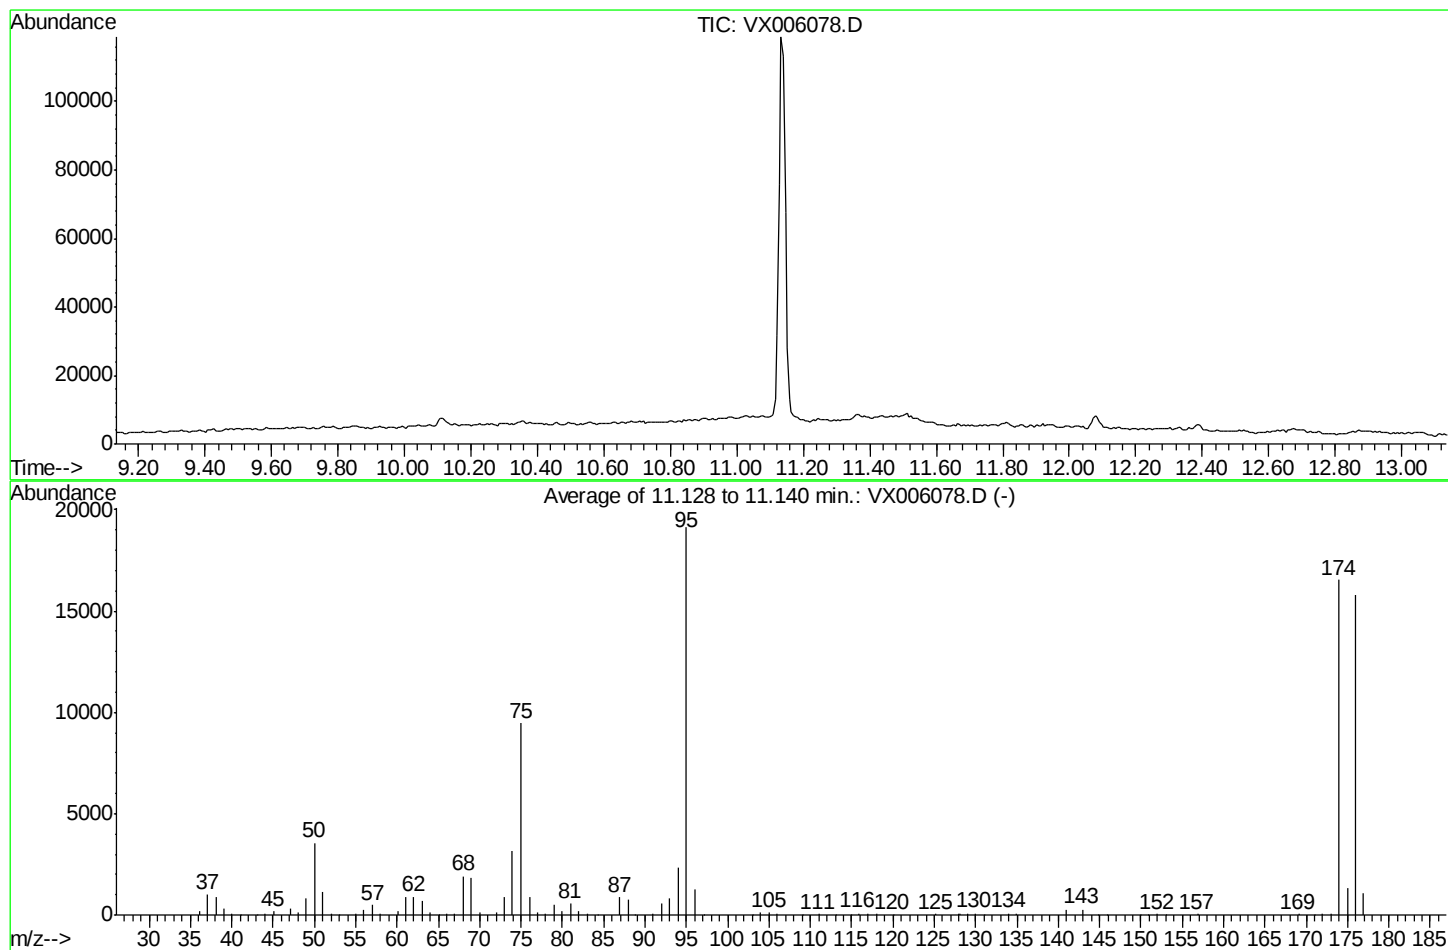

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	3556	PASS
75	95	30	60	49.5	9462	PASS
95	95	100	100	100.0	19132	PASS
96	95	5	9	6.6	1264	PASS
173	174	0.00	2	0.6	92	PASS
174	95	50	100	86.4	16537	PASS
175	174	5	9	8.0	1315	PASS
176	174	95	101	95.6	15816	PASS
177	176	5	9	6.9	1090	PASS