

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX111919\
 Data File : VX013455.D
 Acq On : 19 Nov 2019 10:35
 Operator : JC/SP
 Sample : VX1119WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1119WBL01

Quant Time: Nov 19 16:20:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 02 07:06:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	736276	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	1194203	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	1044867	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	464571	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	434145	49.77	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.54%	
35) Dibromofluoromethane	5.48	113	358016	47.80	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.60%	
50) Toluene-d8	8.71	98	1413295	50.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.10%	
62) 4-Bromofluorobenzene	11.13	95	473151	46.43	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.86%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX111919\
Data File : VX013455.D
Acq On : 19 Nov 2019 10:35
Operator : JC/SP
Sample : VX1119WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1119WBL01

Quant Time: Nov 19 16:20:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 02 07:06:38 2019
Response via : Initial Calibration

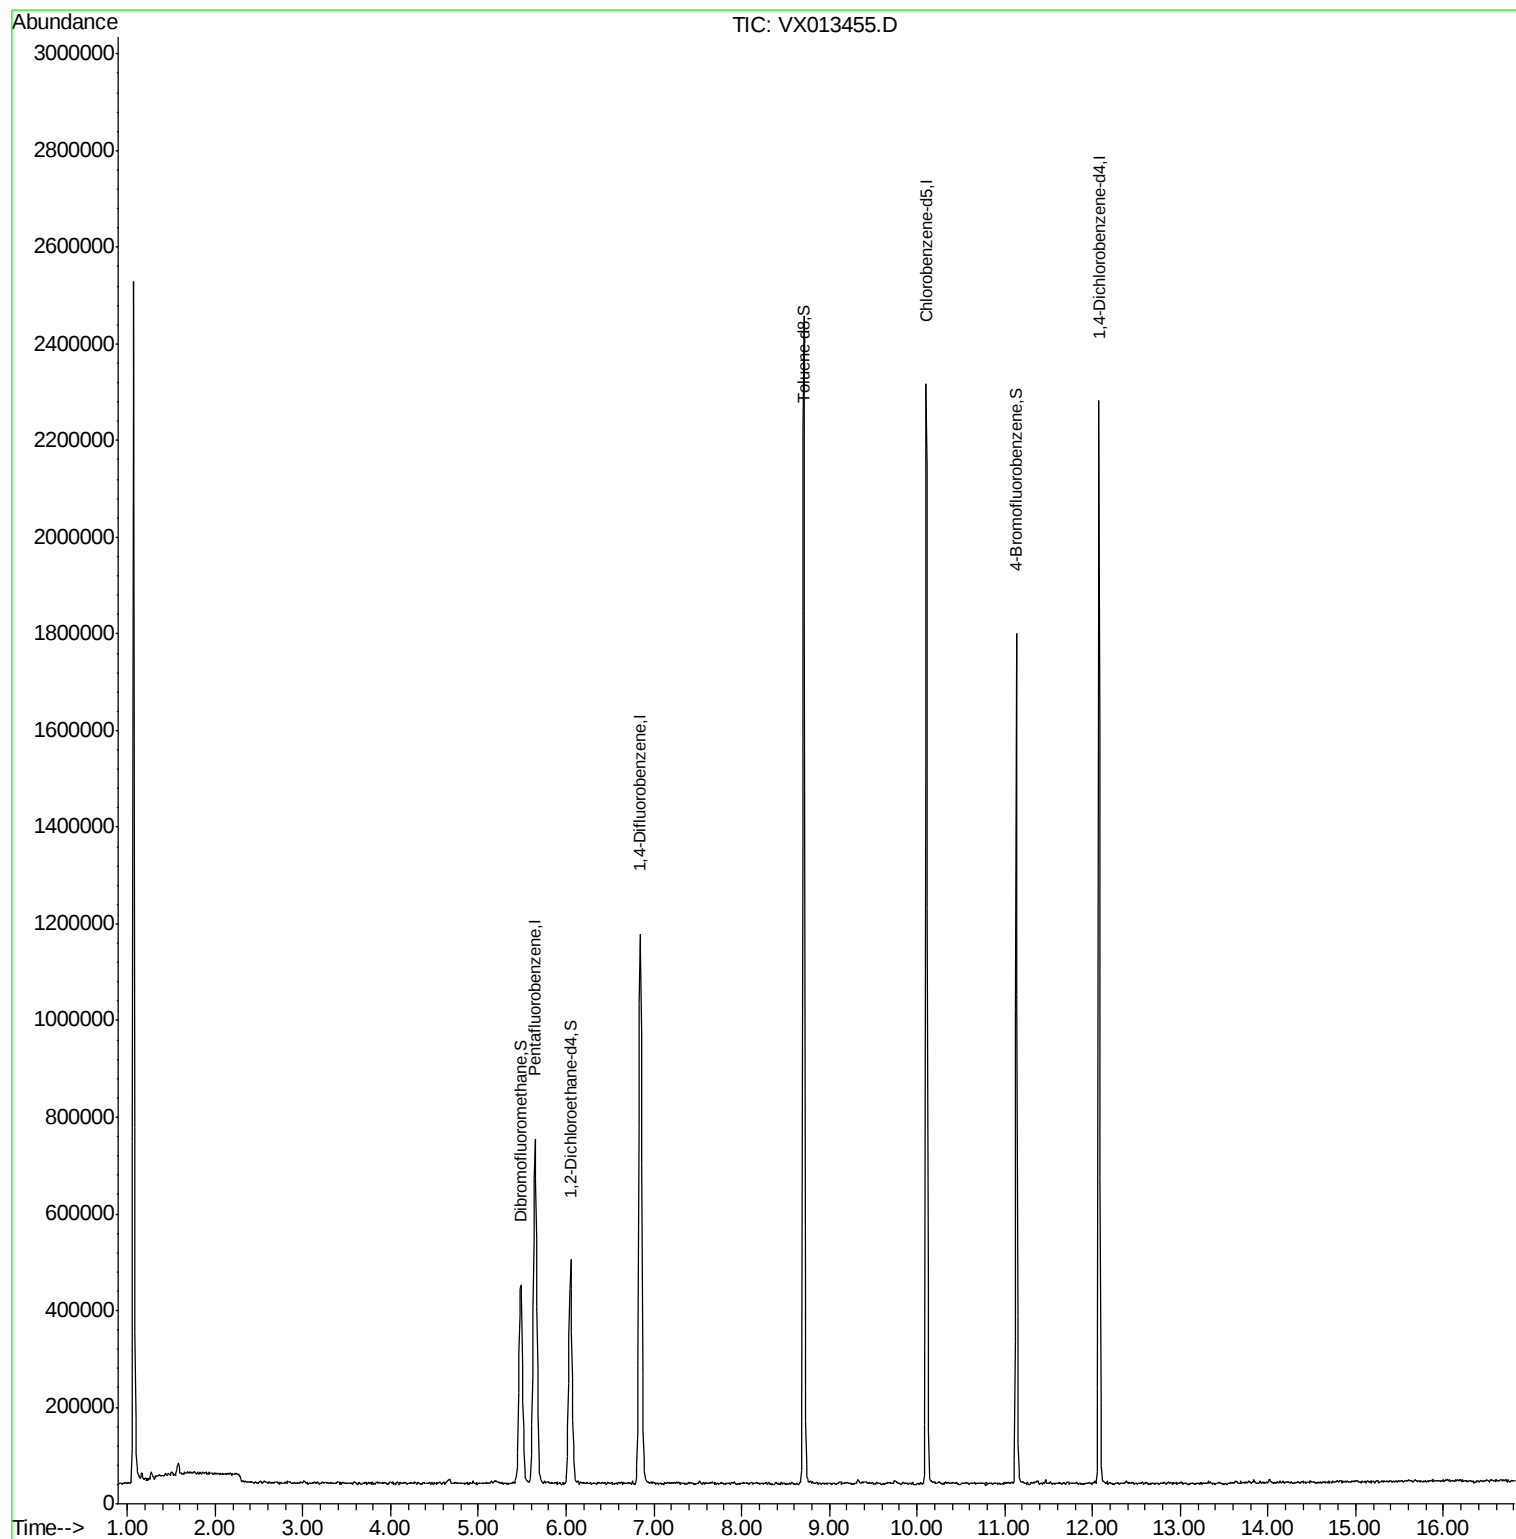

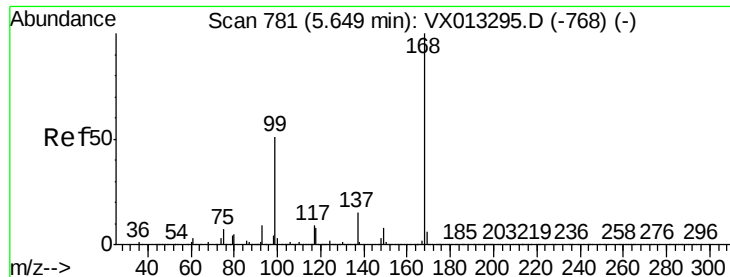

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.00 min

Lab File: VX013455.D

Acq: 19 Nov 2019 10:35

Instrument :

MSVOA_X

ClientSampleId :


VX1119WBL01

Tot Ion:168 Resp: 736276

Ion Ratio Lower Upper

168 100

99 48.9 40.8 61.2

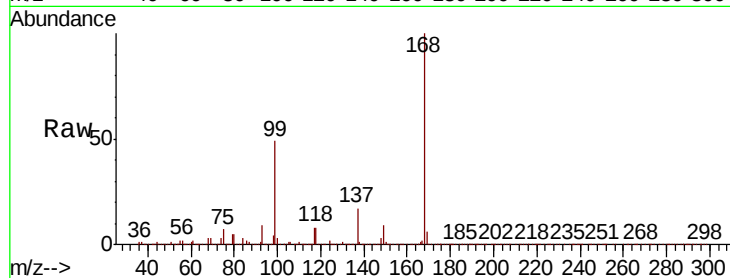

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

250000

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

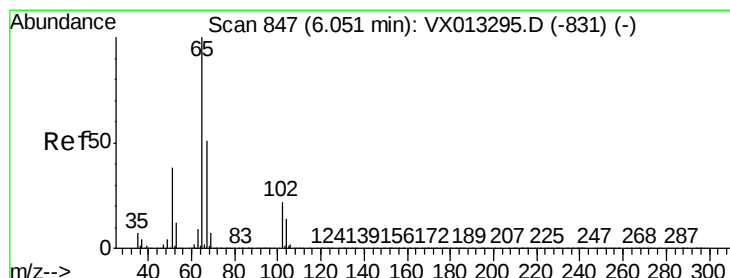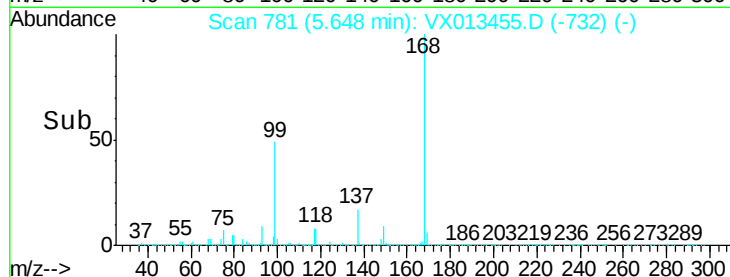

#33

1,2-Dichloroethane-d4

Concen: 49.772 ug/l

RT: 6.05 min Scan# 847

Delta R.T. -0.00 min

Lab File: VX013455.D


Acq: 19 Nov 2019 10:35

Tgt Ion: 65 Resp: 434145

Ion Ratio Lower Upper

65 100

67 51.8 0.0 104.2

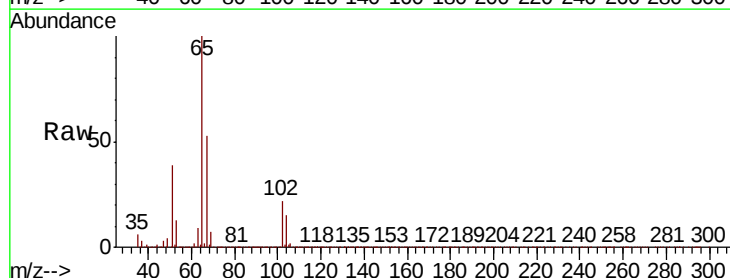

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.05

150000


100000


50000

0

Time-->

5.90 6.00 6.10 6.20

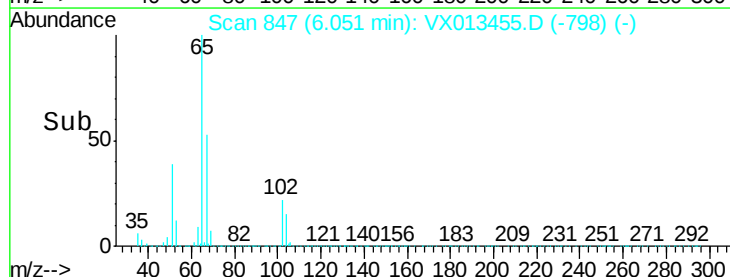

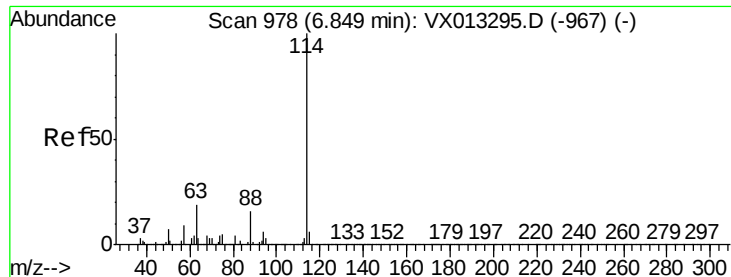

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 977

Delta R.T. -0.01 min

Lab File: VX013455.D

Acq: 19 Nov 2019 10:35

Instrument :

MSVOA_X

ClientSampleId :

VX1119WBL01


Tot Ion:114 Resp: 1194203

Ion Ratio Lower Upper

114 100

63 20.3 0.0 38.4




88 15.9 0.0 32.2

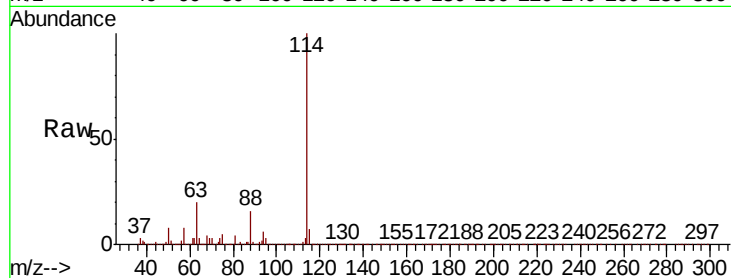

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

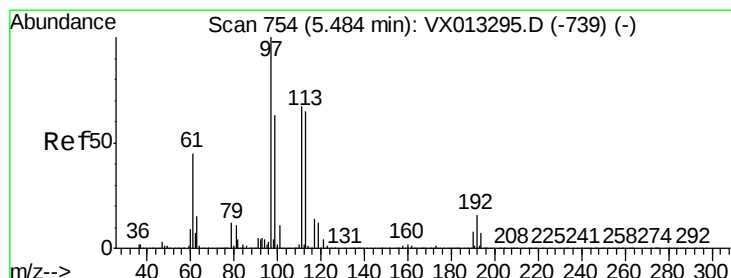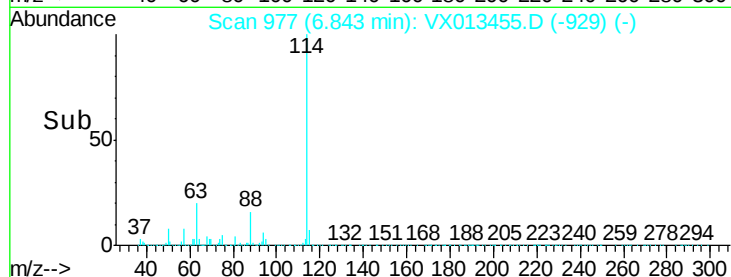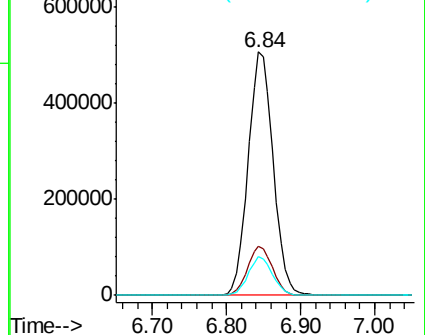

#35

Dibromofluoromethane

Concen: 47.798 ug/l

RT: 5.48 min Scan# 754

Delta R.T. -0.00 min

Lab File: VX013455.D

Acq: 19 Nov 2019 10:35


Tgt Ion:113 Resp: 358016

Ion Ratio Lower Upper

113 100

111 104.5 81.9 122.9



192 23.2 19.1 28.7

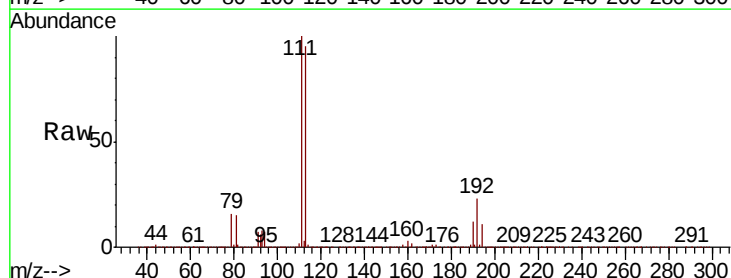


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



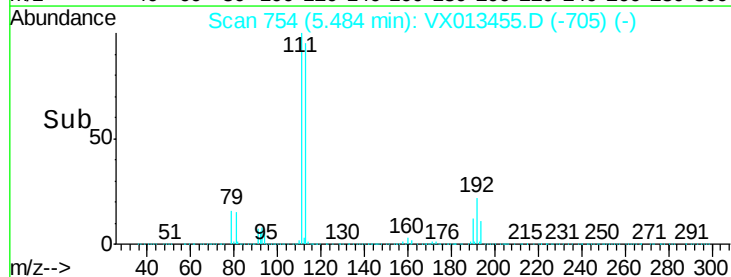
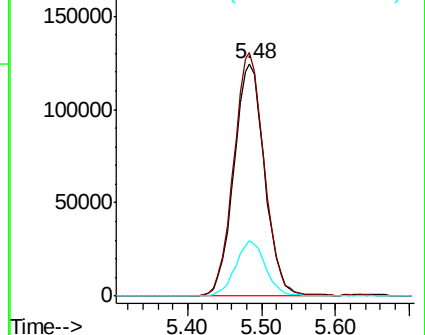


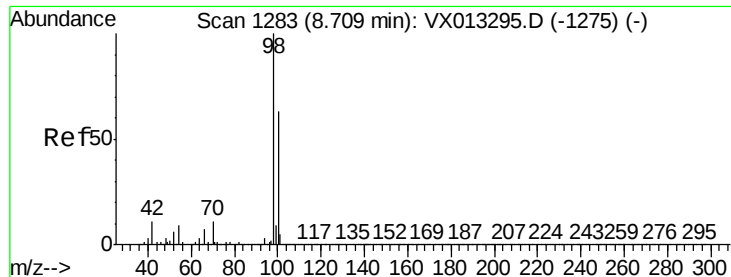

#50
Toluene-d8
Concen: 50.051 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. -0.00 min
Lab File: VX013455.D
Acq: 19 Nov 2019 10:35




Instrument :
MSVOA_X
ClientSampleId :
VX1119WBL01


Tot Ion: 98 Resp: 1413295
Ion Ratio Lower Upper
98 100
100 65.6 52.2 78.2

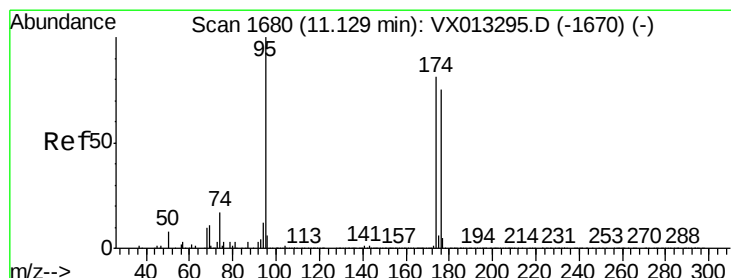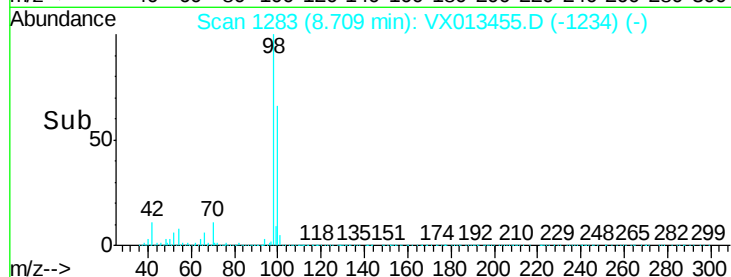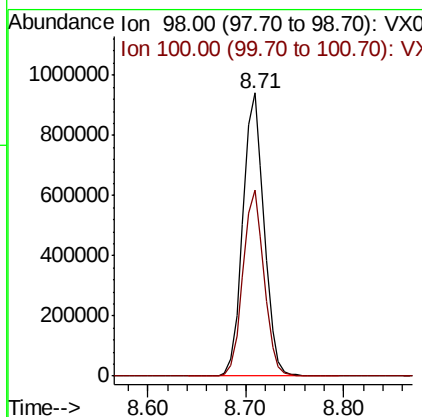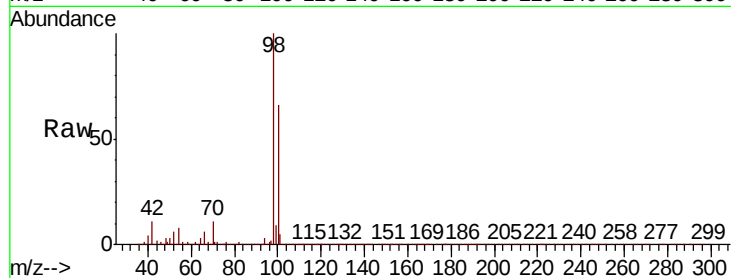

#62
4-Bromofluorobenzene
Concen: 46.428 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. -0.00 min
Lab File: VX013455.D
Acq: 19 Nov 2019 10:35

Tgt Ion: 95 Resp: 473151
Ion Ratio Lower Upper
95 100
174 88.7 0.0 179.8
176 84.3 0.0 173.0


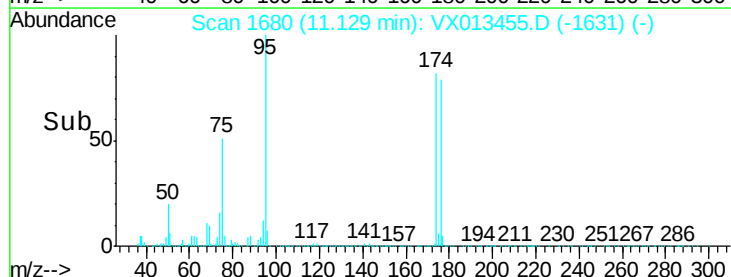
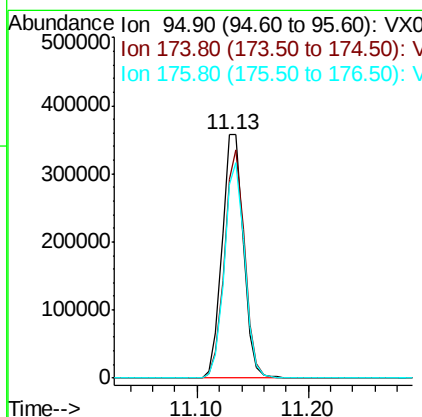
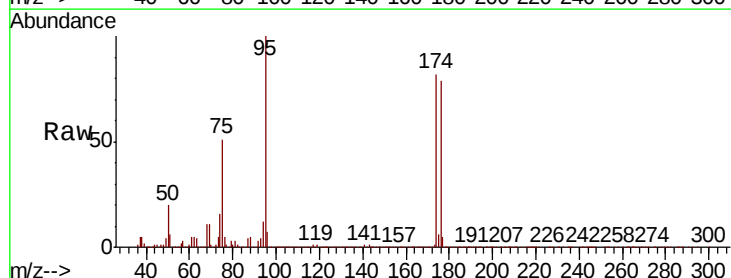


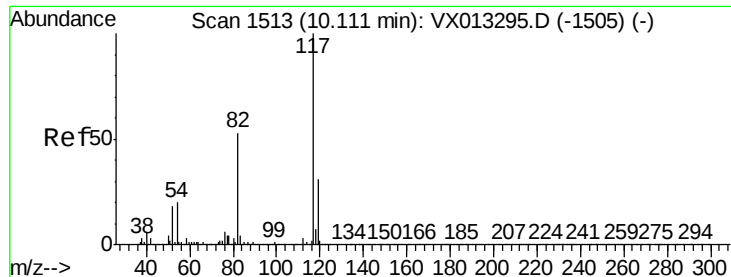

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX013455.D
Acq: 19 Nov 2019 10:35

Instrument :
MSVOA_X
ClientSampleId :
VX1119WBL01

Tot Ion:117 Resp: 1044867
Ion Ratio Lower Upper
117 100
82 56.2 42.6 64.0
119 31.8 24.8 37.2

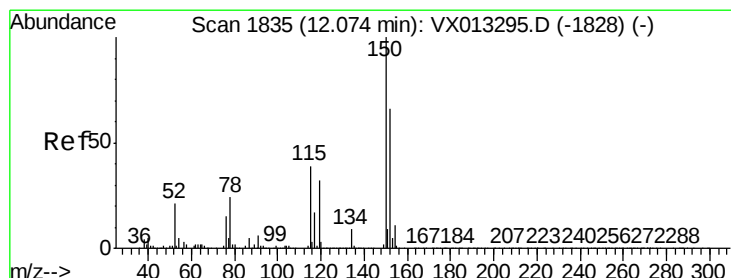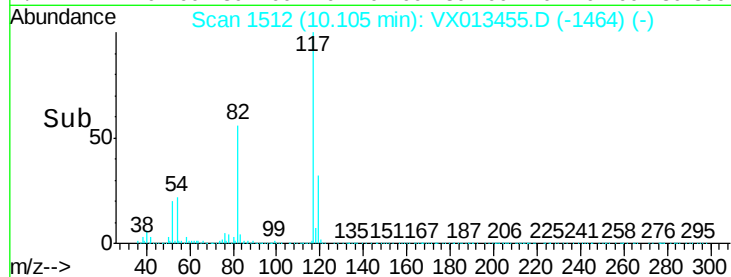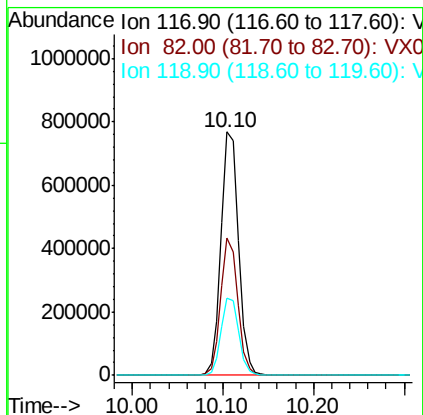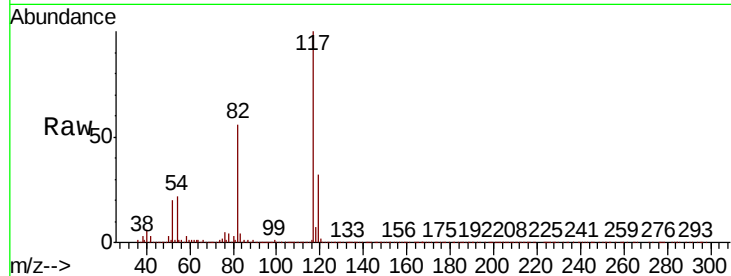

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. -0.00 min
Lab File: VX013455.D
Acq: 19 Nov 2019 10:35

Tgt Ion:152 Resp: 464571
Ion Ratio Lower Upper
152 100
115 55.2 39.5 118.3
150 158.0 0.0 344.4

