
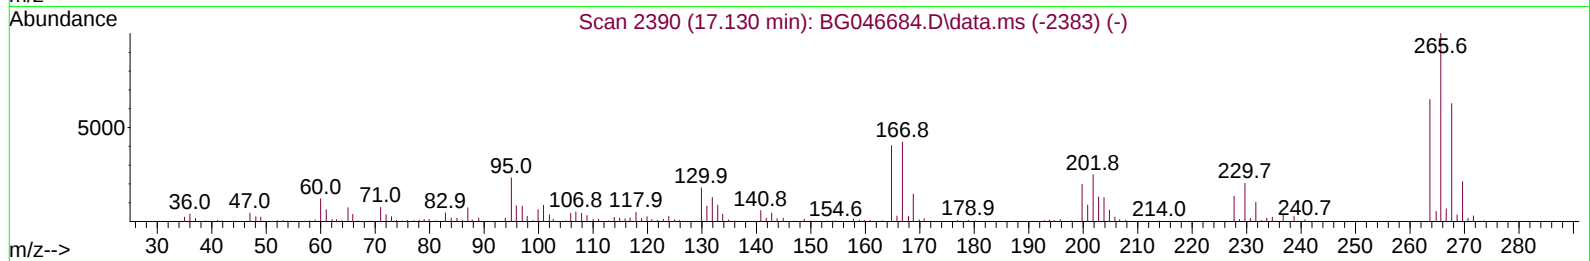
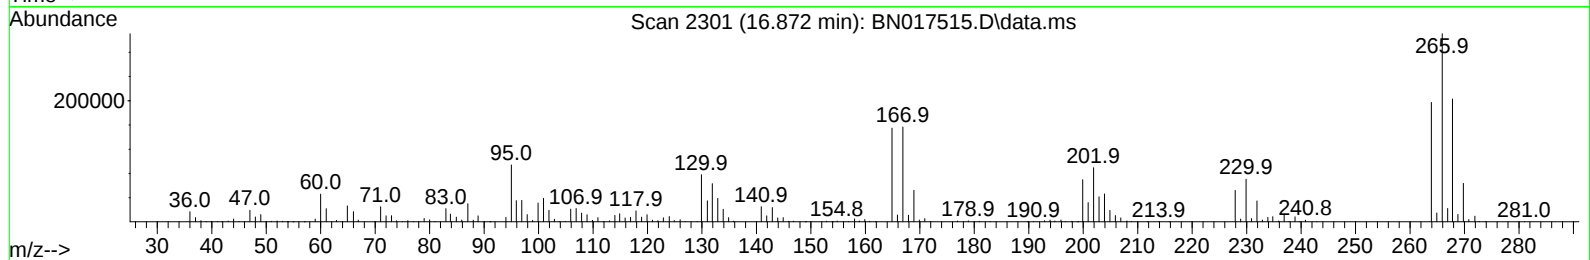


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111921\
Data File : BN017515.D
Acq On : 19 Nov 2021 09:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 11:43:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:42:56 2021
Response via : Initial Calibration

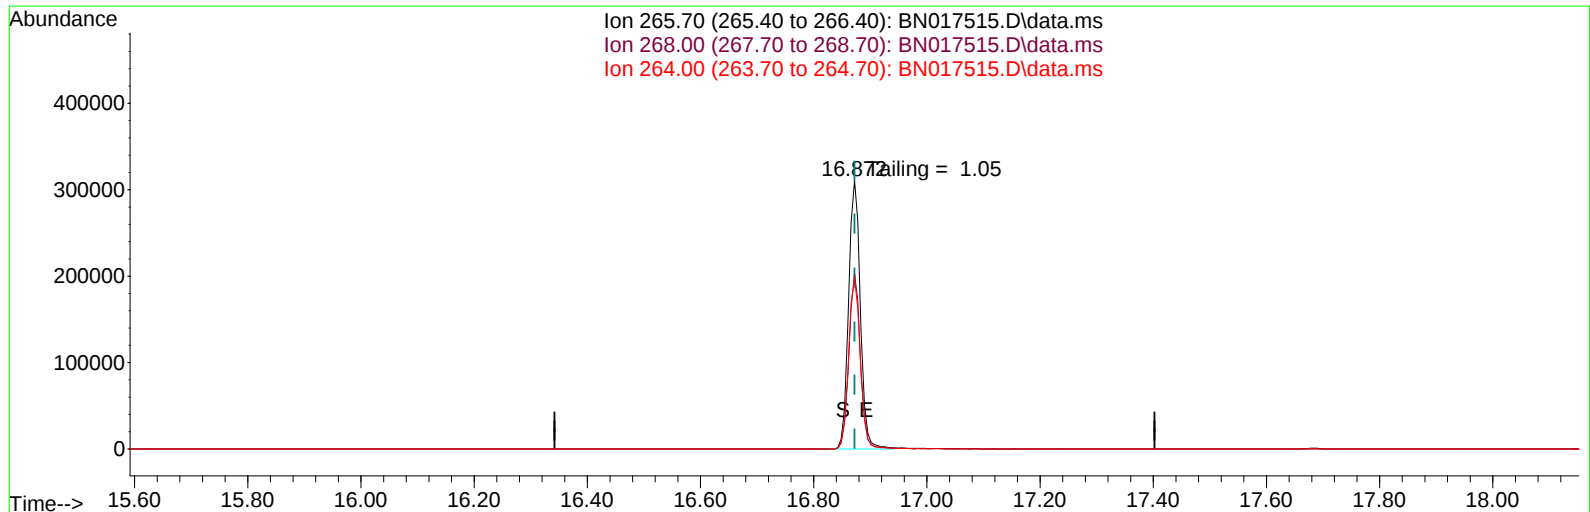

TIC: BN017515.D\data.ms

(70) Pentachlorophenol (C)

16.872min (0.000) 18448.12 ng

response 449530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.31
264.00	61.60	63.56
0.00	0.00	0.00