

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025216.D
 Acq On : 18 Nov 2021 18:00
 Operator : JC/MD
 Sample : M4677-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB9

Quant Time: Nov 19 05:29:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 19 05:25:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	183556	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	163812	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	77819	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	47433	38.250	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.500%
7) Chloroethane-d5	1.660	69	40586	57.426	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	114.860%
11) 1,1-Dichloroethene-d2	2.307	63	59863	28.068	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.140%#
21) 2-Butanone-d5	4.459	46	79609	84.952	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.950%
24) Chloroform-d	5.062	84	86628	39.709	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.420%
26) 1,2-Dichloroethane-d4	5.958	65	54801	41.443	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.880%
32) Benzene-d6	5.977	84	181966	40.700	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.400%
36) 1,2-Dichloropropane-d6	7.312	67	56122	41.110	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	82.220%
41) Toluene-d8	8.653	98	167390	39.205	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.400%#
43) trans-1,3-Dichloroprop...	8.952	79	27714	37.397	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.800%
47) 2-Hexanone-d5	9.385	63	59441	81.085	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.080%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	79064	40.211	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	80.420%
66) 1,2-Dichlorobenzene-d4	12.323	152	63988	41.480	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.960%
Target Compounds					Qvalue	
13) Acetone	2.380	43	6606	7.515	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025216.D
Acq On : 18 Nov 2021 18:00
Operator : JC/MD
Sample : M4677-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB9

Quant Time: Nov 19 05:29:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 19 05:25:45 2021
Response via : Initial Calibration

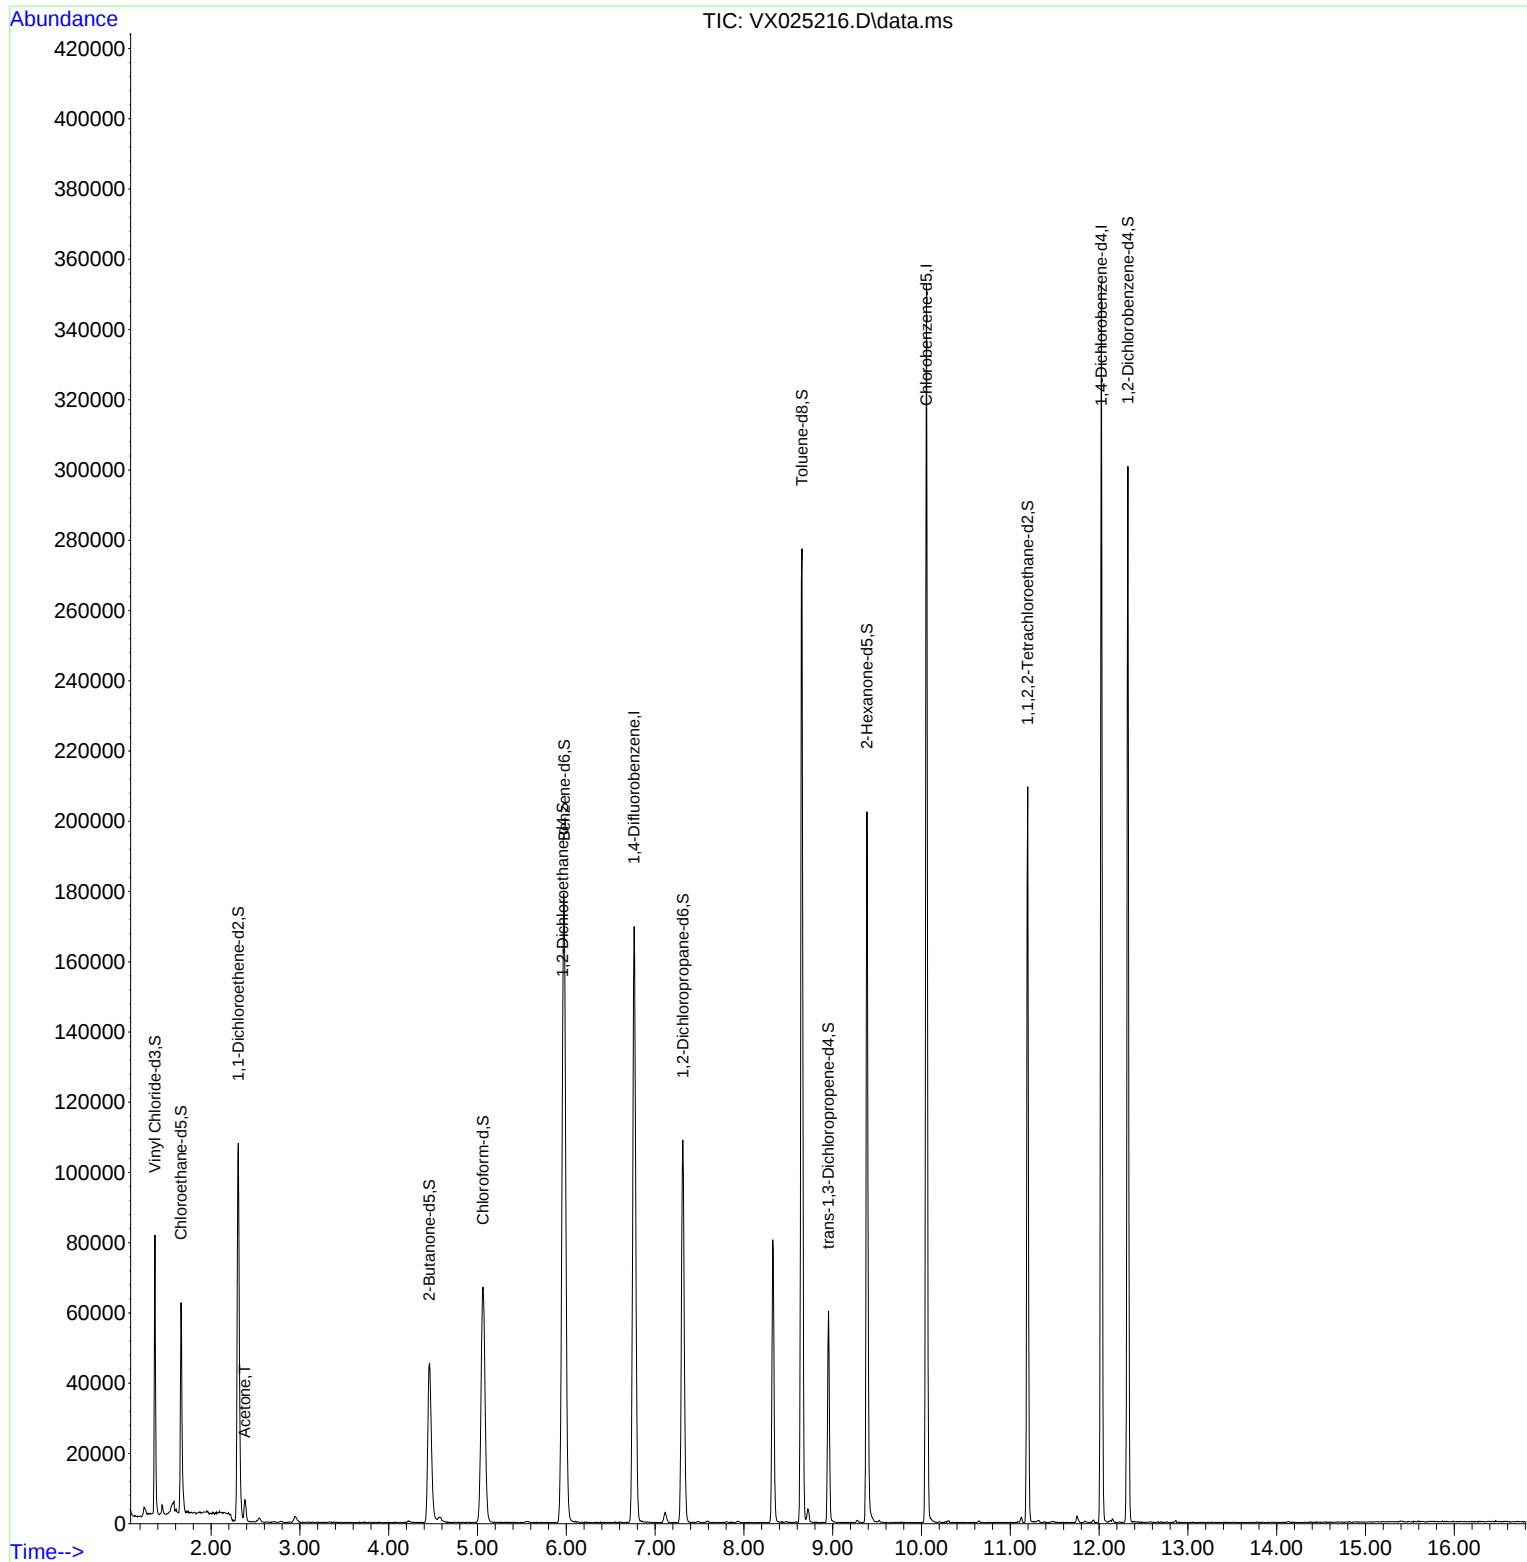

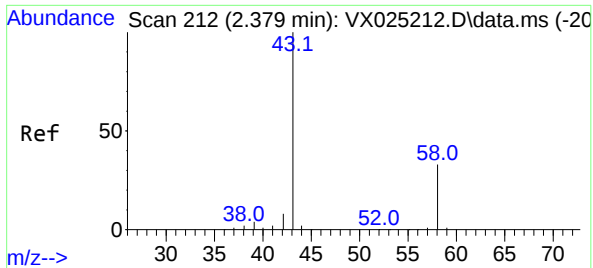

#13
 Acetone
 Concen: 7.515 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX025216.D
 Acq: 18 Nov 2021 18:00

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB9

Tgt Ion: 43 Resp: 6606
 Ion Ratio Lower Upper
 43 100
 58 30.1 0.0 64.8

