

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025219.D
 Acq On : 18 Nov 2021 19:10
 Operator : JC/MD
 Sample : M4677-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB1

Quant Time: Nov 19 05:29:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 19 05:25:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	174264	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	157590	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	73176	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	47819	40.618	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.240%
7) Chloroethane-d5	1.666	69	40794	60.798	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	121.600%
11) 1,1-Dichloroethene-d2	2.306	63	60236	29.748	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	59.500%#
21) 2-Butanone-d5	4.458	46	81890	92.045	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.050%
24) Chloroform-d	5.062	84	87604	42.298	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	5.958	65	56012	44.617	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.240%
32) Benzene-d6	5.976	84	182873	42.518	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.040%
36) 1,2-Dichloropropane-d6	7.312	67	56990	43.394	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.780%
41) Toluene-d8	8.653	98	169823	41.345	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.700%
43) trans-1,3-Dichloroprop...	8.952	79	27826	39.031	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.060%
47) 2-Hexanone-d5	9.384	63	61652	87.421	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.420%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	79529	42.044	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.080%
66) 1,2-Dichlorobenzene-d4	12.323	152	65256	44.986	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.980%
Target Compounds						
					Qvalue	
13) Acetone	2.380	43	1773	2.125	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025219.D
Acq On : 18 Nov 2021 19:10
Operator : JC/MD
Sample : M4677-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB1

Quant Time: Nov 19 05:29:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 19 05:25:45 2021
Response via : Initial Calibration

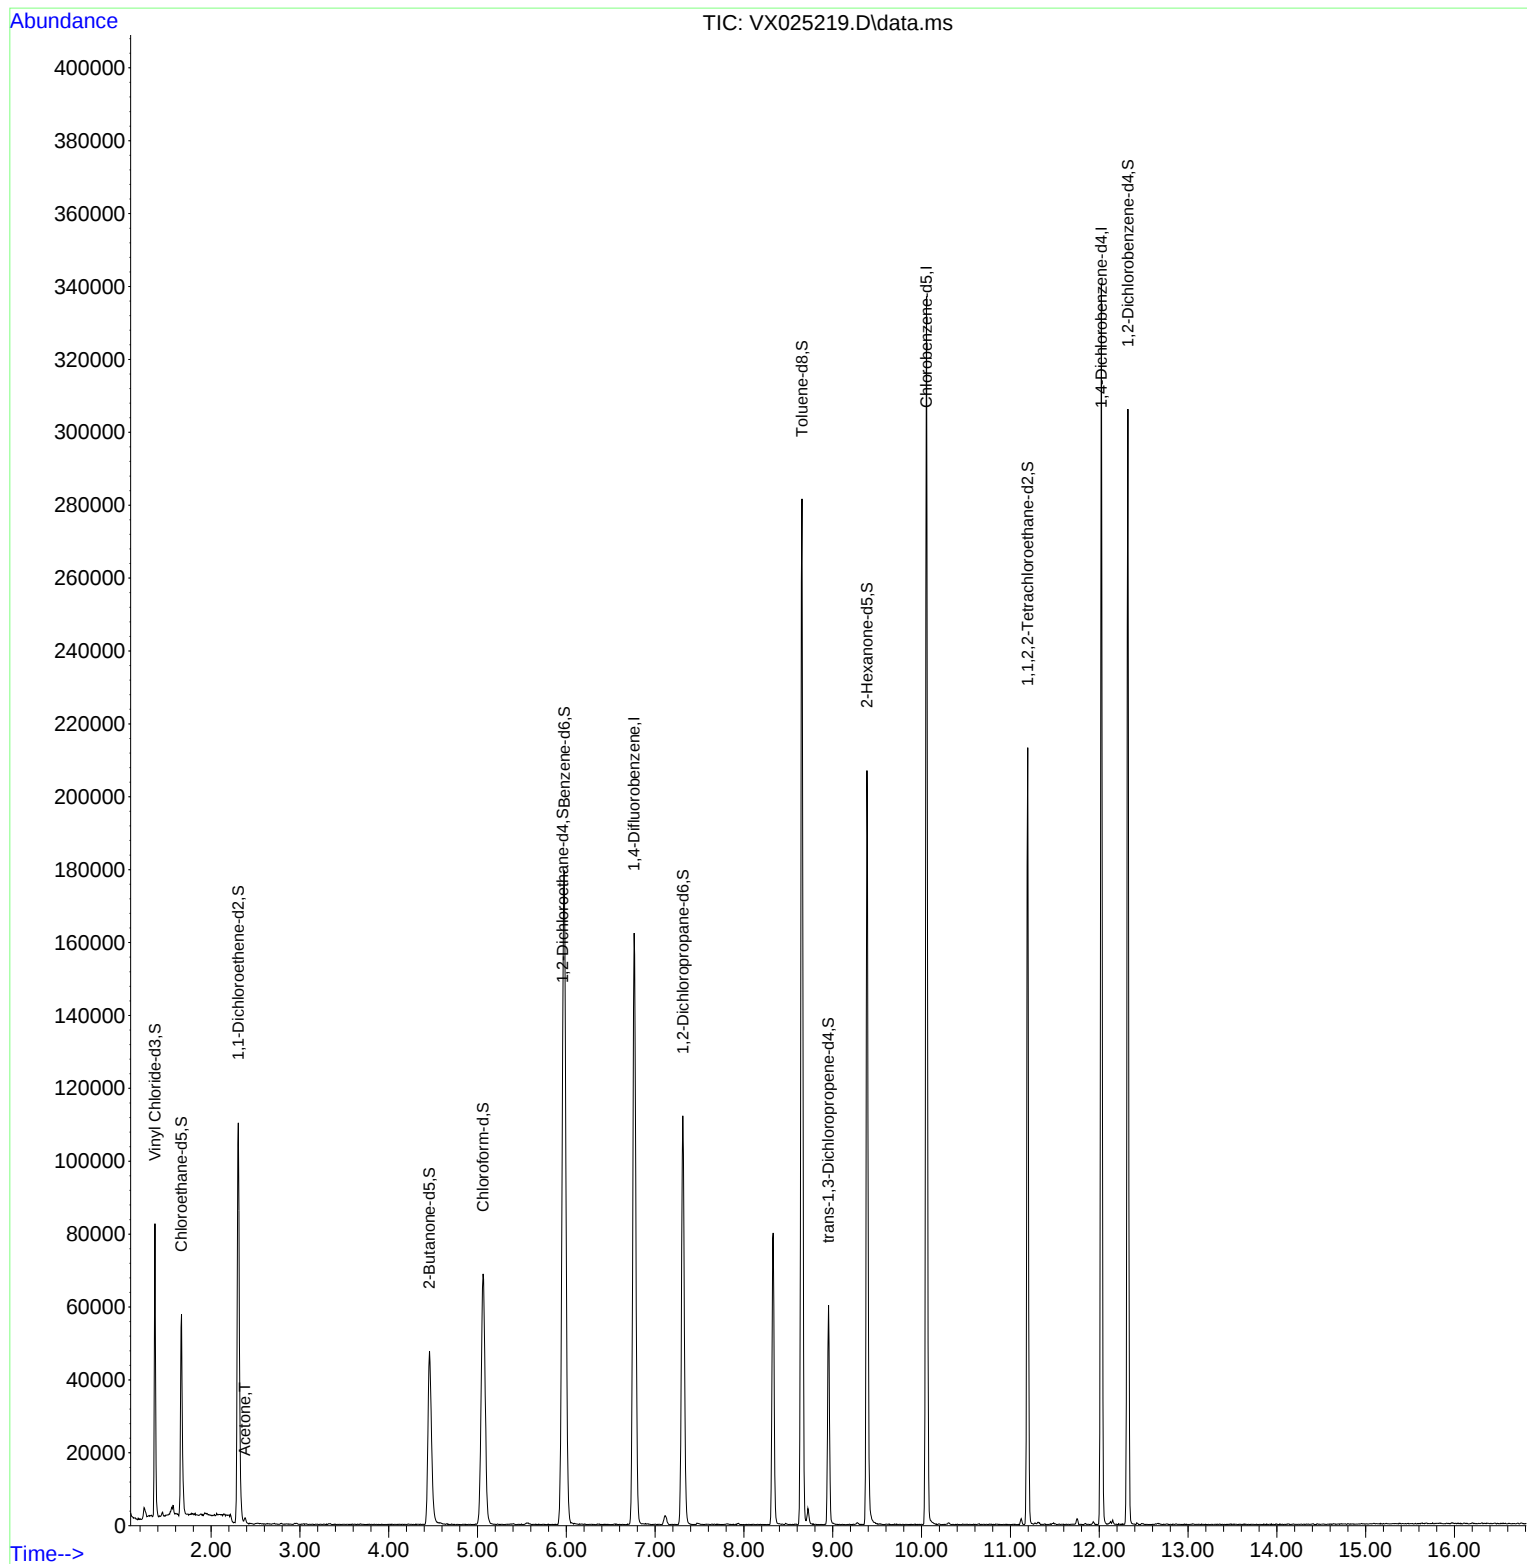

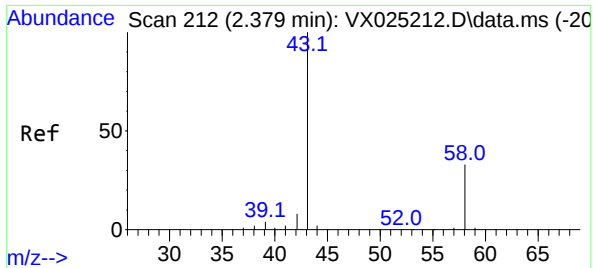

#13
 Acetone
 Concen: 2.125 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX025219.D
 Acq: 18 Nov 2021 19:10

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB1

Tgt Ion: 43 Resp: 1773
 Ion Ratio Lower Upper
 43 100
 58 25.2 0.0 64.8

