

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025227.D
 Acq On : 18 Nov 2021 22:18
 Operator : JC/MD
 Sample : M4677-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB0

Quant Time: Nov 19 05:31:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 19 05:25:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	171034	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	152841	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	72815	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	44825	38.794	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.580%
7) Chloroethane-d5	1.666	69	38576	58.578	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	117.160%
11) 1,1-Dichloroethene-d2	2.306	63	57431	28.899	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.800%#
21) 2-Butanone-d5	4.458	46	75931	86.959	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.960%
24) Chloroform-d	5.062	84	85989	42.302	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	5.964	65	54867	44.531	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.060%
32) Benzene-d6	5.976	84	177034	42.439	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.880%
36) 1,2-Dichloropropane-d6	7.312	67	55094	43.254	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.500%
41) Toluene-d8	8.653	98	163588	41.065	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.120%
43) trans-1,3-Dichloroprop...	8.951	79	26594	38.462	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.920%
47) 2-Hexanone-d5	9.384	63	57702	84.362	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.360%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	76722	41.821	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.640%
66) 1,2-Dichlorobenzene-d4	12.323	152	63706	44.135	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.260%
Target Compounds						
					Qvalue	
51) Chlorobenzene	10.079	112	48973	14.944	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025227.D
Acq On : 18 Nov 2021 22:18
Operator : JC/MD
Sample : M4677-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB0

Quant Time: Nov 19 05:31:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 19 05:25:45 2021
Response via : Initial Calibration

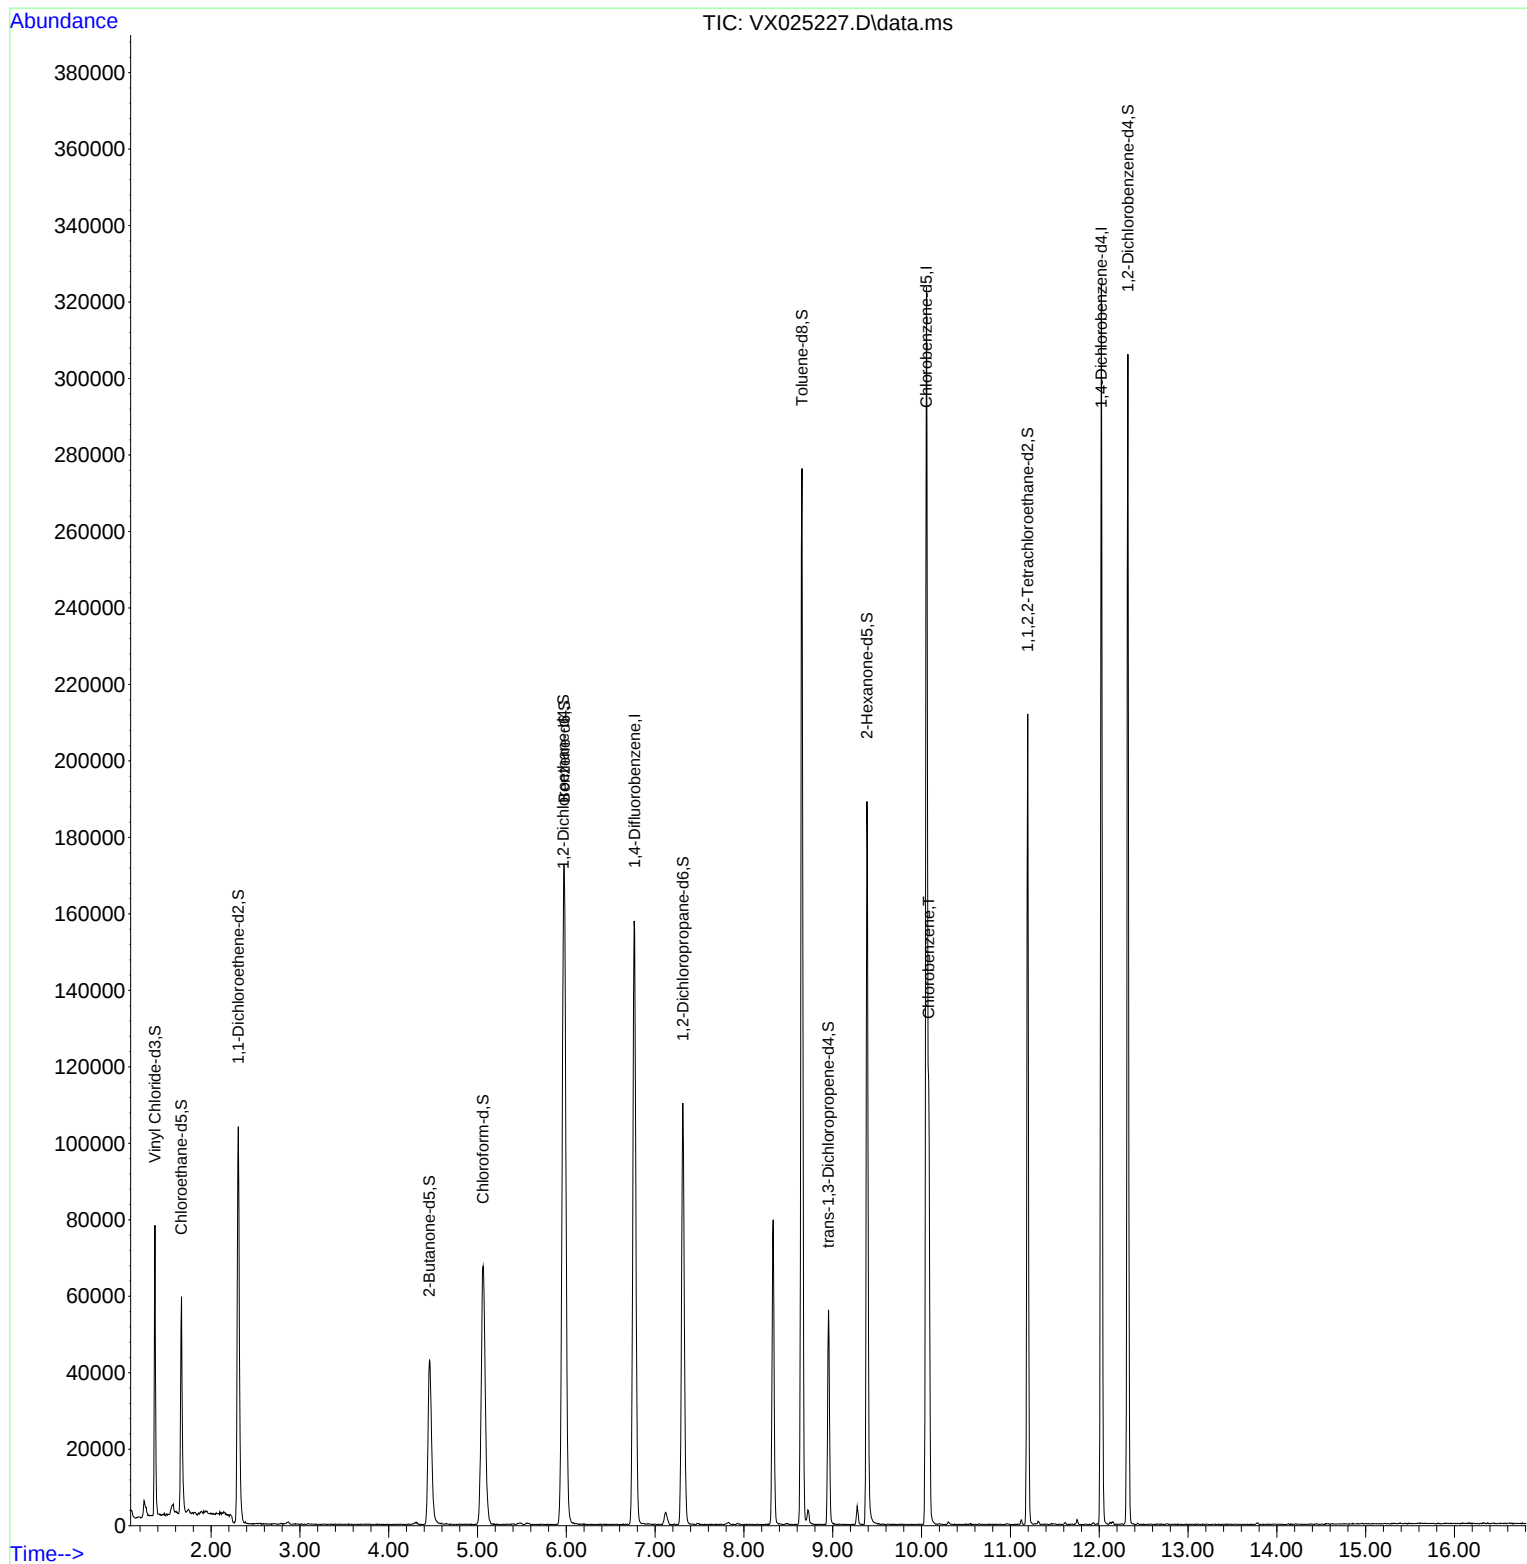

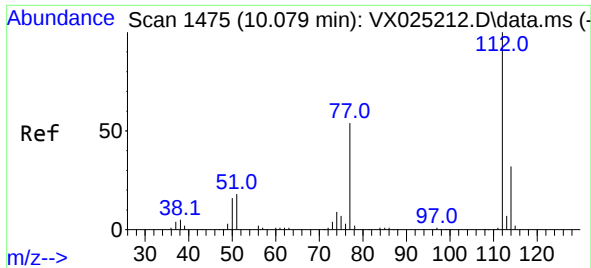

#51
Chlorobenzene
Concen: 14.944 ug/L
RT: 10.079 min Scan# 14
Delta R.T. 0.000 min
Lab File: VX025227.D
Acq: 18 Nov 2021 22:18

Instrument :
MSVOA_X
ClientSampleId :
H0AB0

Tgt Ion	Ratio	Lower	Upper
112	100		
114	31.9	22.7	42.3
77	53.4	46.8	70.2

