

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025214.D
 Acq On : 18 Nov 2021 17:13
 Operator : JC/MD
 Sample : M4677-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	89046	88643	14.86%	1.833%
2	1.660	91	94	103	rVB	65958	86627	14.52%	1.791%
3	2.306	194	200	208	rBV	123133	201892	33.85%	4.174%
4	2.782	276	278	279	rBV2	346	357	0.06%	0.007%
5	2.947	297	305	313	rVB3	2016	4808	0.81%	0.099%
6	3.032	318	319	321	rBV2	181	143	0.02%	0.003%
7	3.300	362	363	366	rVB	167	151	0.03%	0.003%
8	3.428	381	384	385	rBV	258	180	0.03%	0.004%
9	3.568	405	407	408	rBV	136	107	0.02%	0.002%
10	3.879	457	458	462	rBV	105	70	0.01%	0.001%
11	3.983	472	475	476	rBV2	120	105	0.02%	0.002%
12	4.062	486	488	490	rBV2	149	107	0.02%	0.002%
13	4.452	543	552	566	rBV	49943	137350	23.03%	2.840%
14	4.800	608	609	613	rBV	139	129	0.02%	0.003%
15	4.861	618	619	621	rBV	158	66	0.01%	0.001%
16	5.056	641	651	667	rVB	75952	234200	39.26%	4.842%
17	5.306	691	692	693	rVB	208	76	0.01%	0.002%
18	5.324	693	695	696	rBV2	208	150	0.03%	0.003%
19	5.361	699	701	702	rVB2	104	63	0.01%	0.001%
20	5.379	702	704	705	rBV	113	85	0.01%	0.002%
21	5.538	728	730	731	rBV	248	183	0.03%	0.004%
22	5.720	759	760	761	rBV	191	88	0.01%	0.002%
23	5.781	768	770	773	rBV	128	106	0.02%	0.002%
24	5.970	789	801	818	rBV2	202406	596462	100.00%	12.331%
25	6.214	840	841	843	rBV	167	111	0.02%	0.002%
26	6.354	863	864	867	rBV2	119	136	0.02%	0.003%
27	6.470	881	883	886	rBV3	116	163	0.03%	0.003%
28	6.531	891	893	894	rBV	99	81	0.01%	0.002%
29	6.592	902	903	904	rBV	177	92	0.02%	0.002%
30	6.763	921	931	947	rBV	169910	410936	68.90%	8.496%
31	6.940	958	960	962	rBV3	161	136	0.02%	0.003%
32	7.001	968	970	972	rVB	166	94	0.02%	0.002%
33	7.117	981	989	995	rBV3	3798	8480	1.42%	0.175%
34	7.312	1012	1021	1036	rVB	122939	269451	45.17%	5.571%
35	7.415	1036	1038	1040	rBV	197	82	0.01%	0.002%
36	7.586	1060	1066	1070	rBV3	451	903	0.15%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025214.D
 Acq On : 18 Nov 2021 17:13
 Operator : JC/MD
 Sample : M4677-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	7.659	1077	1078	1080	rBV2	104	71	0.01%	0.001%
38	7.860	1109	1111	1115	rVB2	133	141	0.02%	0.003%
39	7.933	1119	1123	1127	rVB3	533	783	0.13%	0.016%
40	8.074	1145	1146	1149	rBV2	92	90	0.02%	0.002%
41	8.208	1165	1168	1172	rVB2	91	146	0.02%	0.003%
42	8.238	1172	1173	1177	rVB	115	103	0.02%	0.002%
43	8.275	1177	1179	1180	rBV	152	121	0.02%	0.003%
44	8.324	1180	1187	1198	rBV	93273	153082	25.67%	3.165%
45	8.476	1208	1212	1216	rVB3	334	555	0.09%	0.011%
46	8.525	1219	1220	1221	rBV	129	68	0.01%	0.001%
47	8.567	1224	1227	1228	rBV	170	209	0.04%	0.004%
48	8.647	1234	1240	1248	rBV	318164	502324	84.22%	10.385%
49	8.952	1284	1290	1298	rBV	70270	100098	16.78%	2.069%
50	9.195	1329	1330	1332	rVB	123	67	0.01%	0.001%
51	9.214	1332	1333	1335	rBV	119	56	0.01%	0.001%
52	9.232	1335	1336	1338	rVB2	96	57	0.01%	0.001%
53	9.384	1355	1361	1374	rBV	225780	311700	52.26%	6.444%
54	9.573	1391	1392	1393	rBV	105	60	0.01%	0.001%
55	9.640	1402	1403	1405	rBV2	100	71	0.01%	0.001%
56	9.768	1423	1424	1426	rBV	207	115	0.02%	0.002%
57	9.811	1429	1431	1433	rBV	130	82	0.01%	0.002%
58	9.872	1439	1441	1443	rBV2	116	92	0.02%	0.002%
59	9.890	1443	1444	1447	rVB2	117	80	0.01%	0.002%
60	9.915	1447	1448	1453	rBV2	206	303	0.05%	0.006%
61	9.976	1456	1458	1459	rBV2	173	117	0.02%	0.002%
62	10.055	1465	1471	1487	rBV	380174	492680	82.60%	10.186%
63	10.305	1508	1512	1515	rVB2	879	979	0.16%	0.020%
64	10.421	1528	1531	1533	rBV	124	124	0.02%	0.003%
65	10.518	1546	1547	1549	rBV	142	109	0.02%	0.002%
66	10.695	1574	1576	1578	rBV	178	100	0.02%	0.002%
67	10.744	1583	1584	1585	rBV	220	87	0.01%	0.002%
68	10.817	1595	1596	1599	rBV2	127	122	0.02%	0.003%
69	10.860	1601	1603	1605	rVV	140	99	0.02%	0.002%
70	10.921	1612	1613	1614	rBV	125	54	0.01%	0.001%
71	11.079	1637	1639	1641	rBV	256	211	0.04%	0.004%
72	11.122	1642	1646	1652	rVB2	2043	2765	0.46%	0.057%
73	11.195	1652	1658	1667	rBV	236931	302660	50.74%	6.257%
74	11.457	1698	1701	1702	rBV	237	241	0.04%	0.005%
75	11.640	1729	1731	1735	rVB2	222	286	0.05%	0.006%
76	11.683	1735	1738	1739	rBV2	175	179	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025214.D
 Acq On : 18 Nov 2021 17:13
 Operator : JC/MD
 Sample : M4677-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	11.695	1739	1740	1741	rVV	243	105	0.02%	0.002%
78	11.750	1745	1749	1756	rVV5	1891	3025	0.51%	0.063%
79	11.847	1761	1765	1767	rVB3	348	415	0.07%	0.009%
80	11.933	1776	1779	1783	rVB3	1131	1484	0.25%	0.031%
81	12.024	1789	1794	1806	rVB	386552	471440	79.04%	9.747%
82	12.122	1808	1810	1812	rBV2	581	641	0.11%	0.013%
83	12.231	1822	1828	1829	rBV3	396	580	0.10%	0.012%
84	12.323	1838	1843	1851	rVB	355660	441953	74.10%	9.137%
85	12.488	1867	1870	1873	rBV	281	386	0.06%	0.008%
86	12.859	1927	1931	1934	rVB2	881	1029	0.17%	0.021%
87	13.103	1968	1971	1974	rBV2	113	123	0.02%	0.003%
88	13.311	2004	2005	2008	rVB	222	132	0.02%	0.003%
89	13.341	2008	2010	2011	rBV	207	131	0.02%	0.003%
90	13.457	2026	2029	2031	rBV2	147	159	0.03%	0.003%
91	13.475	2031	2032	2033	rBV	119	52	0.01%	0.001%
92	13.615	2053	2055	2057	rBV2	163	203	0.03%	0.004%
93	13.646	2059	2060	2061	rBV	208	89	0.01%	0.002%
94	13.823	2088	2089	2090	rVB	144	53	0.01%	0.001%
95	13.993	2115	2117	2121	rBV2	179	192	0.03%	0.004%
96	14.024	2121	2122	2125	rVB2	143	120	0.02%	0.002%
97	14.249	2157	2159	2160	rBV	186	152	0.03%	0.003%
98	14.323	2170	2171	2172	rBV	131	59	0.01%	0.001%
99	14.377	2179	2180	2181	rBV	195	85	0.01%	0.002%
100	14.499	2196	2200	2202	rBV2	210	310	0.05%	0.006%




Sum of corrected areas: 4837018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025214.D
Acq On : 18 Nov 2021 17:13
Operator : JC/MD
Sample : M4677-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

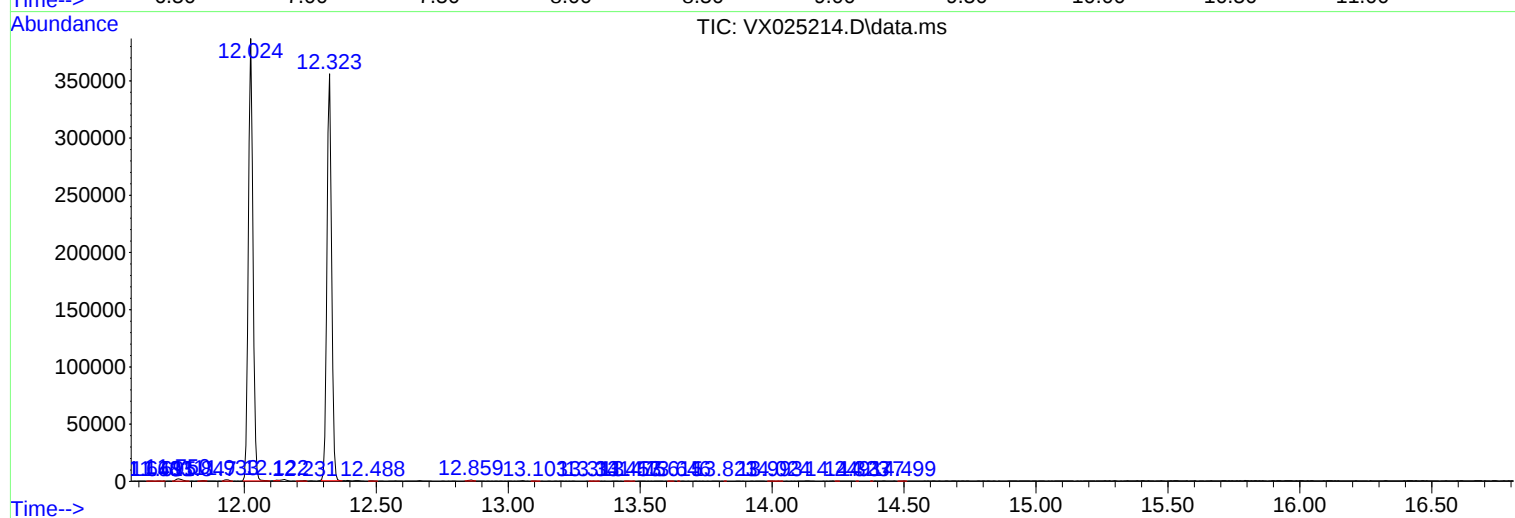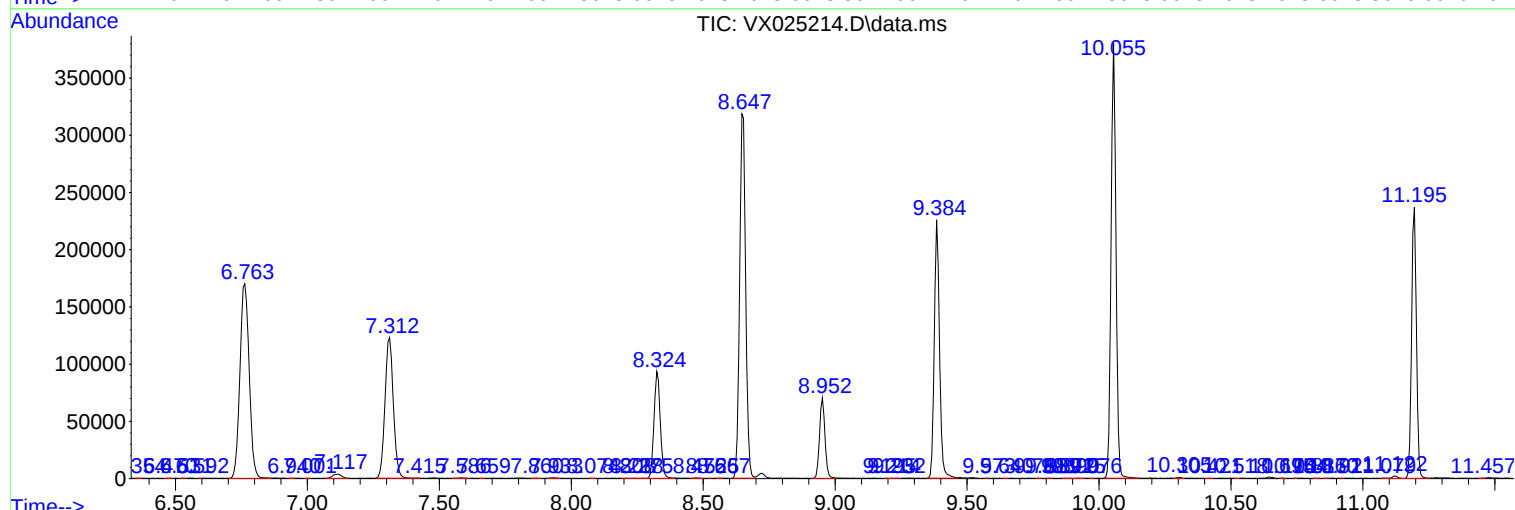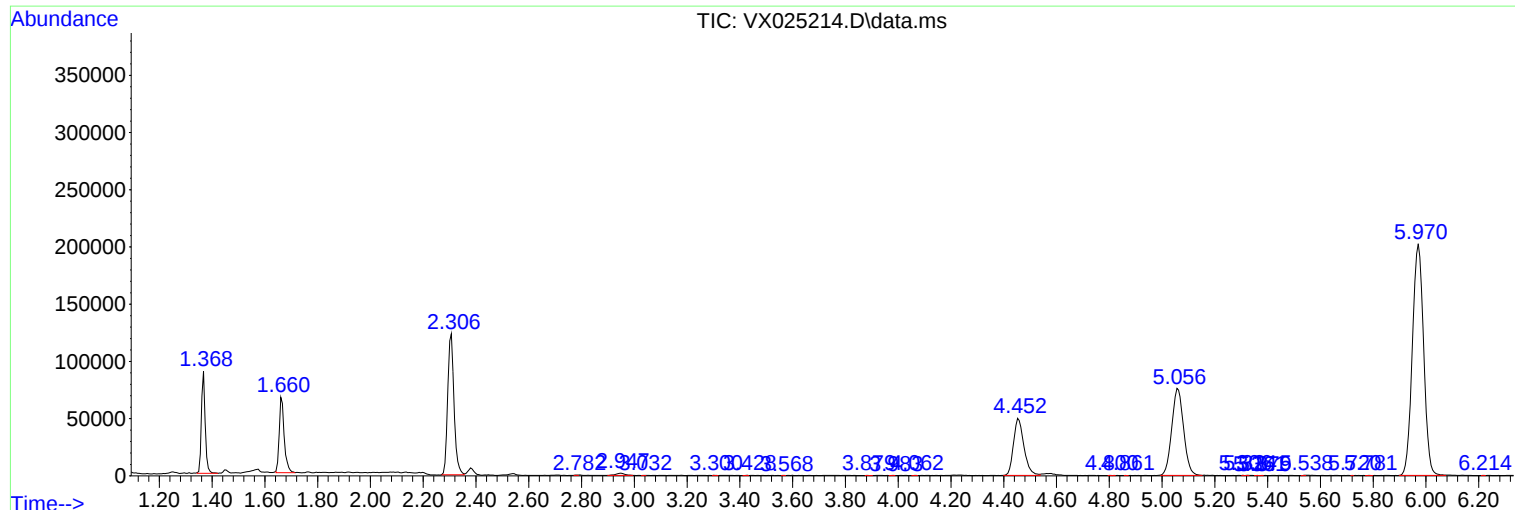

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025214.D
Acq On : 18 Nov 2021 17:13
Operator : JC/MD
Sample : M4677-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025214.D
Acq On : 18 Nov 2021 17:13
Operator : JC/MD
Sample : M4677-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc