

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025216.D
 Acq On : 18 Nov 2021 18:00
 Operator : JC/MD
 Sample : M4677-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	79678	77734	14.68%	1.764%
2	1.447	57	59	64	rVB	2643	2794	0.53%	0.063%
3	1.660	90	94	103	rVB	59873	76466	14.44%	1.735%
4	2.307	193	200	209	rBV	107605	178859	33.78%	4.058%
5	2.380	209	212	220	rVB	6199	9978	1.88%	0.226%
6	2.544	231	239	244	rVB3	1167	2462	0.46%	0.056%
7	2.947	298	305	314	rBV4	1720	4439	0.84%	0.101%
8	3.142	334	337	340	rBV2	181	234	0.04%	0.005%
9	3.191	343	345	347	rBV2	153	154	0.03%	0.003%
10	3.386	375	377	379	rVV	224	144	0.03%	0.003%
11	3.410	379	381	384	rVB2	172	177	0.03%	0.004%
12	3.599	411	412	417	rBV2	90	154	0.03%	0.003%
13	3.715	428	431	432	rBV	129	128	0.02%	0.003%
14	4.075	488	490	495	rVB	159	151	0.03%	0.003%
15	4.215	511	513	514	rBV2	358	340	0.06%	0.008%
16	4.459	544	553	567	rBV	45501	129614	24.48%	2.941%
17	4.739	597	599	601	rVV	222	161	0.03%	0.004%
18	5.062	639	652	672	rBV2	67100	211393	39.92%	4.796%
19	5.221	676	678	680	rVV2	150	157	0.03%	0.004%
20	5.379	703	704	707	rBV	124	127	0.02%	0.003%
21	5.556	728	733	734	rBV3	244	406	0.08%	0.009%
22	5.666	750	751	754	rBV2	172	152	0.03%	0.003%
23	5.806	773	774	777	rBV2	142	155	0.03%	0.004%
24	5.971	789	801	821	rBV2	179184	529491	100.00%	12.012%
25	6.099	821	822	825	rVB2	241	153	0.03%	0.003%
26	6.172	830	834	837	rVB2	175	278	0.05%	0.006%
27	6.202	837	839	842	rBV2	196	183	0.03%	0.004%
28	6.324	856	859	861	rBV	158	141	0.03%	0.003%
29	6.556	892	897	900	rVB2	246	345	0.07%	0.008%
30	6.592	902	903	905	rBV2	218	176	0.03%	0.004%
31	6.763	920	931	942	rBV	169707	399324	75.42%	9.059%
32	6.989	967	968	971	rVB2	199	168	0.03%	0.004%
33	7.019	971	973	975	rBV2	179	156	0.03%	0.004%
34	7.111	981	988	998	rVB2	2958	6269	1.18%	0.142%
35	7.202	1000	1003	1005	rVB2	157	151	0.03%	0.003%
36	7.312	1012	1021	1032	rBV	109046	237209	44.80%	5.381%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025216.D
 Acq On : 18 Nov 2021 18:00
 Operator : JC/MD
 Sample : M4677-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	7.482	1045	1049	1053	rBV2	316	589	0.11%	0.013%
38	7.568	1060	1063	1064	rBV	169	190	0.04%	0.004%
39	7.592	1064	1067	1071	rVB3	433	693	0.13%	0.016%
40	7.720	1084	1088	1090	rBV2	139	207	0.04%	0.005%
41	7.854	1107	1110	1111	rVB2	214	161	0.03%	0.004%
42	7.867	1111	1112	1114	rBV	199	149	0.03%	0.003%
43	7.934	1117	1123	1130	rBV3	490	1004	0.19%	0.023%
44	8.324	1181	1187	1197	rVV	80450	131999	24.93%	2.995%
45	8.580	1227	1229	1233	rVB2	232	275	0.05%	0.006%
46	8.653	1234	1241	1248	rBV	277298	440429	83.18%	9.992%
47	8.720	1249	1252	1261	rVB	3774	6125	1.16%	0.139%
48	8.952	1285	1290	1301	rVV	60292	87126	16.45%	1.977%
49	9.061	1305	1308	1310	rVV2	109	125	0.02%	0.003%
50	9.171	1325	1326	1330	rBV2	118	176	0.03%	0.004%
51	9.281	1338	1344	1348	rBV2	681	1044	0.20%	0.024%
52	9.385	1356	1361	1375	rBV	202274	285436	53.91%	6.476%
53	9.525	1382	1384	1388	rVB3	563	489	0.09%	0.011%
54	9.635	1401	1402	1405	rVB	148	136	0.03%	0.003%
55	9.689	1407	1411	1413	rVB2	103	142	0.03%	0.003%
56	9.781	1425	1426	1429	rBV2	167	174	0.03%	0.004%
57	9.933	1450	1451	1454	rBV	148	137	0.03%	0.003%
58	10.055	1466	1471	1488	rVB	352615	467779	88.35%	10.612%
59	10.208	1492	1496	1499	rVB3	240	359	0.07%	0.008%
60	10.269	1505	1506	1508	rVV	280	203	0.04%	0.005%
61	10.299	1508	1511	1514	rVV2	543	659	0.12%	0.015%
62	10.647	1564	1568	1572	rVV3	498	657	0.12%	0.015%
63	10.945	1616	1617	1622	rBV2	128	161	0.03%	0.004%
64	11.079	1634	1639	1642	rBV2	290	365	0.07%	0.008%
65	11.122	1642	1646	1650	rVV2	1464	1761	0.33%	0.040%
66	11.195	1652	1658	1668	rBV	209486	266847	50.40%	6.054%
67	11.323	1673	1679	1685	rVB6	613	1250	0.24%	0.028%
68	11.378	1686	1688	1691	rVB	239	210	0.04%	0.005%
69	11.451	1696	1700	1702	rBV	284	434	0.08%	0.010%
70	11.476	1702	1704	1707	rVV2	356	477	0.09%	0.011%
71	11.518	1710	1711	1715	rBV2	150	127	0.02%	0.003%
72	11.592	1722	1723	1727	rBV2	145	128	0.02%	0.003%
73	11.677	1735	1737	1741	rBV2	134	181	0.03%	0.004%
74	11.750	1744	1749	1755	rVB5	1823	2611	0.49%	0.059%
75	11.835	1760	1763	1767	rBV2	402	612	0.12%	0.014%
76	11.933	1776	1779	1782	rVB3	750	958	0.18%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025216.D
 Acq On : 18 Nov 2021 18:00
 Operator : JC/MD
 Sample : M4677-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1805	rVV	353363	447760	84.56%	10.158%
78	12.110	1807	1808	1809	rVV	394	251	0.05%	0.006%
79	12.146	1813	1814	1818	rVV3	1038	1126	0.21%	0.026%
80	12.323	1837	1843	1850	rBV	300575	380751	71.91%	8.638%
81	12.482	1868	1869	1871	rBV	204	127	0.02%	0.003%
82	12.664	1896	1899	1900	rBV	258	221	0.04%	0.005%
83	12.695	1902	1904	1907	rVB3	230	239	0.05%	0.005%
84	12.768	1913	1916	1917	rBV2	168	186	0.04%	0.004%
85	12.866	1928	1932	1934	rVV2	589	669	0.13%	0.015%
86	12.896	1934	1937	1940	rVV2	106	137	0.03%	0.003%
87	13.274	1996	1999	2001	rBV2	195	197	0.04%	0.004%
88	13.542	2042	2043	2048	rVB2	169	214	0.04%	0.005%
89	13.585	2048	2050	2052	rBV2	127	163	0.03%	0.004%
90	14.243	2155	2158	2162	rVB2	146	245	0.05%	0.006%
91	14.292	2162	2166	2168	rBV	125	152	0.03%	0.003%
92	14.317	2168	2170	2172	rBV	143	138	0.03%	0.003%
93	14.378	2178	2180	2184	rBV2	204	234	0.04%	0.005%
94	14.810	2249	2251	2257	rVB2	327	540	0.10%	0.012%
95	14.878	2257	2262	2263	rBV2	248	437	0.08%	0.010%
96	15.377	2343	2344	2345	rBV	215	137	0.03%	0.003%
97	15.560	2371	2374	2378	rBV3	286	513	0.10%	0.012%
98	15.865	2423	2424	2426	rBV	299	134	0.03%	0.003%
99	16.194	2477	2478	2481	rBV2	197	154	0.03%	0.003%
100	16.463	2521	2522	2523	rBV	326	136	0.03%	0.003%




Sum of corrected areas: 4407869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025216.D
Acq On : 18 Nov 2021 18:00
Operator : JC/MD
Sample : M4677-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

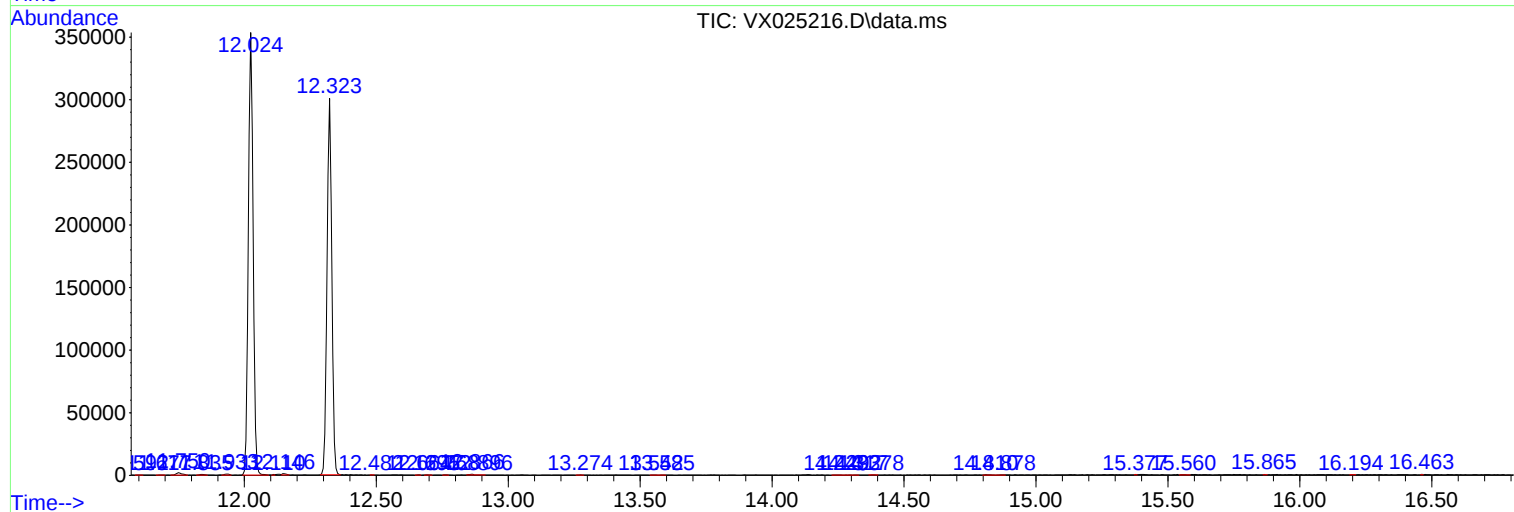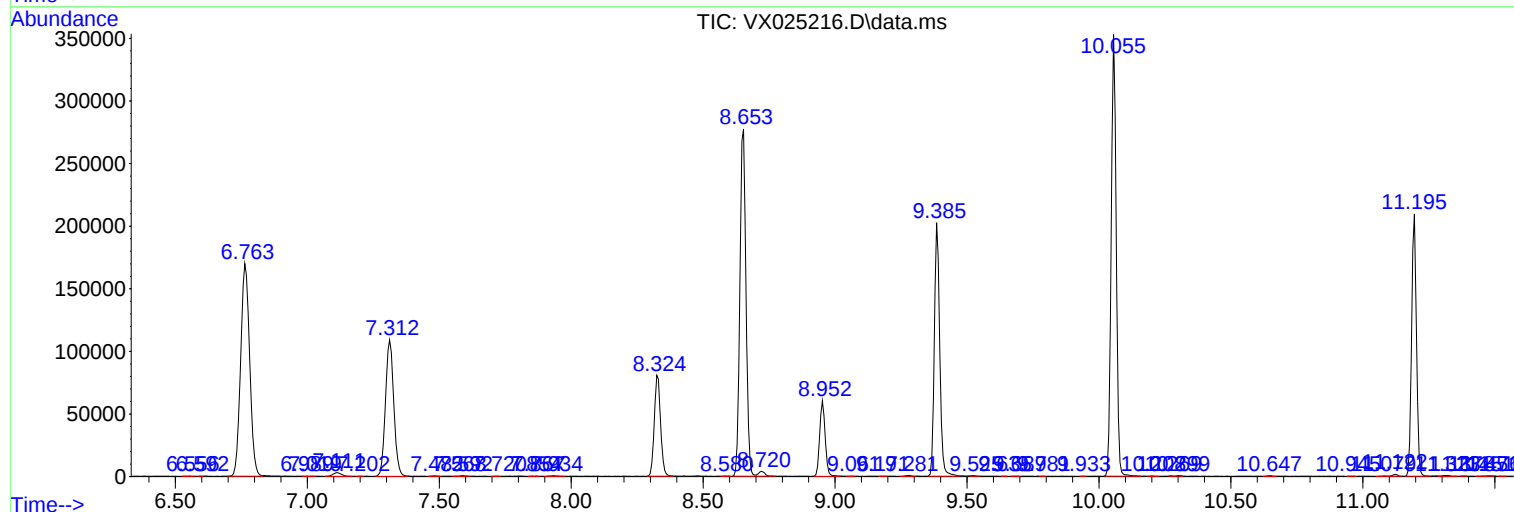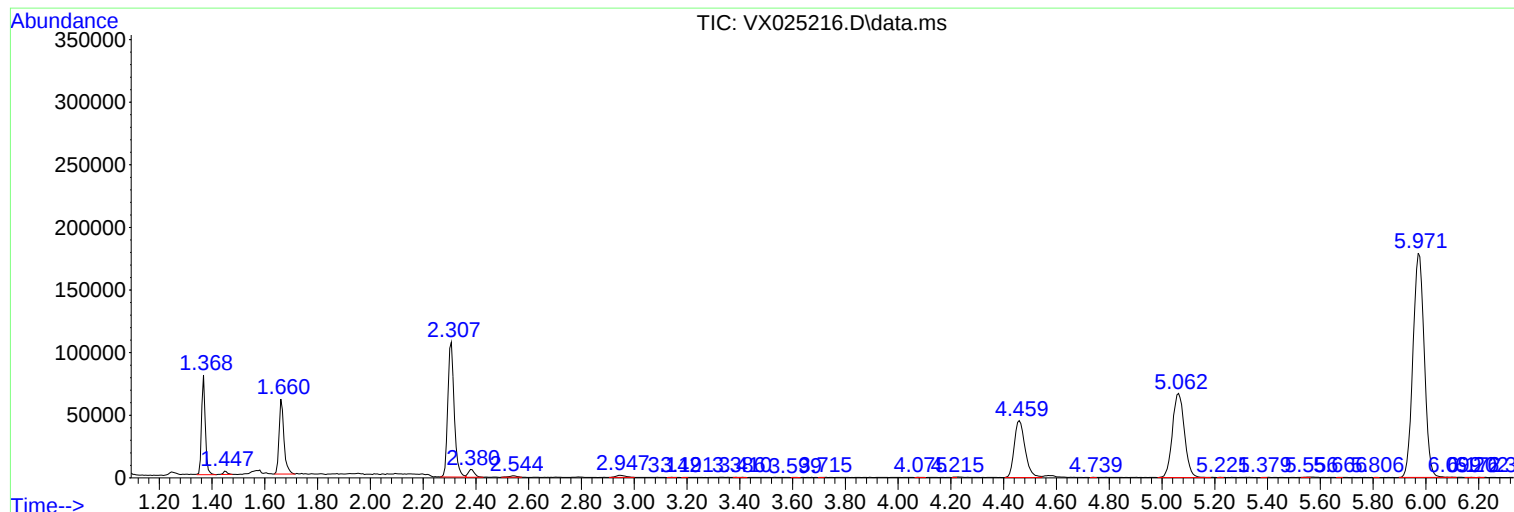

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025216.D
Acq On : 18 Nov 2021 18:00
Operator : JC/MD
Sample : M4677-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025216.D
Acq On : 18 Nov 2021 18:00
Operator : JC/MD
Sample : M4677-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc