

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025217.D
 Acq On : 18 Nov 2021 18:23
 Operator : JC/MD
 Sample : M4677-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV	3246	5408	1.02%	0.123%
2	1.368	42	46	53	rVB	76759	74351	14.08%	1.688%
3	1.660	90	94	106	rVB	56699	75038	14.21%	1.704%
4	2.306	193	200	208	rBV	106617	174913	33.13%	3.972%
5	2.380	208	212	218	rVB	6307	10132	1.92%	0.230%
6	2.538	236	238	241	rVB2	357	397	0.08%	0.009%
7	2.697	261	264	269	rBV3	237	475	0.09%	0.011%
8	2.788	276	279	281	rBV2	425	466	0.09%	0.011%
9	2.965	302	308	312	rVB3	442	964	0.18%	0.022%
10	3.075	323	326	328	rBV	142	150	0.03%	0.003%
11	3.331	365	368	371	rBV2	139	224	0.04%	0.005%
12	3.434	382	385	388	rBV2	157	199	0.04%	0.005%
13	3.544	402	403	405	rBV	172	171	0.03%	0.004%
14	3.690	426	427	430	rBV	196	158	0.03%	0.004%
15	3.745	434	436	438	rBV2	253	270	0.05%	0.006%
16	3.885	456	459	461	rBV2	116	129	0.02%	0.003%
17	3.995	475	477	480	rBV2	99	125	0.02%	0.003%
18	4.154	501	503	508	rBV2	106	162	0.03%	0.004%
19	4.221	508	514	516	rBV3	395	704	0.13%	0.016%
20	4.458	544	553	568	rBV	48823	137632	26.07%	3.125%
21	4.690	588	591	592	rBV2	210	170	0.03%	0.004%
22	4.715	592	595	598	rVV2	162	202	0.04%	0.005%
23	4.769	601	604	605	rBV	135	179	0.03%	0.004%
24	4.952	631	634	637	rVB2	138	162	0.03%	0.004%
25	5.062	640	652	668	rVV	69748	212050	40.17%	4.815%
26	5.342	696	698	701	rVB	197	170	0.03%	0.004%
27	5.373	701	703	704	rBV2	228	160	0.03%	0.004%
28	5.550	728	732	734	rBV2	356	487	0.09%	0.011%
29	5.970	789	801	818	rBV2	179480	527905	100.00%	11.988%
30	6.611	904	906	908	rVB2	186	155	0.03%	0.004%
31	6.763	921	931	946	rBV	164351	389213	73.73%	8.838%
32	6.976	965	966	968	rBV2	193	158	0.03%	0.004%
33	7.110	982	988	998	rVB5	2579	6049	1.15%	0.137%
34	7.312	1012	1021	1035	rVB	111816	239773	45.42%	5.445%
35	7.421	1037	1039	1040	rVB	250	145	0.03%	0.003%
36	7.464	1044	1046	1047	rBV2	202	163	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025217.D
 Acq On : 18 Nov 2021 18:23
 Operator : JC/MD
 Sample : M4677-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	7.482	1047	1049	1052	rVB	308	242	0.05%	0.005%
38	7.586	1063	1066	1073	rVB2	591	846	0.16%	0.019%
39	7.836	1106	1107	1109	rBV	124	122	0.02%	0.003%
40	7.927	1119	1122	1129	rBV3	370	583	0.11%	0.013%
41	8.043	1140	1141	1143	rBV	156	128	0.02%	0.003%
42	8.281	1179	1180	1181	rBV	187	115	0.02%	0.003%
43	8.330	1181	1188	1197	rVV	80541	133305	25.25%	3.027%
44	8.470	1210	1211	1212	rBV	254	119	0.02%	0.003%
45	8.549	1222	1224	1226	rBV	199	115	0.02%	0.003%
46	8.653	1234	1241	1248	rVV	284566	444010	84.11%	10.083%
47	8.720	1248	1252	1262	rVB	3716	6744	1.28%	0.153%
48	8.854	1272	1274	1278	rVB	141	122	0.02%	0.003%
49	8.952	1284	1290	1298	rBV	60685	86015	16.29%	1.953%
50	9.049	1304	1306	1310	rVB2	184	167	0.03%	0.004%
51	9.238	1335	1337	1340	rBV	207	259	0.05%	0.006%
52	9.281	1340	1344	1347	rBV3	297	381	0.07%	0.009%
53	9.384	1355	1361	1381	rBV	216680	305048	57.78%	6.927%
54	9.519	1381	1383	1387	rVB3	482	684	0.13%	0.016%
55	9.616	1396	1399	1401	rBV2	123	127	0.02%	0.003%
56	9.653	1403	1405	1408	rBV2	105	134	0.03%	0.003%
57	10.055	1465	1471	1487	rVB	334241	458330	86.82%	10.408%
58	10.195	1492	1494	1496	rVB2	312	236	0.04%	0.005%
59	10.250	1499	1503	1506	rBV2	79	125	0.02%	0.003%
60	10.500	1543	1544	1547	rVB	147	126	0.02%	0.003%
61	10.604	1559	1561	1564	rVV	158	146	0.03%	0.003%
62	10.646	1565	1568	1572	rVB2	469	609	0.12%	0.014%
63	10.866	1600	1604	1606	rVB2	207	261	0.05%	0.006%
64	11.122	1642	1646	1650	rBV2	1544	1929	0.37%	0.044%
65	11.195	1652	1658	1666	rBV	217347	277680	52.60%	6.306%
66	11.384	1687	1689	1693	rBV3	186	228	0.04%	0.005%
67	11.451	1698	1700	1701	rBV2	209	175	0.03%	0.004%
68	11.579	1718	1721	1724	rVB2	178	190	0.04%	0.004%
69	11.616	1724	1727	1729	rVB	222	219	0.04%	0.005%
70	11.634	1729	1730	1734	rBV	198	208	0.04%	0.005%
71	11.671	1734	1736	1741	rVV	153	194	0.04%	0.004%
72	11.750	1745	1749	1755	rVV4	1504	2212	0.42%	0.050%
73	11.799	1755	1757	1759	rVB2	191	138	0.03%	0.003%
74	11.847	1759	1765	1766	rBV2	474	545	0.10%	0.012%
75	11.933	1774	1779	1783	rVB3	870	1105	0.21%	0.025%
76	12.024	1789	1794	1806	rBV	349036	431890	81.81%	9.807%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025217.D
 Acq On : 18 Nov 2021 18:23
 Operator : JC/MD
 Sample : M4677-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	12.122	1807	1810	1812	rBV3	506	617	0.12%	0.014%
78	12.219	1824	1826	1829	rBV2	267	224	0.04%	0.005%
79	12.323	1837	1843	1851	rVB	303115	383218	72.59%	8.702%
80	12.433	1857	1861	1864	rVB3	429	476	0.09%	0.011%
81	12.481	1867	1869	1874	rVB2	161	202	0.04%	0.005%
82	12.567	1880	1883	1885	rVB	283	332	0.06%	0.008%
83	12.597	1885	1888	1889	rBV2	139	126	0.02%	0.003%
84	12.664	1896	1899	1900	rBV2	167	151	0.03%	0.003%
85	12.756	1913	1914	1919	rVB3	185	233	0.04%	0.005%
86	12.859	1929	1931	1935	rVB	574	523	0.10%	0.012%
87	12.969	1946	1949	1950	rBV	149	115	0.02%	0.003%
88	13.152	1976	1979	1981	rVV2	128	118	0.02%	0.003%
89	13.396	2017	2019	2021	rBV	152	124	0.02%	0.003%
90	13.676	2063	2065	2071	rBV2	160	273	0.05%	0.006%
91	13.731	2071	2074	2075	rBV2	174	120	0.02%	0.003%
92	14.140	2136	2141	2142	rBV	360	442	0.08%	0.010%
93	14.262	2158	2161	2162	rBV	185	125	0.02%	0.003%
94	14.384	2179	2181	2185	rVB2	219	195	0.04%	0.004%
95	14.426	2185	2188	2189	rBV2	156	151	0.03%	0.003%
96	14.865	2258	2260	2265	rBV3	215	321	0.06%	0.007%
97	14.993	2280	2281	2283	rBV2	205	150	0.03%	0.003%
98	15.091	2295	2297	2298	rBV	227	171	0.03%	0.004%
99	15.926	2433	2434	2436	rBV2	260	114	0.02%	0.003%
100	16.304	2494	2496	2497	rBV	302	184	0.03%	0.004%


Sum of corrected areas: 4403726

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025217.D
Acq On : 18 Nov 2021 18:23
Operator : JC/MD
Sample : M4677-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

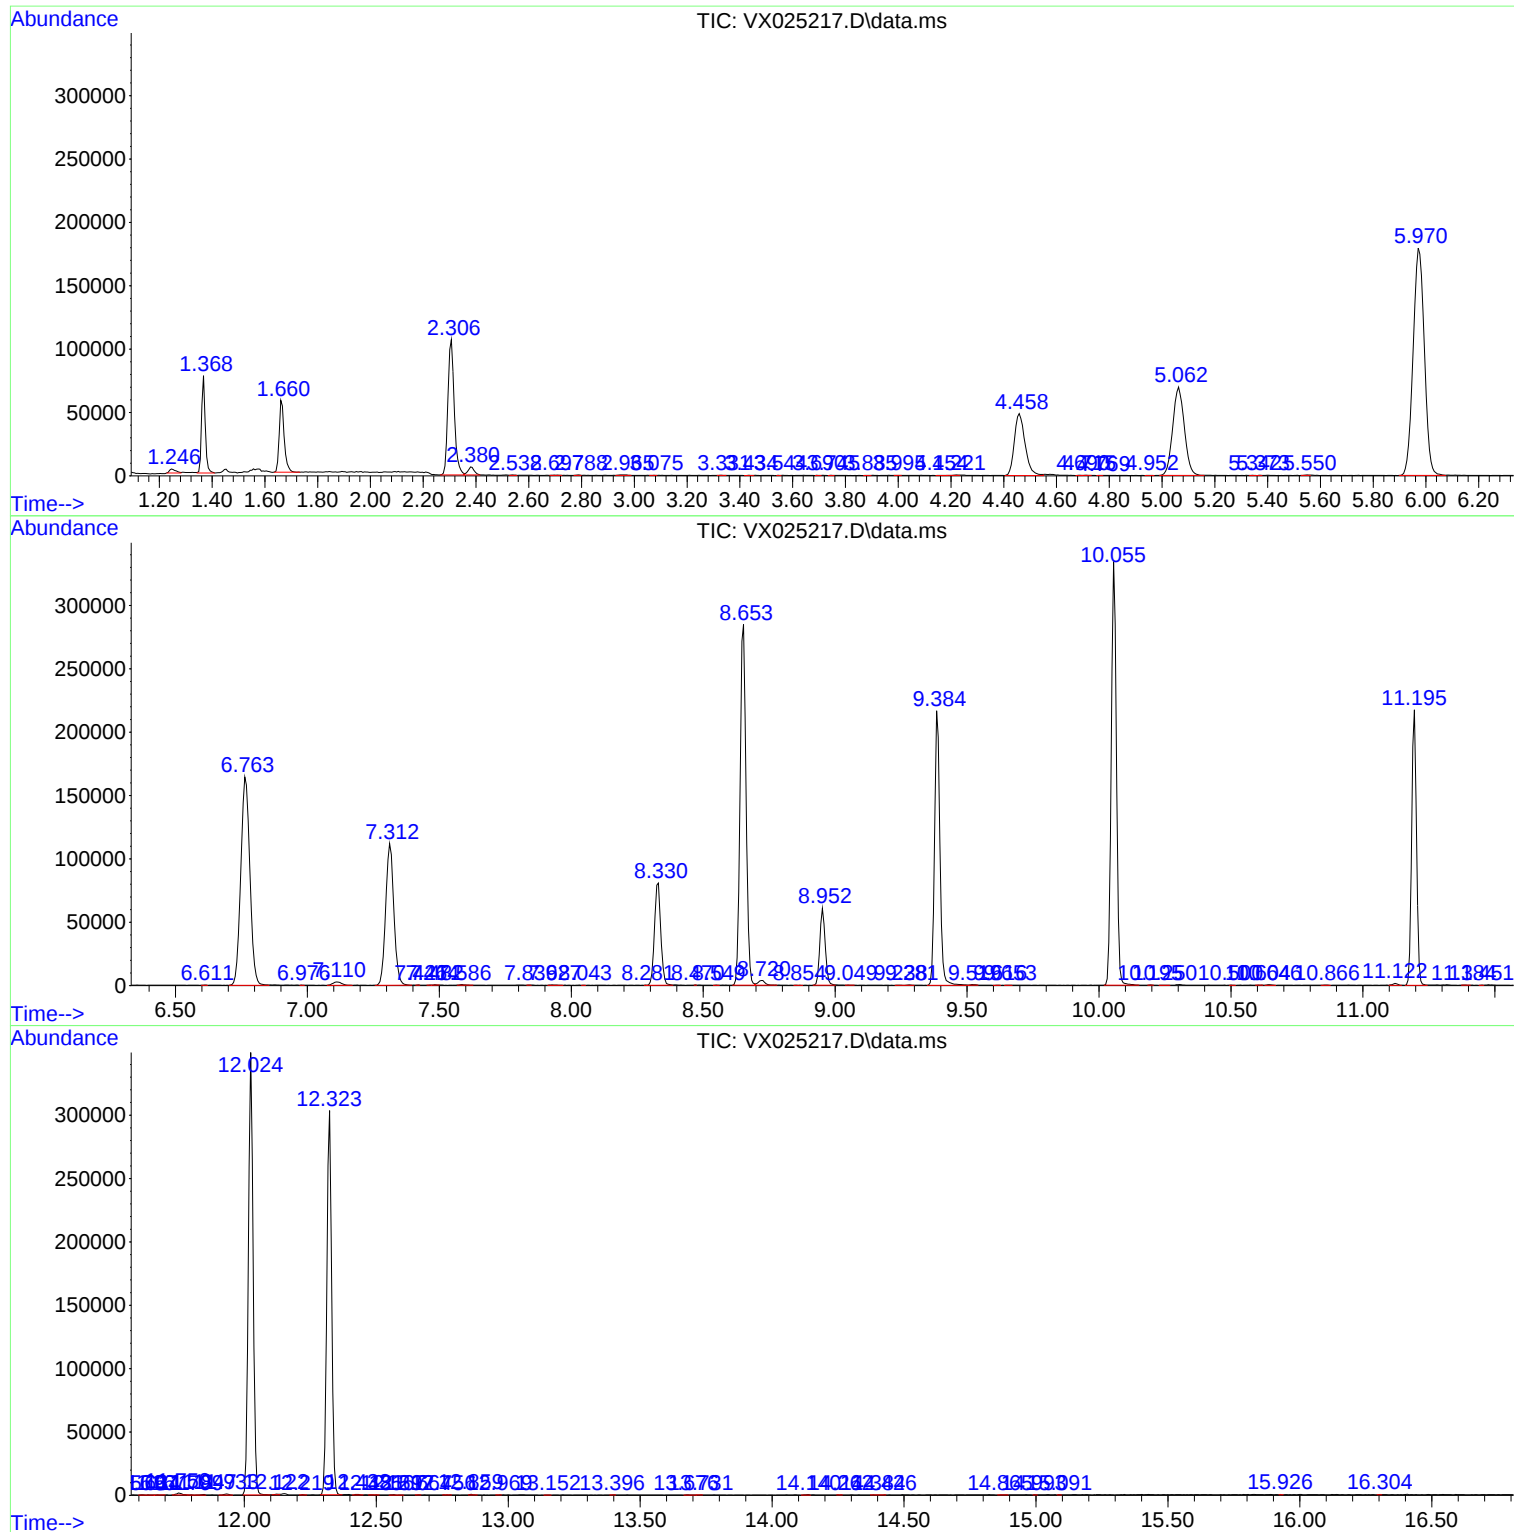

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025217.D
Acq On : 18 Nov 2021 18:23
Operator : JC/MD
Sample : M4677-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025217.D
Acq On : 18 Nov 2021 18:23
Operator : JC/MD
Sample : M4677-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
