

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025220.D
 Acq On : 18 Nov 2021 19:34
 Operator : JC/MD
 Sample : M4677-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV4	2528	4141	0.77%	0.094%
2	1.368	42	46	52	rBV	79343	76477	14.23%	1.738%
3	1.660	90	94	106	rVB	58440	77694	14.45%	1.765%
4	2.306	193	200	210	rBV	109711	181011	33.67%	4.113%
5	2.514	230	234	237	rBV3	281	368	0.07%	0.008%
6	2.959	300	307	310	rVB4	462	1044	0.19%	0.024%
7	3.483	392	393	395	rBV	141	111	0.02%	0.003%
8	3.770	437	440	441	rBV	128	121	0.02%	0.003%
9	3.934	463	467	468	rBV2	144	154	0.03%	0.003%
10	4.001	476	478	479	rBV	167	136	0.03%	0.003%
11	4.111	494	496	498	rBV	206	170	0.03%	0.004%
12	4.184	506	508	513	rBV2	155	226	0.04%	0.005%
13	4.233	513	516	518	rBV2	177	205	0.04%	0.005%
14	4.269	520	522	525	rVB2	121	121	0.02%	0.003%
15	4.367	536	538	539	rBV	138	124	0.02%	0.003%
16	4.385	539	541	544	rVB	206	106	0.02%	0.002%
17	4.458	544	553	568	rBV2	47167	133393	24.81%	3.031%
18	4.794	605	608	609	rBV	145	127	0.02%	0.003%
19	4.861	617	619	621	rBV	148	123	0.02%	0.003%
20	5.056	640	651	669	rBV	70922	218780	40.70%	4.971%
21	5.379	702	704	705	rBV	155	101	0.02%	0.002%
22	5.403	706	708	710	rVB2	262	159	0.03%	0.004%
23	5.556	726	733	741	rVB3	356	1063	0.20%	0.024%
24	5.848	780	781	784	rBV	118	120	0.02%	0.003%
25	5.891	786	788	790	rBV2	142	186	0.03%	0.004%
26	5.970	790	801	816	rBV2	183489	537594	100.00%	12.215%
27	6.098	821	822	823	rVB	352	131	0.02%	0.003%
28	6.342	859	862	863	rBV2	116	123	0.02%	0.003%
29	6.537	891	894	895	rBV2	151	154	0.03%	0.003%
30	6.665	913	915	918	rVB	184	114	0.02%	0.003%
31	6.763	920	931	945	rBV	160716	379537	70.60%	8.624%
32	7.110	980	988	996	rVB3	2922	6699	1.25%	0.152%
33	7.208	1000	1004	1005	rVB	134	136	0.03%	0.003%
34	7.238	1007	1009	1012	rVB	243	193	0.04%	0.004%
35	7.312	1012	1021	1035	rBV	111243	243165	45.23%	5.525%
36	7.482	1045	1049	1058	rBV3	429	732	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025220.D
 Acq On : 18 Nov 2021 19:34
 Operator : JC/MD
 Sample : M4677-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	7.708	1084	1086	1089	rVB2	127	161	0.03%	0.004%
38	7.757	1092	1094	1096	rVV2	136	121	0.02%	0.003%
39	7.830	1101	1106	1112	rVB4	715	1554	0.29%	0.035%
40	8.031	1136	1139	1141	rBV2	124	147	0.03%	0.003%
41	8.098	1149	1150	1154	rVB	134	117	0.02%	0.003%
42	8.141	1154	1157	1159	rBV2	87	108	0.02%	0.002%
43	8.177	1161	1163	1167	rVB2	130	118	0.02%	0.003%
44	8.208	1167	1168	1171	rBV2	115	109	0.02%	0.002%
45	8.330	1181	1188	1197	rBV	83245	134134	24.95%	3.048%
46	8.464	1207	1210	1212	rBV3	193	284	0.05%	0.006%
47	8.549	1222	1224	1225	rBV2	127	102	0.02%	0.002%
48	8.653	1234	1241	1248	rBV	289380	448983	83.52%	10.202%
49	8.720	1248	1252	1261	rVB	4151	6548	1.22%	0.149%
50	8.952	1284	1290	1303	rBV	61453	87807	16.33%	1.995%
51	9.128	1317	1319	1321	rBV2	123	114	0.02%	0.003%
52	9.281	1337	1344	1347	rBV3	767	1145	0.21%	0.026%
53	9.384	1356	1361	1373	rBV	206037	296484	55.15%	6.737%
54	9.519	1380	1383	1387	rVB2	1143	1569	0.29%	0.036%
55	9.823	1429	1433	1436	rBV2	135	242	0.05%	0.005%
56	9.927	1446	1450	1452	rBV2	116	151	0.03%	0.003%
57	10.055	1465	1471	1491	rVB	339064	450491	83.80%	10.236%
58	10.305	1508	1512	1515	rBV2	495	730	0.14%	0.017%
59	10.342	1515	1518	1521	rVV2	134	137	0.03%	0.003%
60	10.445	1531	1535	1539	rVB	140	202	0.04%	0.005%
61	10.494	1542	1543	1546	rBV	157	135	0.03%	0.003%
62	10.646	1566	1568	1570	rVB2	216	202	0.04%	0.005%
63	10.671	1570	1572	1574	rBV2	175	220	0.04%	0.005%
64	10.713	1577	1579	1582	rVV2	137	156	0.03%	0.004%
65	10.774	1587	1589	1590	rVV2	189	124	0.02%	0.003%
66	10.805	1591	1594	1598	rVV3	361	475	0.09%	0.011%
67	11.085	1638	1640	1642	rVB	148	123	0.02%	0.003%
68	11.122	1642	1646	1652	rBV3	1316	1881	0.35%	0.043%
69	11.195	1652	1658	1665	rVV	218627	274385	51.04%	6.234%
70	11.274	1669	1671	1674	rVV3	432	536	0.10%	0.012%
71	11.305	1674	1676	1682	rVB2	746	1193	0.22%	0.027%
72	11.488	1701	1706	1707	rBV3	340	427	0.08%	0.010%
73	11.652	1732	1733	1736	rVB2	221	164	0.03%	0.004%
74	11.677	1736	1737	1738	rBV	174	120	0.02%	0.003%
75	11.750	1745	1749	1754	rVB2	1447	2105	0.39%	0.048%
76	11.841	1762	1764	1769	rVB2	386	406	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025220.D
 Acq On : 18 Nov 2021 19:34
 Operator : JC/MD
 Sample : M4677-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	11.939	1775	1780	1784	rVB3	674	1023	0.19%	0.023%
78	11.975	1784	1786	1789	rBV	148	110	0.02%	0.002%
79	12.024	1789	1794	1806	rVV	339914	422283	78.55%	9.595%
80	12.128	1806	1811	1812	rVV3	746	949	0.18%	0.022%
81	12.152	1812	1815	1818	rVV3	1092	1444	0.27%	0.033%
82	12.323	1837	1843	1855	rVB	307303	391939	72.91%	8.905%
83	12.427	1857	1860	1864	rBV2	549	602	0.11%	0.014%
84	12.664	1895	1899	1902	rVV2	560	494	0.09%	0.011%
85	12.768	1911	1916	1921	rVB2	351	502	0.09%	0.011%
86	13.054	1961	1963	1968	rVB2	356	265	0.05%	0.006%
87	13.371	2014	2015	2018	rBV	122	101	0.02%	0.002%
88	13.439	2023	2026	2027	rBV2	118	105	0.02%	0.002%
89	13.591	2050	2051	2053	rBV	153	127	0.02%	0.003%
90	13.701	2067	2069	2073	rVB2	120	115	0.02%	0.003%
91	13.731	2073	2074	2077	rBV	174	142	0.03%	0.003%
92	14.134	2137	2140	2144	rBV2	245	339	0.06%	0.008%
93	14.237	2154	2157	2158	rVB2	221	185	0.03%	0.004%
94	14.274	2161	2163	2164	rBV	163	105	0.02%	0.002%
95	14.335	2170	2173	2175	rVB2	194	169	0.03%	0.004%
96	14.365	2175	2178	2180	rBV2	120	138	0.03%	0.003%
97	15.139	2304	2305	2312	rBV2	259	355	0.07%	0.008%
98	15.188	2312	2313	2314	rBV	306	138	0.03%	0.003%
99	16.438	2516	2518	2520	rBV2	263	247	0.05%	0.006%
100	16.627	2547	2549	2551	rBV	233	166	0.03%	0.004%


Sum of corrected areas: 4401092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025220.D
Acq On : 18 Nov 2021 19:34
Operator : JC/MD
Sample : M4677-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

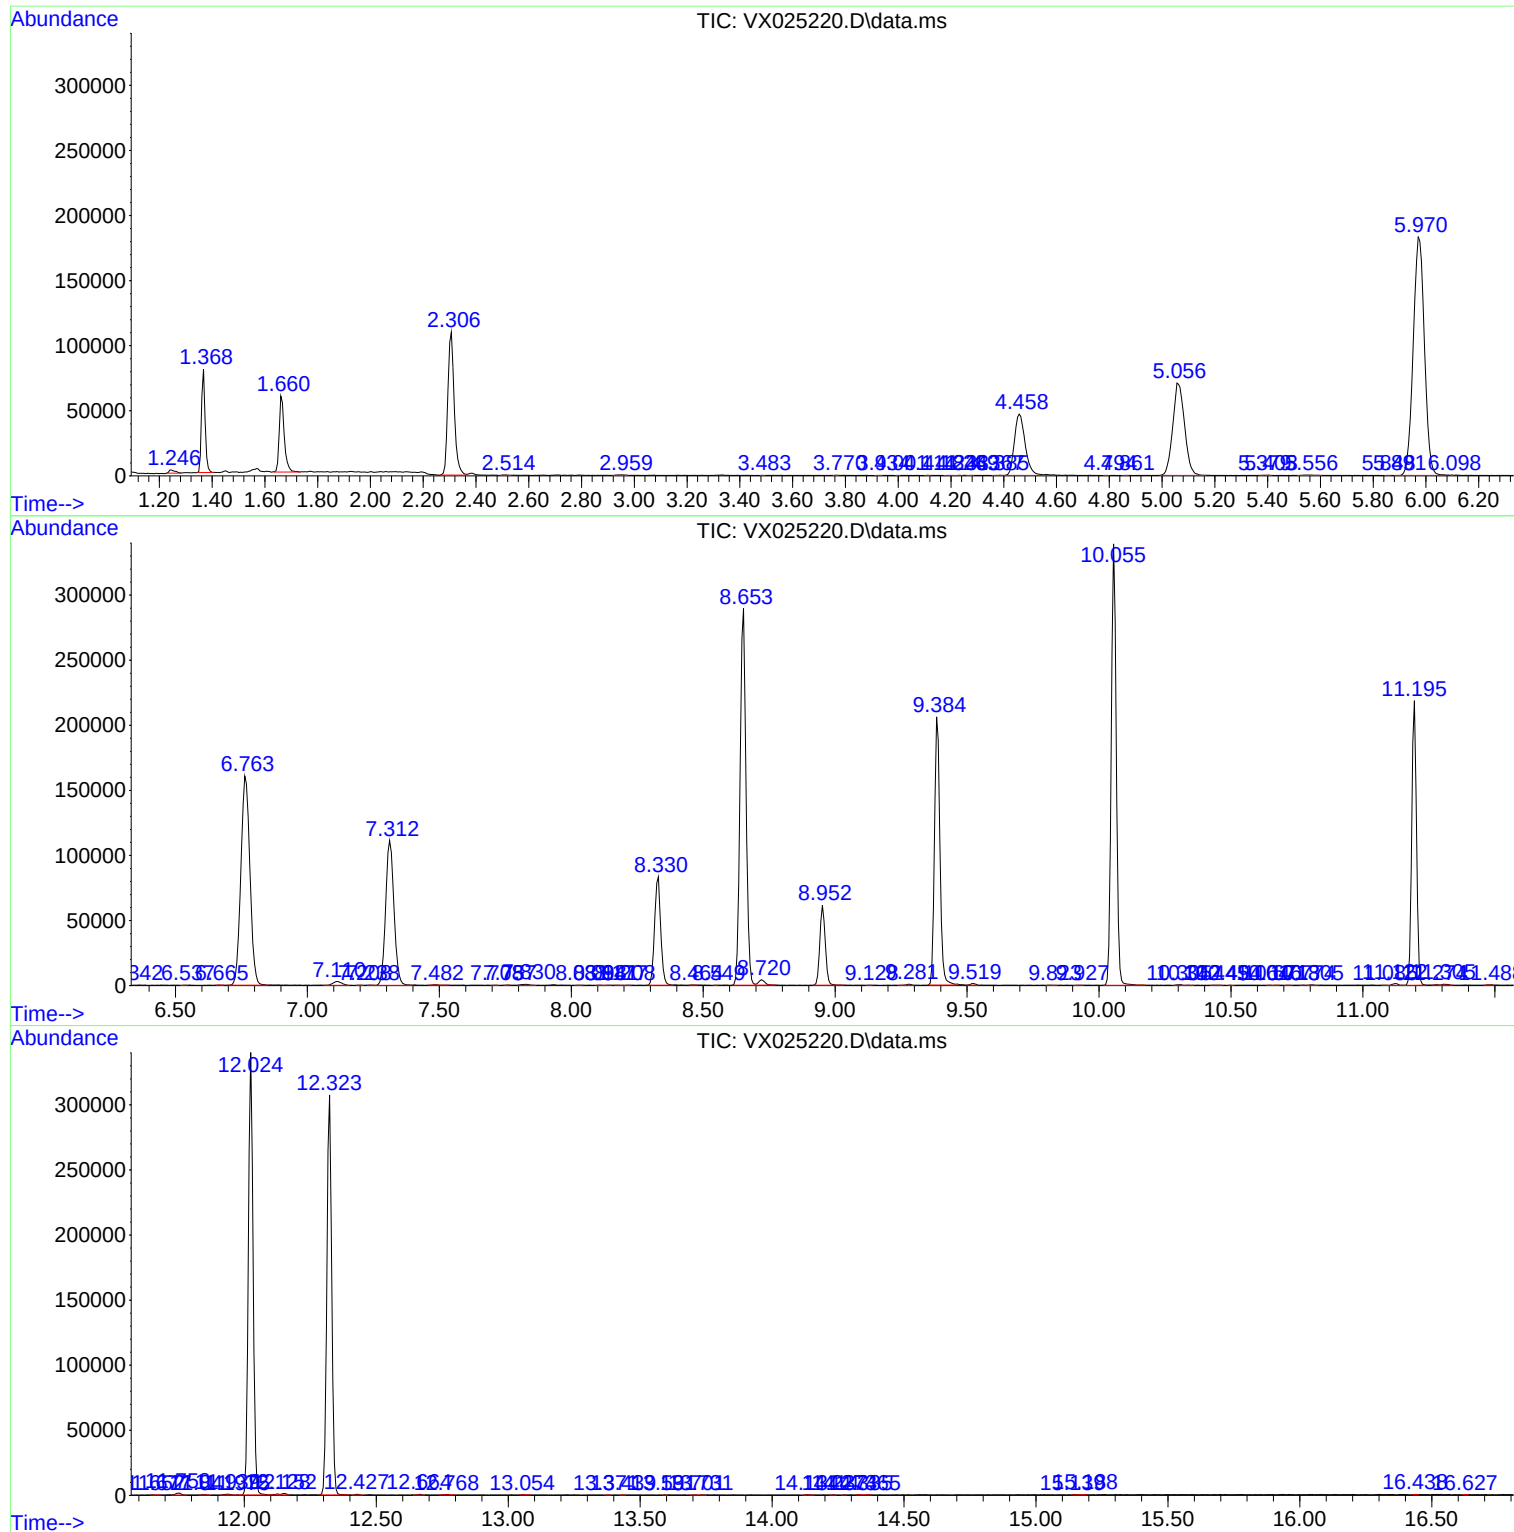

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025220.D
Acq On : 18 Nov 2021 19:34
Operator : JC/MD
Sample : M4677-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025220.D
Acq On : 18 Nov 2021 19:34
Operator : JC/MD
Sample : M4677-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc