

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025221.D
 Acq On : 18 Nov 2021 19:57
 Operator : JC/MD
 Sample : M4677-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	31	rBV2	2671	4712	0.19%	0.063%
2	1.368	42	46	56	rVB	79785	77240	3.15%	1.031%
3	1.666	91	95	104	rVB	55950	77831	3.18%	1.039%
4	2.306	194	200	211	rBV	112438	179934	7.34%	2.401%
5	2.782	277	278	280	rBV2	256	204	0.01%	0.003%
6	2.941	298	304	312	rBV3	1017	2244	0.09%	0.030%
7	3.093	323	329	339	rVB	6277	11604	0.47%	0.155%
8	3.276	358	359	362	rBV	165	151	0.01%	0.002%
9	3.501	395	396	399	rBV2	135	156	0.01%	0.002%
10	3.989	475	476	479	rVB2	145	127	0.01%	0.002%
11	4.123	496	498	501	rBV2	131	172	0.01%	0.002%
12	4.215	511	513	516	rVB	204	137	0.01%	0.002%
13	4.251	518	519	521	rBV2	130	140	0.01%	0.002%
14	4.288	524	525	530	rVV2	177	189	0.01%	0.003%
15	4.489	544	558	585	rVB2	140625	470473	19.20%	6.278%
16	4.867	616	620	621	rBV	136	164	0.01%	0.002%
17	5.062	640	652	670	rVV	69593	215873	8.81%	2.881%
18	5.324	693	695	698	rVV	121	147	0.01%	0.002%
19	5.367	700	702	703	rBV	279	213	0.01%	0.003%
20	5.379	703	704	707	rBV3	300	393	0.02%	0.005%
21	5.562	729	734	739	rVB2	415	862	0.04%	0.012%
22	5.629	742	745	747	rBV2	225	232	0.01%	0.003%
23	5.855	779	782	784	rVB2	129	153	0.01%	0.002%
24	5.970	789	801	816	rBV2	179970	535020	21.84%	7.139%
25	6.550	893	896	898	rBV2	181	199	0.01%	0.003%
26	6.598	898	904	909	rVV2	107	235	0.01%	0.003%
27	6.672	914	916	917	rBV	234	136	0.01%	0.002%
28	6.763	921	931	944	rBV	161265	380355	15.52%	5.075%
29	6.989	966	968	972	rVB	173	162	0.01%	0.002%
30	7.129	981	991	1009	rBV2	124338	276020	11.27%	3.683%
31	7.312	1013	1021	1032	rBV	113583	243583	9.94%	3.250%
32	7.476	1046	1048	1050	rBV2	483	494	0.02%	0.007%
33	7.751	1091	1093	1096	rBV2	142	136	0.01%	0.002%
34	7.781	1096	1098	1099	rBV	130	137	0.01%	0.002%
35	7.934	1119	1123	1127	rBV2	395	761	0.03%	0.010%
36	8.220	1168	1170	1171	rBV2	204	130	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025221.D
 Acq On : 18 Nov 2021 19:57
 Operator : JC/MD
 Sample : M4677-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	8.281	1176	1180	1181	rBV2	344	360	0.01%	0.005%
38	8.330	1181	1188	1196	rVB	80376	133268	5.44%	1.778%
39	8.470	1209	1211	1214	rVV	414	381	0.02%	0.005%
40	8.561	1222	1226	1228	rVV2	131	168	0.01%	0.002%
41	8.604	1228	1233	1234	rVV3	527	753	0.03%	0.010%
42	8.653	1234	1241	1248	rVV	290274	451335	18.42%	6.023%
43	8.720	1249	1252	1262	rVV	3794	6485	0.26%	0.087%
44	8.818	1265	1268	1271	rBV	163	161	0.01%	0.002%
45	8.860	1273	1275	1276	rVV	190	128	0.01%	0.002%
46	8.952	1284	1290	1301	rVV	63665	92614	3.78%	1.236%
47	9.104	1311	1315	1321	rVV2	309	435	0.02%	0.006%
48	9.275	1336	1343	1356	rBV	1677168	2450187	100.00%	32.695%
49	9.384	1356	1361	1379	rVB	203757	291760	11.91%	3.893%
50	9.537	1384	1386	1387	rVV	265	197	0.01%	0.003%
51	9.561	1387	1390	1396	rVV3	694	1034	0.04%	0.014%
52	9.622	1396	1400	1402	rVV3	608	778	0.03%	0.010%
53	9.720	1414	1416	1418	rVB	283	203	0.01%	0.003%
54	9.823	1428	1433	1434	rBV3	218	279	0.01%	0.004%
55	9.878	1440	1442	1443	rBV	161	154	0.01%	0.002%
56	10.055	1465	1471	1484	rBV	333934	451794	18.44%	6.029%
57	10.275	1505	1507	1508	rVB	323	161	0.01%	0.002%
58	10.305	1508	1512	1517	rBV3	656	1180	0.05%	0.016%
59	10.360	1518	1521	1525	rVV2	439	651	0.03%	0.009%
60	10.421	1527	1531	1533	rVB2	122	123	0.01%	0.002%
61	10.457	1533	1537	1541	rBV2	183	278	0.01%	0.004%
62	10.494	1541	1543	1546	rVB	188	199	0.01%	0.003%
63	10.598	1557	1560	1562	rVB2	220	242	0.01%	0.003%
64	10.732	1578	1582	1583	rBV2	134	177	0.01%	0.002%
65	10.774	1587	1589	1593	rBV3	436	457	0.02%	0.006%
66	10.854	1600	1602	1604	rBV2	345	302	0.01%	0.004%
67	10.957	1615	1619	1622	rVB3	213	339	0.01%	0.005%
68	11.122	1642	1646	1651	rVB3	1567	1963	0.08%	0.026%
69	11.195	1652	1658	1665	rBV	217426	277832	11.34%	3.707%
70	11.274	1669	1671	1673	rBV	329	252	0.01%	0.003%
71	11.457	1698	1701	1702	rBV3	247	317	0.01%	0.004%
72	11.482	1702	1705	1707	rVV3	721	816	0.03%	0.011%
73	11.549	1713	1716	1720	rVB2	229	320	0.01%	0.004%
74	11.616	1725	1727	1728	rBV	284	263	0.01%	0.004%
75	11.677	1736	1737	1740	rBV	152	134	0.01%	0.002%
76	11.719	1740	1744	1745	rVV2	223	282	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025221.D
 Acq On : 18 Nov 2021 19:57
 Operator : JC/MD
 Sample : M4677-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Title : VOC Analysis

77	11.756	1745	1750	1753	rVV3	1511	2330	0.10%	0.031%
78	11.841	1762	1764	1767	rVB	334	228	0.01%	0.003%
79	11.933	1776	1779	1783	rVB4	630	922	0.04%	0.012%
80	11.975	1783	1786	1789	rBV	152	294	0.01%	0.004%
81	12.024	1789	1794	1802	rBV	362989	433125	17.68%	5.780%
82	12.152	1813	1815	1821	rVB2	988	1011	0.04%	0.013%
83	12.225	1824	1827	1828	rBV	200	257	0.01%	0.003%
84	12.323	1836	1843	1852	rBV	325456	402836	16.44%	5.375%
85	12.421	1857	1859	1865	rVB3	541	654	0.03%	0.009%
86	12.634	1890	1894	1895	rVB2	231	233	0.01%	0.003%
87	12.652	1895	1897	1898	rBV	200	141	0.01%	0.002%
88	12.756	1912	1914	1919	rVV2	257	315	0.01%	0.004%
89	12.981	1950	1951	1954	rBV2	174	158	0.01%	0.002%
90	13.055	1961	1963	1964	rBV	157	149	0.01%	0.002%
91	13.164	1977	1981	1983	rBV	137	128	0.01%	0.002%
92	13.237	1989	1993	1995	rBV2	101	144	0.01%	0.002%
93	13.640	2055	2059	2061	rBV	170	231	0.01%	0.003%
94	13.945	2107	2109	2112	rVB2	181	167	0.01%	0.002%
95	14.097	2133	2134	2137	rBV	206	170	0.01%	0.002%
96	14.231	2152	2156	2157	rBV	99	129	0.01%	0.002%
97	14.268	2159	2162	2165	rBV2	206	251	0.01%	0.003%
98	14.304	2166	2168	2171	rVB2	212	194	0.01%	0.003%
99	14.524	2202	2204	2205	rBV	195	136	0.01%	0.002%
100	15.390	2344	2346	2349	rBV2	289	349	0.01%	0.005%




Sum of corrected areas: 7494033

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025221.D
Acq On : 18 Nov 2021 19:57
Operator : JC/MD
Sample : M4677-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

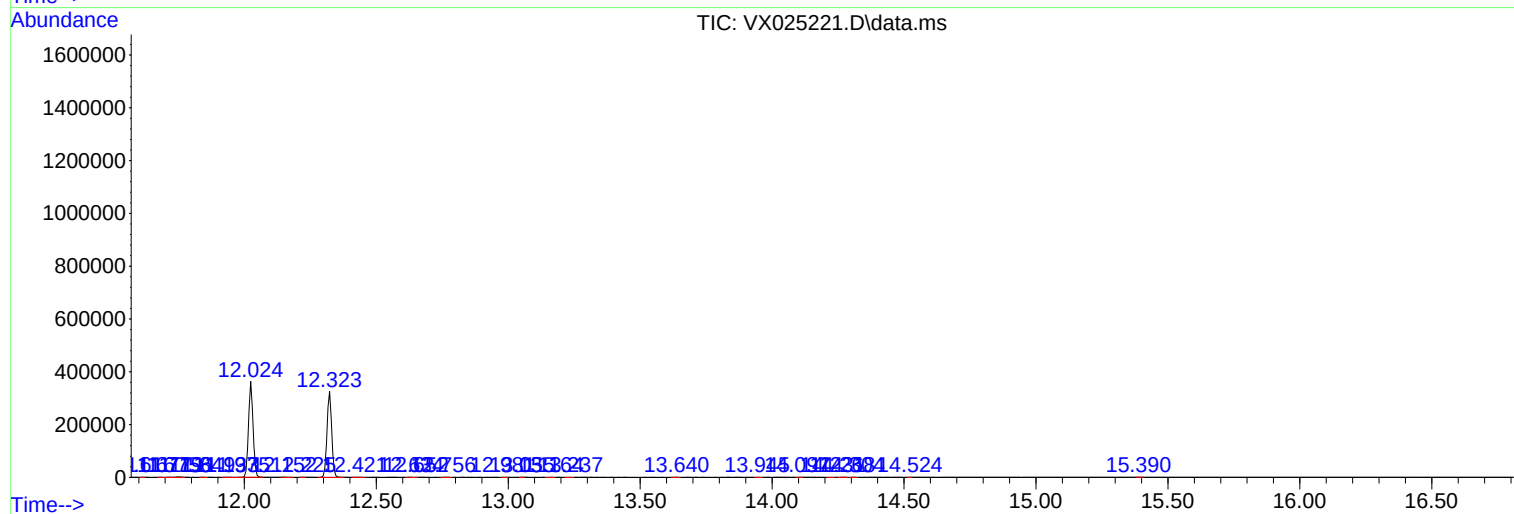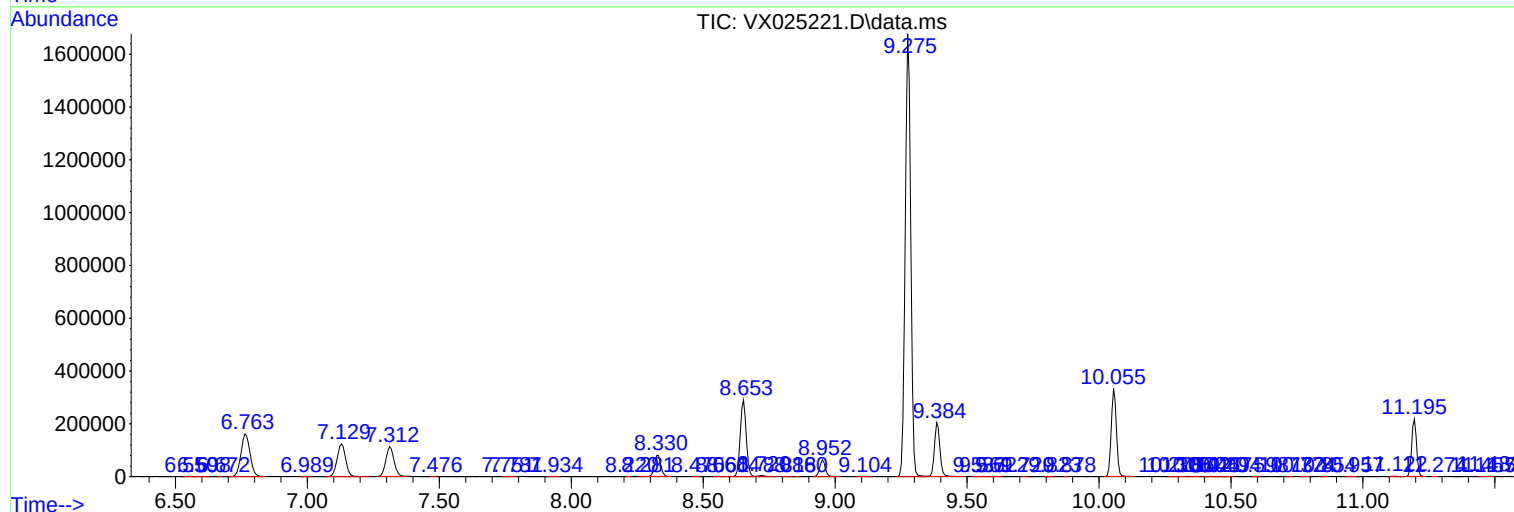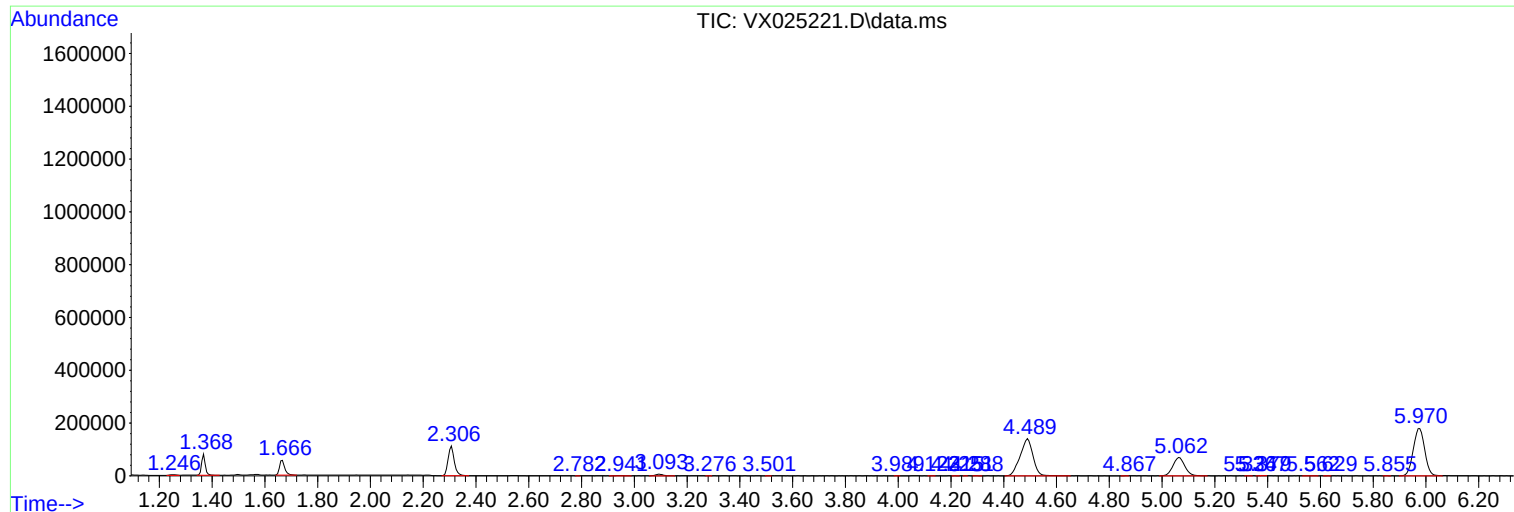

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025221.D
Acq On : 18 Nov 2021 19:57
Operator : JC/MD
Sample : M4677-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025221.D
Acq On : 18 Nov 2021 19:57
Operator : JC/MD
Sample : M4677-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc