

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025222.D
 Acq On : 18 Nov 2021 20:20
 Operator : JC/MD
 Sample : M4677-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	23	26	32	rBV4	2657	4684	0.18%	0.061%
2	1.367	42	46	53	rVB	81094	77393	3.02%	1.014%
3	1.666	91	95	103	rVB	58944	77644	3.03%	1.017%
4	2.306	194	200	210	rVB	111759	177911	6.94%	2.331%
5	2.544	236	239	244	rVB4	522	828	0.03%	0.011%
6	2.702	263	265	266	rBV2	250	211	0.01%	0.003%
7	2.788	277	279	285	rBV4	325	435	0.02%	0.006%
8	2.885	292	295	298	rVB2	177	230	0.01%	0.003%
9	2.946	304	305	308	rVB	308	204	0.01%	0.003%
10	3.019	316	317	320	rVB	168	117	0.00%	0.002%
11	3.093	323	329	338	rVB	5768	11481	0.45%	0.150%
12	3.288	360	361	364	rBV2	129	161	0.01%	0.002%
13	3.404	376	380	382	rBV	123	183	0.01%	0.002%
14	3.690	426	427	432	rVB	226	259	0.01%	0.003%
15	3.733	432	434	437	rBV2	178	188	0.01%	0.002%
16	4.324	529	531	535	rVB2	128	161	0.01%	0.002%
17	4.385	538	541	544	rBV2	131	165	0.01%	0.002%
18	4.489	544	558	574	rBV2	143398	472697	18.45%	6.194%
19	4.922	627	629	634	rVB	148	181	0.01%	0.002%
20	4.964	634	636	638	rBV	106	129	0.01%	0.002%
21	5.062	640	652	666	rBV	69889	218444	8.53%	2.863%
22	5.287	687	689	693	rBV2	126	159	0.01%	0.002%
23	5.324	693	695	698	rVV2	145	206	0.01%	0.003%
24	5.391	700	706	710	rVB3	395	681	0.03%	0.009%
25	5.550	728	732	733	rBV2	299	306	0.01%	0.004%
26	5.970	789	801	816	rBV2	181855	539043	21.04%	7.064%
27	6.208	837	840	842	rVB2	123	152	0.01%	0.002%
28	6.244	845	846	850	rVV2	191	185	0.01%	0.002%
29	6.324	857	859	863	rBV2	135	218	0.01%	0.003%
30	6.763	922	931	942	rBV	157735	379302	14.80%	4.970%
31	7.128	982	991	1010	rBV	131109	282541	11.03%	3.702%
32	7.311	1012	1021	1032	rBV	109695	244643	9.55%	3.206%
33	7.476	1045	1048	1053	rBV3	290	522	0.02%	0.007%
34	7.787	1098	1099	1100	rBV	206	119	0.00%	0.002%
35	7.805	1100	1102	1108	rVB3	321	451	0.02%	0.006%
36	7.915	1118	1120	1121	rBV	255	190	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025222.D
 Acq On : 18 Nov 2021 20:20
 Operator : JC/MD
 Sample : M4677-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	8.000	1132	1134	1138	rBV2	166	231	0.01%	0.003%
38	8.031	1138	1139	1142	rVV	150	122	0.00%	0.002%
39	8.201	1162	1167	1170	rBV2	96	192	0.01%	0.003%
40	8.329	1181	1188	1200	rVB	82983	135751	5.30%	1.779%
41	8.415	1200	1202	1203	rVB2	204	128	0.00%	0.002%
42	8.433	1203	1205	1208	rVB2	272	276	0.01%	0.004%
43	8.470	1208	1211	1212	rBV2	273	277	0.01%	0.004%
44	8.592	1229	1231	1234	rBV2	291	394	0.02%	0.005%
45	8.653	1234	1241	1249	rVV	294261	451441	17.62%	5.916%
46	8.720	1249	1252	1258	rVB	3581	5495	0.21%	0.072%
47	8.951	1284	1290	1301	rVB	64701	92801	3.62%	1.216%
48	9.098	1313	1314	1318	rVB	175	170	0.01%	0.002%
49	9.274	1336	1343	1356	rBV	1741389	2562002	100.00%	33.573%
50	9.384	1356	1361	1379	rVV	208678	302867	11.82%	3.969%
51	9.500	1379	1380	1383	rVV2	542	468	0.02%	0.006%
52	9.561	1387	1390	1396	rVB3	450	739	0.03%	0.010%
53	9.616	1396	1399	1404	rBV	270	418	0.02%	0.005%
54	9.908	1445	1447	1449	rBV	167	129	0.01%	0.002%
55	10.006	1462	1463	1465	rBV2	191	128	0.00%	0.002%
56	10.055	1465	1471	1485	rBV	333755	453977	17.72%	5.949%
57	10.207	1494	1496	1498	rBV	170	192	0.01%	0.003%
58	10.299	1509	1511	1517	rVV	725	898	0.04%	0.012%
59	10.366	1519	1522	1525	rBV3	323	397	0.02%	0.005%
60	10.402	1527	1528	1533	rBV	181	197	0.01%	0.003%
61	10.469	1537	1539	1542	rVB2	176	164	0.01%	0.002%
62	10.567	1554	1555	1557	rVV	281	147	0.01%	0.002%
63	10.640	1565	1567	1570	rVB	178	144	0.01%	0.002%
64	10.927	1613	1614	1619	rVB2	137	138	0.01%	0.002%
65	11.018	1628	1629	1632	rBV2	219	215	0.01%	0.003%
66	11.122	1642	1646	1651	rVB	1611	1993	0.08%	0.026%
67	11.195	1652	1658	1668	rBV	219346	279018	10.89%	3.656%
68	11.274	1670	1671	1675	rBV3	437	525	0.02%	0.007%
69	11.390	1685	1690	1695	rBV3	248	461	0.02%	0.006%
70	11.481	1702	1705	1711	rVB3	769	1019	0.04%	0.013%
71	11.725	1742	1745	1746	rBV	247	272	0.01%	0.004%
72	11.750	1746	1749	1755	rVB5	1469	2066	0.08%	0.027%
73	11.847	1762	1765	1767	rBV2	245	280	0.01%	0.004%
74	11.890	1770	1772	1775	rBV	103	125	0.00%	0.002%
75	11.933	1776	1779	1782	rVB3	701	871	0.03%	0.011%
76	11.969	1782	1785	1786	rBV	122	154	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025222.D
 Acq On : 18 Nov 2021 20:20
 Operator : JC/MD
 Sample : M4677-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1801	rBV	353979	434373	16.95%	5.692%
78	12.128	1809	1811	1812	rBV	416	260	0.01%	0.003%
79	12.182	1819	1820	1824	rVB2	175	143	0.01%	0.002%
80	12.323	1837	1843	1851	rBV	314975	401900	15.69%	5.267%
81	12.384	1851	1853	1856	rVB3	360	277	0.01%	0.004%
82	12.426	1856	1860	1865	rBV3	556	856	0.03%	0.011%
83	12.658	1897	1898	1901	rBV2	230	280	0.01%	0.004%
84	12.847	1928	1929	1931	rVB	246	152	0.01%	0.002%
85	13.054	1961	1963	1967	rVB	295	266	0.01%	0.003%
86	13.091	1967	1969	1971	rBV	92	117	0.00%	0.002%
87	13.420	2021	2023	2026	rVB	154	116	0.00%	0.002%
88	13.481	2031	2033	2035	rVB2	160	128	0.00%	0.002%
89	13.615	2054	2055	2058	rBV	192	186	0.01%	0.002%
90	13.737	2074	2075	2078	rVB	266	190	0.01%	0.002%
91	13.774	2078	2081	2084	rBV2	200	352	0.01%	0.005%
92	14.127	2136	2139	2144	rBV3	243	447	0.02%	0.006%
93	14.249	2157	2159	2160	rBV	164	142	0.01%	0.002%
94	14.450	2190	2192	2193	rVB	178	117	0.00%	0.002%
95	14.469	2193	2195	2196	rBV2	134	119	0.00%	0.002%
96	14.523	2202	2204	2205	rBV2	155	135	0.01%	0.002%
97	14.633	2219	2222	2224	rBV	255	262	0.01%	0.003%
98	14.883	2261	2263	2267	rVB3	192	195	0.01%	0.003%
99	15.328	2334	2336	2338	rVB2	361	224	0.01%	0.003%
100	16.566	2538	2539	2541	rBV	281	174	0.01%	0.002%




Sum of corrected areas: 7631117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025222.D
Acq On : 18 Nov 2021 20:20
Operator : JC/MD
Sample : M4677-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

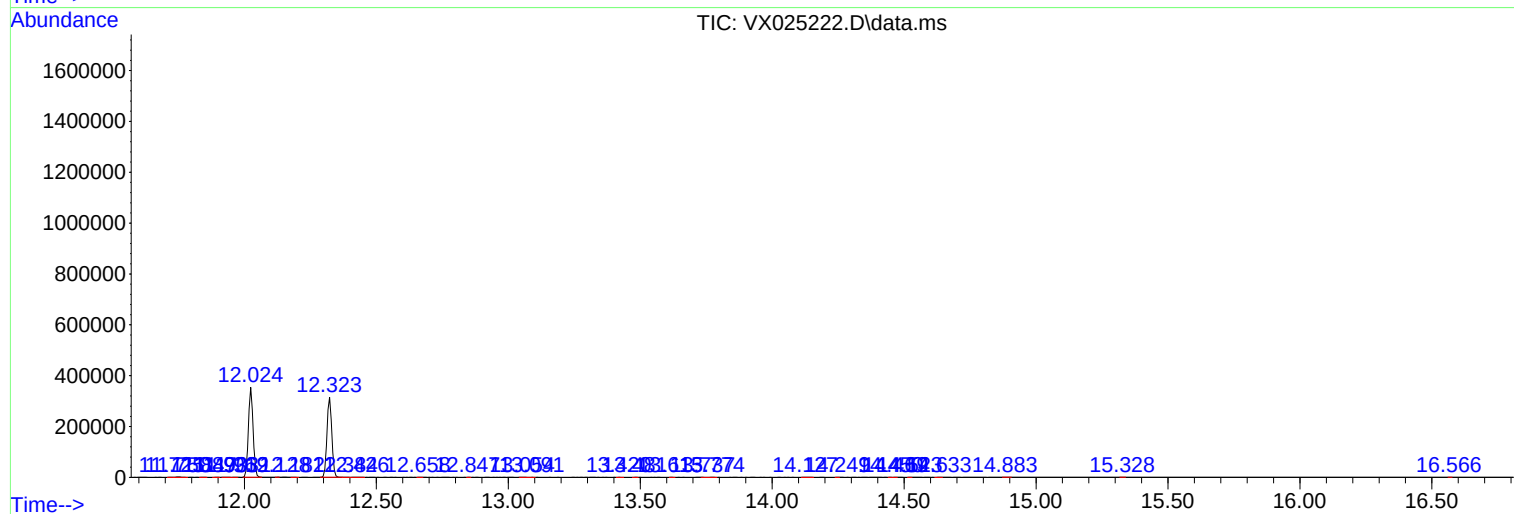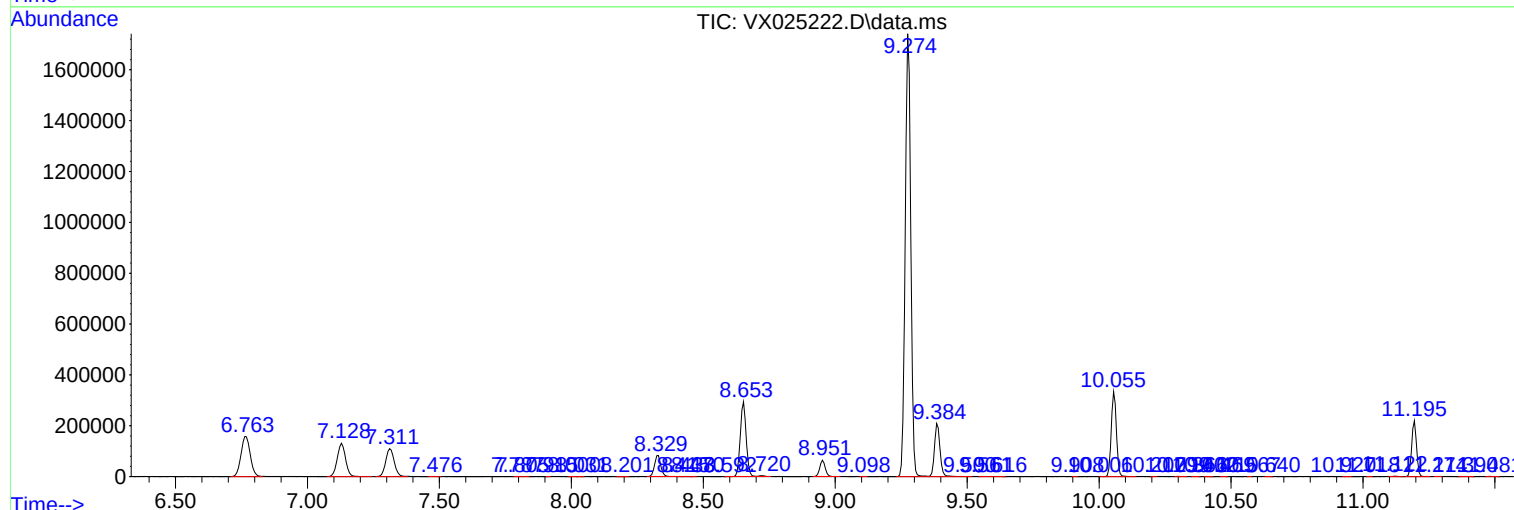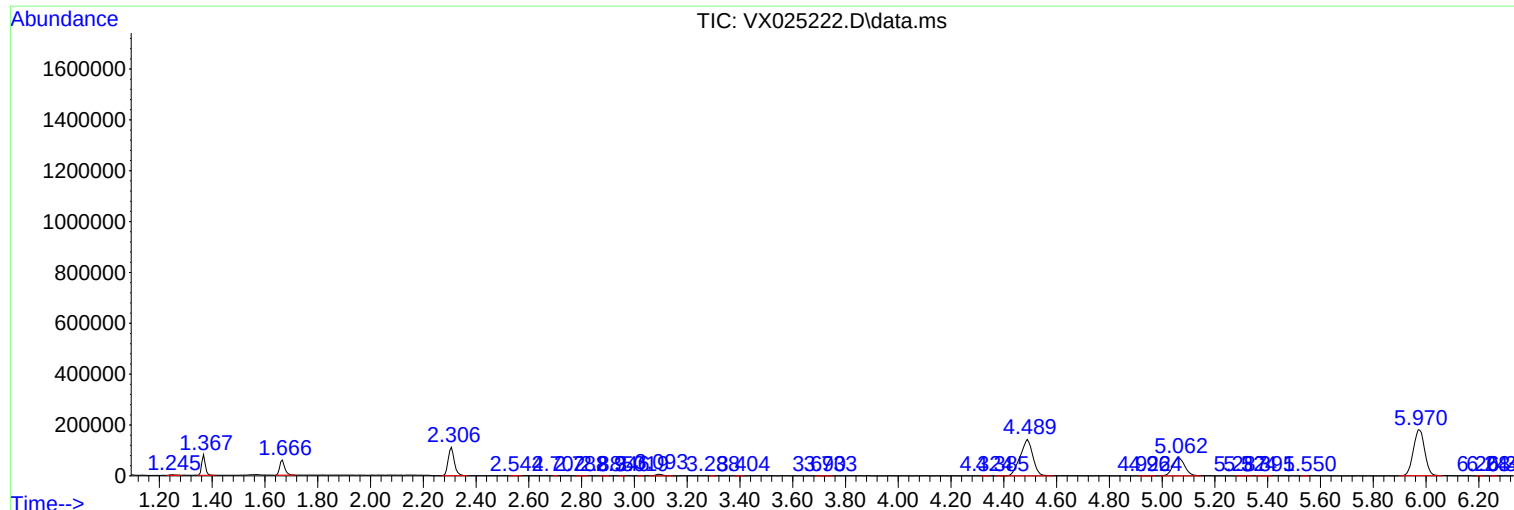

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025222.D
Acq On : 18 Nov 2021 20:20
Operator : JC/MD
Sample : M4677-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025222.D
Acq On : 18 Nov 2021 20:20
Operator : JC/MD
Sample : M4677-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc