

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025224.D
 Acq On : 18 Nov 2021 21:07
 Operator : JC/MD
 Sample : M4677-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	52	rBV	79691	76076	14.15%	1.714%
2	1.495	65	67	70	rVB	4542	4405	0.82%	0.099%
3	1.666	90	95	105	rVB	57287	78140	14.54%	1.760%
4	2.306	193	200	211	rBV	109616	180352	33.55%	4.062%
5	2.459	224	225	226	rBV	281	132	0.02%	0.003%
6	2.623	251	252	256	rBV2	176	156	0.03%	0.004%
7	2.703	263	265	269	rBV2	309	406	0.08%	0.009%
8	2.946	297	305	315	rVB	4854	11063	2.06%	0.249%
9	3.123	329	334	341	rVB4	430	1030	0.19%	0.023%
10	3.337	368	369	371	rBV	162	118	0.02%	0.003%
11	3.391	377	378	381	rBV2	110	128	0.02%	0.003%
12	3.471	386	391	392	rBV2	163	193	0.04%	0.004%
13	3.617	406	415	421	rBV2	7853	18007	3.35%	0.406%
14	3.818	446	448	450	rVV	142	123	0.02%	0.003%
15	3.867	454	456	460	rVV2	201	155	0.03%	0.003%
16	4.129	497	499	500	rBV	118	127	0.02%	0.003%
17	4.379	538	540	543	rBV	185	144	0.03%	0.003%
18	4.458	543	553	567	rBV	47721	152657	28.40%	3.438%
19	4.873	618	621	623	rBV	179	213	0.04%	0.005%
20	5.062	640	652	667	rBV	69882	215894	40.16%	4.863%
21	5.501	721	724	725	rBV	132	144	0.03%	0.003%
22	5.562	728	734	735	rBV4	305	464	0.09%	0.010%
23	5.970	789	801	819	rVV2	181677	537565	100.00%	12.108%
24	6.245	844	846	848	rBV2	125	135	0.03%	0.003%
25	6.354	860	864	866	rBV2	405	548	0.10%	0.012%
26	6.464	877	882	885	rBV2	183	259	0.05%	0.006%
27	6.653	910	913	916	rBV2	104	155	0.03%	0.003%
28	6.763	922	931	948	rBV	153001	370259	68.88%	8.340%
29	6.879	948	950	953	rBV	197	169	0.03%	0.004%
30	6.958	960	963	965	rVB2	200	210	0.04%	0.005%
31	6.994	965	969	972	rBV	147	259	0.05%	0.006%
32	7.129	983	991	1000	rVV4	12545	28932	5.38%	0.652%
33	7.189	1000	1001	1004	rVV2	106	120	0.02%	0.003%
34	7.311	1013	1021	1034	rVB	111319	241585	44.94%	5.441%
35	7.476	1047	1048	1053	rVB4	298	366	0.07%	0.008%
36	7.671	1073	1080	1085	rBV3	871	1587	0.30%	0.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025224.D
 Acq On : 18 Nov 2021 21:07
 Operator : JC/MD
 Sample : M4677-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	7.769	1094	1096	1097	rBV2	144	114	0.02%	0.003%
38	7.805	1097	1102	1105	rBV2	286	430	0.08%	0.010%
39	7.933	1119	1123	1128	rBV4	496	771	0.14%	0.017%
40	8.104	1148	1151	1158	rBV	161	233	0.04%	0.005%
41	8.220	1168	1170	1171	rBV	178	147	0.03%	0.003%
42	8.262	1176	1177	1180	rBV	159	128	0.02%	0.003%
43	8.330	1181	1188	1198	rVV	81847	134263	24.98%	3.024%
44	8.470	1210	1211	1212	rBV	278	137	0.03%	0.003%
45	8.653	1234	1241	1248	rBV	283268	444698	82.72%	10.016%
46	8.720	1248	1252	1260	rVB	3918	6517	1.21%	0.147%
47	8.951	1284	1290	1304	rVB	61151	87013	16.19%	1.960%
48	9.061	1307	1308	1311	rBV2	164	157	0.03%	0.004%
49	9.110	1313	1316	1320	rBV2	131	140	0.03%	0.003%
50	9.274	1338	1343	1349	rBV2	14511	21330	3.97%	0.480%
51	9.384	1356	1361	1383	rVB	200892	292132	54.34%	6.580%
52	9.634	1399	1402	1405	rBV2	98	139	0.03%	0.003%
53	10.055	1466	1471	1484	rVB	319998	434172	80.77%	9.779%
54	10.201	1493	1495	1498	rVB2	257	274	0.05%	0.006%
55	10.238	1499	1501	1507	rVV	128	201	0.04%	0.005%
56	10.299	1507	1511	1517	rVV3	432	689	0.13%	0.016%
57	10.451	1532	1536	1538	rBV2	141	162	0.03%	0.004%
58	10.475	1538	1540	1544	rVB2	142	159	0.03%	0.004%
59	10.640	1563	1567	1570	rBV2	134	199	0.04%	0.004%
60	10.786	1589	1591	1595	rVB2	178	175	0.03%	0.004%
61	10.817	1595	1596	1598	rVB	215	153	0.03%	0.003%
62	10.835	1598	1599	1601	rBV2	195	186	0.03%	0.004%
63	10.878	1603	1606	1609	rVB	179	227	0.04%	0.005%
64	11.079	1638	1639	1642	rBV	129	133	0.02%	0.003%
65	11.122	1643	1646	1652	rVV2	1167	1581	0.29%	0.036%
66	11.195	1652	1658	1666	rVV	217774	274660	51.09%	6.186%
67	11.274	1669	1671	1675	rVV3	235	357	0.07%	0.008%
68	11.311	1675	1677	1684	rVB2	747	916	0.17%	0.021%
69	11.384	1684	1689	1692	rBV3	130	214	0.04%	0.005%
70	11.475	1700	1704	1707	rBV3	332	457	0.09%	0.010%
71	11.561	1715	1718	1719	rBV	149	144	0.03%	0.003%
72	11.689	1736	1739	1744	rVV2	99	180	0.03%	0.004%
73	11.750	1744	1749	1754	rVV3	1181	1752	0.33%	0.039%
74	11.805	1757	1758	1761	rBV2	192	219	0.04%	0.005%
75	11.847	1761	1765	1769	rVB2	274	417	0.08%	0.009%
76	11.939	1776	1780	1783	rVB2	744	814	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025224.D
 Acq On : 18 Nov 2021 21:07
 Operator : JC/MD
 Sample : M4677-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1801	rBV	331996	413288	76.88%	9.309%
78	12.152	1813	1815	1820	rVB2	1040	1049	0.20%	0.024%
79	12.262	1831	1833	1835	rVB	201	169	0.03%	0.004%
80	12.323	1837	1843	1857	rVV	309973	392684	73.05%	8.845%
81	12.432	1857	1861	1864	rVB	216	289	0.05%	0.007%
82	12.573	1881	1884	1885	rBV2	144	114	0.02%	0.003%
83	12.664	1895	1899	1901	rBV2	322	299	0.06%	0.007%
84	12.768	1912	1916	1918	rVB3	196	259	0.05%	0.006%
85	12.896	1934	1937	1939	rBV2	156	161	0.03%	0.004%
86	12.914	1939	1940	1942	rBV	176	123	0.02%	0.003%
87	12.963	1944	1948	1949	rBV	160	133	0.02%	0.003%
88	13.048	1961	1962	1964	rBV2	189	114	0.02%	0.003%
89	13.347	2009	2011	2014	rVV	191	115	0.02%	0.003%
90	13.554	2044	2045	2047	rBV	123	124	0.02%	0.003%
91	13.847	2091	2093	2095	rBV2	155	115	0.02%	0.003%
92	13.957	2106	2111	2113	rBV2	154	243	0.05%	0.005%
93	14.097	2133	2134	2136	rVB	186	119	0.02%	0.003%
94	14.133	2138	2140	2141	rBV	258	218	0.04%	0.005%
95	14.225	2152	2155	2157	rBV2	208	180	0.03%	0.004%
96	14.261	2157	2161	2163	rBV3	136	194	0.04%	0.004%
97	14.292	2163	2166	2168	rBV2	141	176	0.03%	0.004%
98	14.524	2201	2204	2205	rBV	243	227	0.04%	0.005%
99	14.578	2211	2213	2214	rVB	189	136	0.03%	0.003%
100	14.706	2233	2234	2237	rVB	266	176	0.03%	0.004%

Sum of corrected areas: 4439771




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025224.D
Acq On : 18 Nov 2021 21:07
Operator : JC/MD
Sample : M4677-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

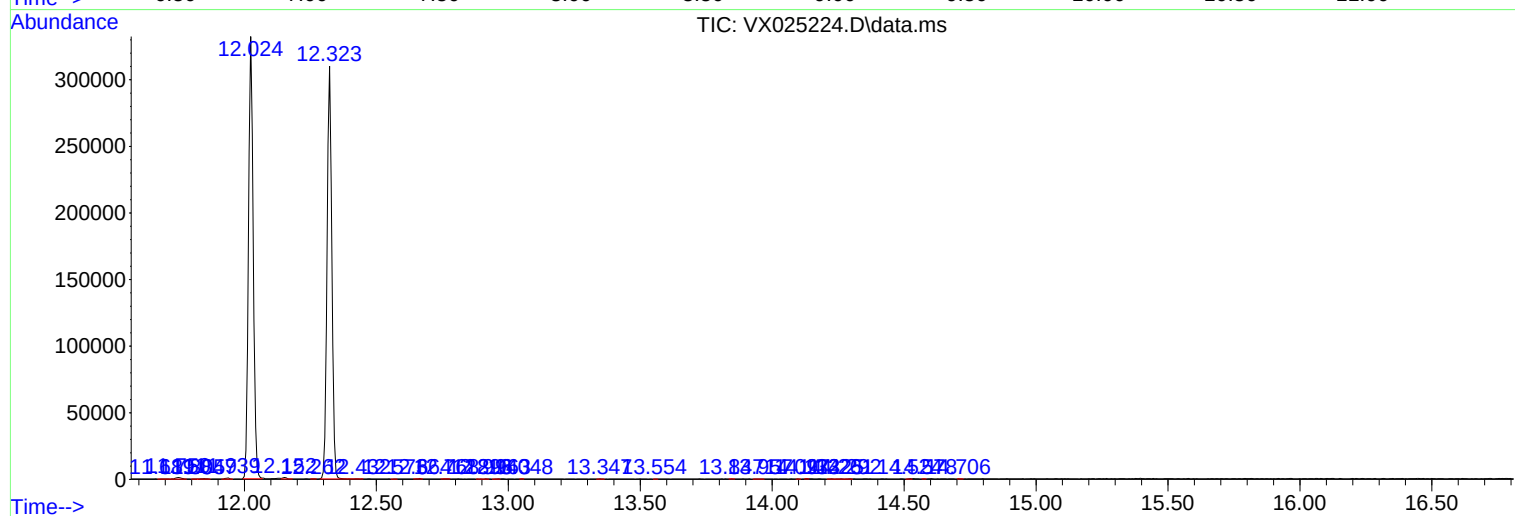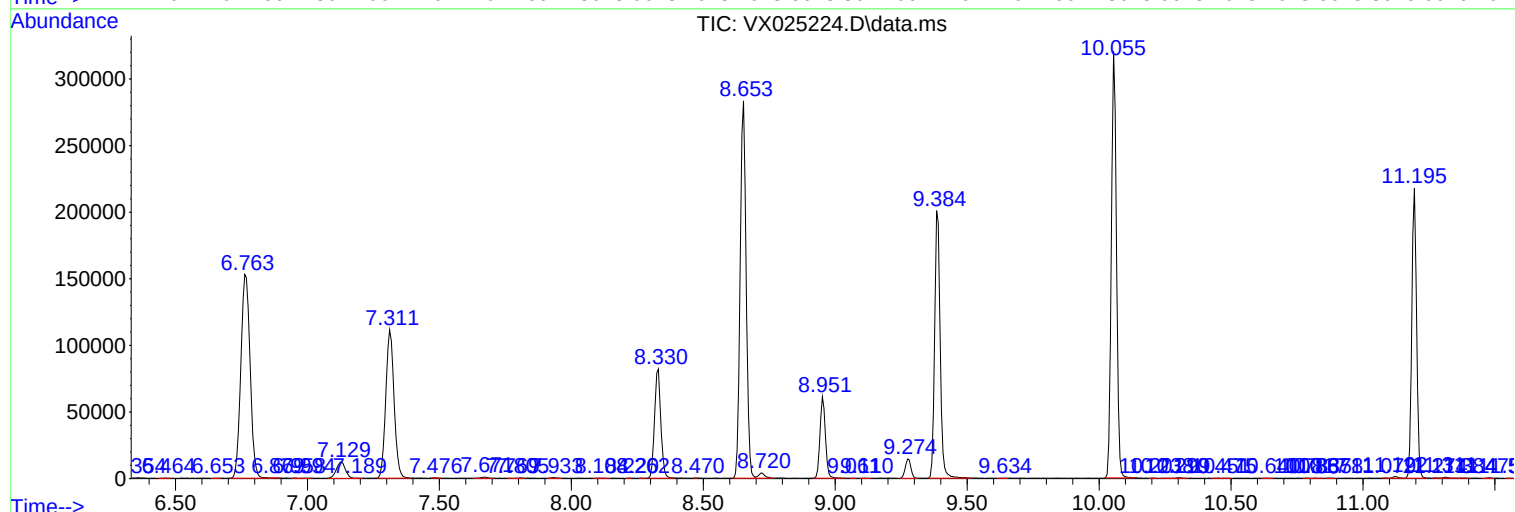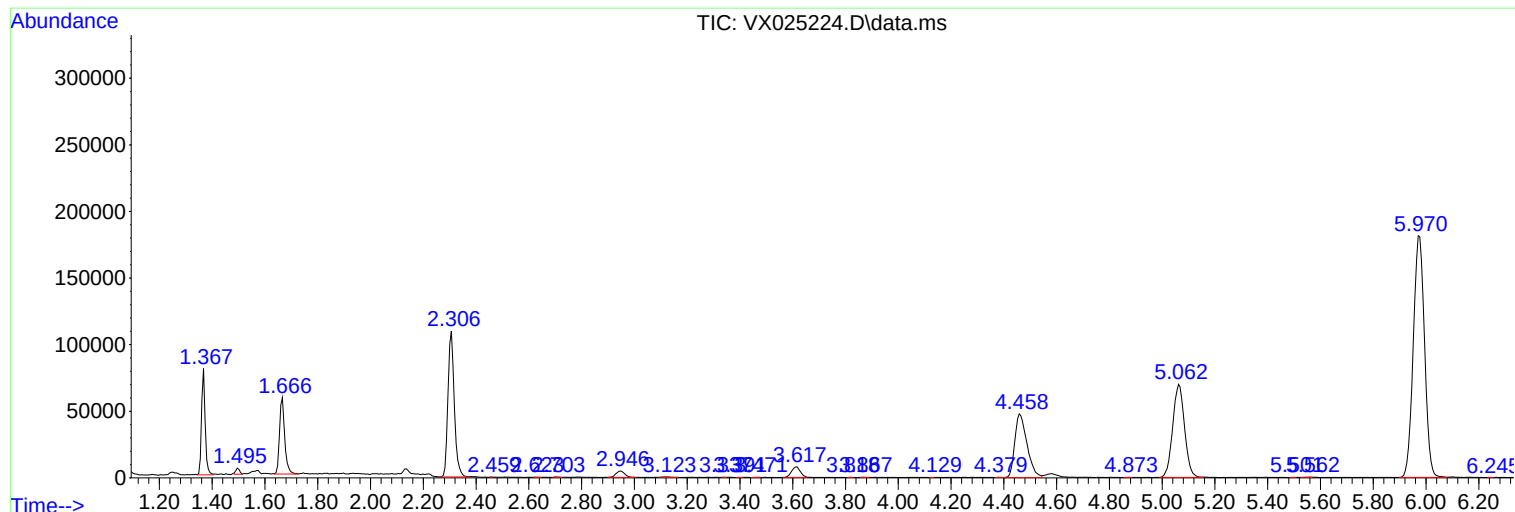

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025224.D
Acq On : 18 Nov 2021 21:07
Operator : JC/MD
Sample : M4677-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025224.D
Acq On : 18 Nov 2021 21:07
Operator : JC/MD
Sample : M4677-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc