

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025227.D
 Acq On : 18 Nov 2021 22:18
 Operator : JC/MD
 Sample : M4677-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV2	4034	7414	1.27%	0.169%
2	1.367	42	46	52	rBV	75961	72918	12.51%	1.663%
3	1.666	90	95	103	rBV	56622	75315	12.92%	1.717%
4	2.306	194	200	211	rVB	103623	169837	29.14%	3.873%
5	2.550	236	240	243	rVB3	313	494	0.08%	0.011%
6	2.581	243	245	246	rBV	180	155	0.03%	0.004%
7	2.788	277	279	282	rVB3	304	300	0.05%	0.007%
8	2.867	288	292	298	rVB3	624	1179	0.20%	0.027%
9	3.020	315	317	321	rVB	213	216	0.04%	0.005%
10	3.050	321	322	325	rBV	153	165	0.03%	0.004%
11	3.099	325	330	334	rVV3	224	350	0.06%	0.008%
12	3.331	365	368	370	rBV	124	164	0.03%	0.004%
13	3.404	377	380	383	rBV2	159	163	0.03%	0.004%
14	3.550	403	404	406	rBV	243	157	0.03%	0.004%
15	4.056	484	487	488	rVB	144	126	0.02%	0.003%
16	4.080	488	491	492	rBV2	103	126	0.02%	0.003%
17	4.202	508	511	513	rBV2	151	158	0.03%	0.004%
18	4.263	520	521	523	rVV3	212	198	0.03%	0.005%
19	4.312	523	529	532	rVV4	647	1314	0.23%	0.030%
20	4.458	544	553	570	rBV	43078	121857	20.91%	2.779%
21	4.647	581	584	585	rBV	191	140	0.02%	0.003%
22	5.062	639	652	668	rVV	67511	213153	36.57%	4.860%
23	5.178	668	671	672	rVB2	165	149	0.03%	0.003%
24	5.330	694	696	698	rBV	165	179	0.03%	0.004%
25	5.391	704	706	707	rBV2	171	182	0.03%	0.004%
26	5.452	714	716	717	rBV	258	198	0.03%	0.005%
27	5.556	728	733	734	rBV2	440	511	0.09%	0.012%
28	5.726	758	761	765	rVB2	136	205	0.04%	0.005%
29	5.891	786	788	790	rBV	152	168	0.03%	0.004%
30	5.970	790	801	818	rBV2	172499	517036	88.71%	11.789%
31	6.507	887	889	892	rBV2	159	183	0.03%	0.004%
32	6.641	908	911	914	rBV2	170	208	0.04%	0.005%
33	6.763	921	931	945	rBV	157883	374567	64.26%	8.541%
34	7.116	982	989	997	rBV8	3250	7689	1.32%	0.175%
35	7.214	1003	1005	1009	rVB	167	173	0.03%	0.004%
36	7.312	1012	1021	1036	rBV	110217	234262	40.19%	5.342%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025227.D
 Acq On : 18 Nov 2021 22:18
 Operator : JC/MD
 Sample : M4677-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	7.476	1045	1048	1050	rBV3	282	382	0.07%	0.009%
38	7.830	1096	1106	1112	rBV4	626	1506	0.26%	0.034%
39	7.927	1116	1122	1125	rBV2	352	540	0.09%	0.012%
40	7.952	1125	1126	1131	rVB	231	158	0.03%	0.004%
41	8.025	1137	1138	1142	rVB2	137	146	0.03%	0.003%
42	8.061	1142	1144	1146	rBV	151	143	0.02%	0.003%
43	8.330	1181	1188	1198	rVV	79628	128526	22.05%	2.931%
44	8.476	1209	1212	1213	rBV2	257	267	0.05%	0.006%
45	8.653	1234	1241	1248	rBV	276124	429625	73.71%	9.796%
46	8.720	1249	1252	1261	rVV2	3769	6328	1.09%	0.144%
47	8.823	1267	1269	1272	rBV	152	172	0.03%	0.004%
48	8.951	1285	1290	1299	rBV	56118	82748	14.20%	1.887%
49	9.073	1309	1310	1314	rBV2	156	182	0.03%	0.004%
50	9.275	1339	1343	1349	rBV2	4776	6305	1.08%	0.144%
51	9.384	1355	1361	1377	rBV	189140	274661	47.12%	6.263%
52	9.561	1388	1390	1392	rBV2	164	160	0.03%	0.004%
53	9.622	1398	1400	1404	rVB2	176	181	0.03%	0.004%
54	9.817	1430	1432	1436	rBV2	100	140	0.02%	0.003%
55	10.055	1465	1471	1488	rVV2	323519	582854	100.00%	13.290%
56	10.201	1491	1495	1499	rVV2	217	356	0.06%	0.008%
57	10.299	1508	1511	1517	rBV3	785	1188	0.20%	0.027%
58	10.488	1539	1542	1543	rVV	137	143	0.02%	0.003%
59	10.500	1543	1544	1547	rVV2	180	160	0.03%	0.004%
60	10.549	1549	1552	1555	rVB2	298	315	0.05%	0.007%
61	10.646	1567	1568	1571	rVB2	212	198	0.03%	0.005%
62	10.768	1587	1588	1592	rBV2	146	141	0.02%	0.003%
63	10.963	1617	1620	1625	rVB3	245	331	0.06%	0.008%
64	11.091	1639	1641	1643	rBV2	158	127	0.02%	0.003%
65	11.122	1643	1646	1650	rVB3	1229	1262	0.22%	0.029%
66	11.195	1652	1658	1669	rVV	211914	262879	45.10%	5.994%
67	11.311	1675	1677	1681	rVB2	831	1013	0.17%	0.023%
68	11.463	1697	1702	1703	rBV2	369	352	0.06%	0.008%
69	11.482	1703	1705	1708	rVV2	151	127	0.02%	0.003%
70	11.542	1714	1715	1719	rBV2	159	222	0.04%	0.005%
71	11.616	1722	1727	1730	rBV3	606	891	0.15%	0.020%
72	11.677	1735	1737	1742	rVB2	116	170	0.03%	0.004%
73	11.750	1745	1749	1755	rVB3	1275	1416	0.24%	0.032%
74	11.853	1759	1766	1768	rVB3	191	386	0.07%	0.009%
75	11.890	1768	1772	1774	rBV2	163	192	0.03%	0.004%
76	11.933	1774	1779	1782	rBV3	527	695	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025227.D
 Acq On : 18 Nov 2021 22:18
 Operator : JC/MD
 Sample : M4677-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 H0AB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1807	rVB	324518	414961	71.19%	9.462%
78	12.122	1807	1810	1813	rBV3	519	672	0.12%	0.015%
79	12.250	1828	1831	1835	rVB3	245	310	0.05%	0.007%
80	12.323	1838	1843	1852	rVB	305914	376170	64.54%	8.577%
81	12.433	1859	1861	1864	rVB2	298	220	0.04%	0.005%
82	12.500	1871	1872	1876	rVB2	181	137	0.02%	0.003%
83	12.548	1876	1880	1881	rBV2	149	148	0.03%	0.003%
84	12.701	1901	1905	1907	rBV	222	231	0.04%	0.005%
85	12.762	1911	1915	1916	rBV	204	277	0.05%	0.006%
86	13.048	1959	1962	1966	rVB2	122	151	0.03%	0.003%
87	13.475	2029	2032	2034	rBV2	113	168	0.03%	0.004%
88	13.780	2078	2082	2087	rVB2	516	844	0.14%	0.019%
89	13.829	2087	2090	2091	rBV	128	152	0.03%	0.003%
90	13.877	2094	2098	2099	rBV	183	199	0.03%	0.005%
91	14.133	2135	2140	2142	rVB2	250	298	0.05%	0.007%
92	14.213	2151	2153	2156	rBV3	116	144	0.02%	0.003%
93	14.511	2200	2202	2205	rVB	214	185	0.03%	0.004%
94	14.621	2217	2220	2222	rBV2	208	303	0.05%	0.007%
95	14.859	2258	2259	2262	rBV2	245	161	0.03%	0.004%
96	15.072	2292	2294	2295	rBV2	168	132	0.02%	0.003%
97	15.176	2309	2311	2312	rBV	199	130	0.02%	0.003%
98	15.487	2360	2362	2363	rBV	296	215	0.04%	0.005%
99	16.200	2477	2479	2480	rVB2	222	138	0.02%	0.003%
100	16.767	2570	2572	2573	rBV	264	144	0.02%	0.003%

Sum of corrected areas: 4385687




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025227.D
Acq On : 18 Nov 2021 22:18
Operator : JC/MD
Sample : M4677-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

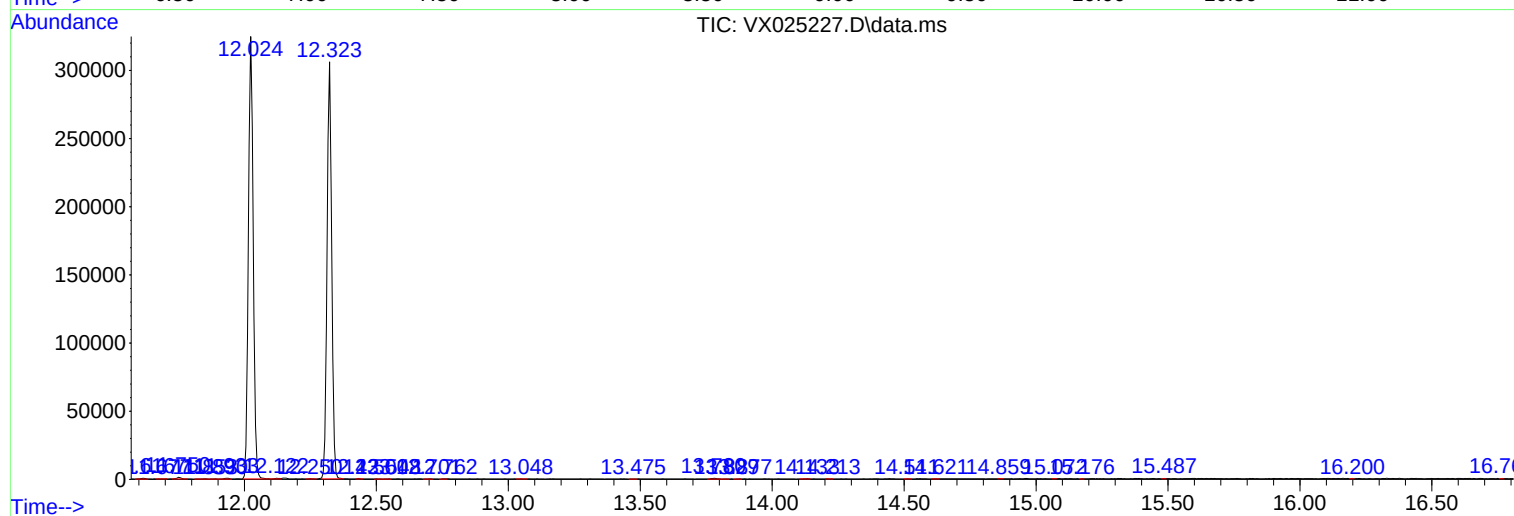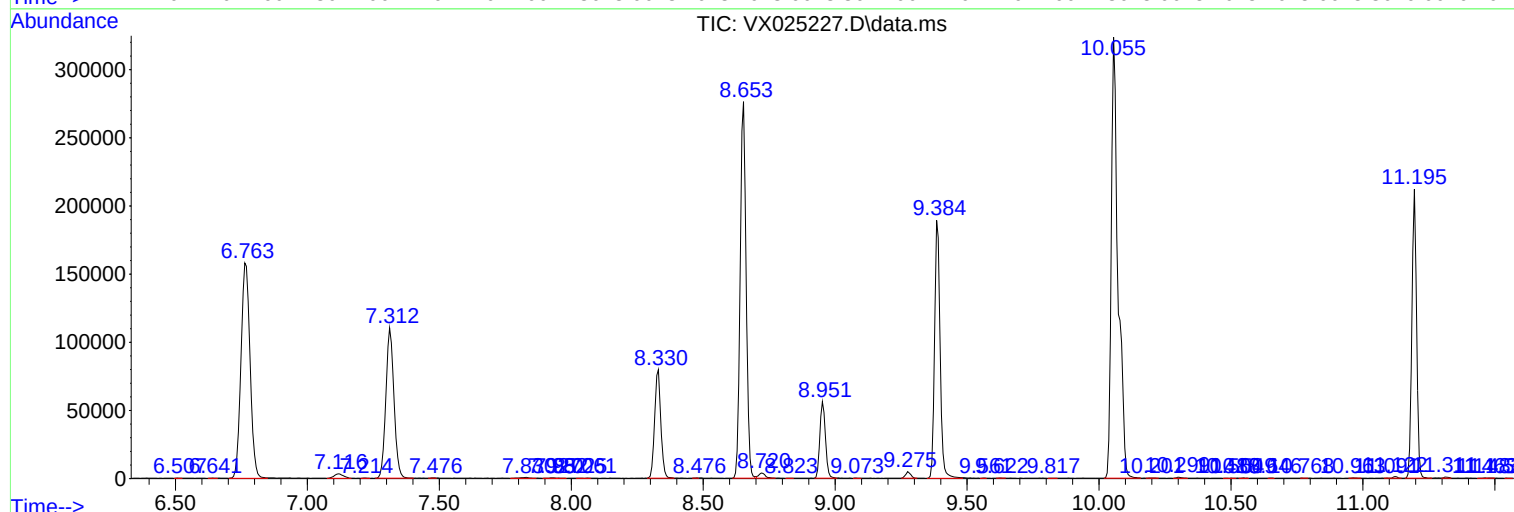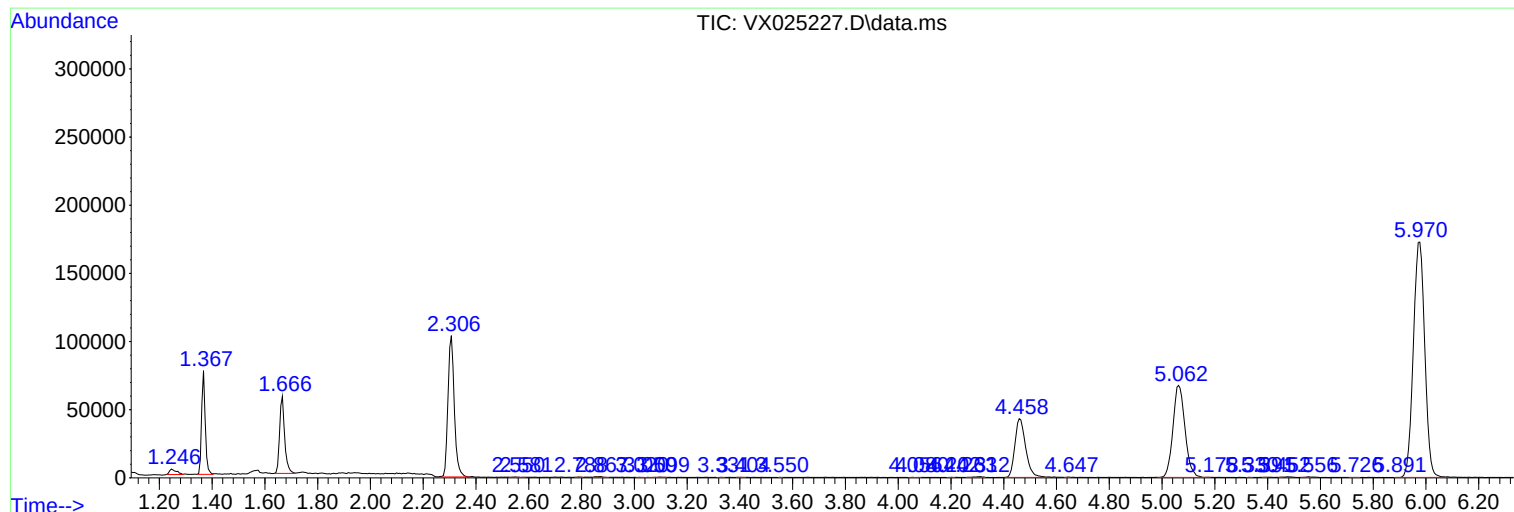

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025227.D
Acq On : 18 Nov 2021 22:18
Operator : JC/MD
Sample : M4677-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025227.D
Acq On : 18 Nov 2021 22:18
Operator : JC/MD
Sample : M4677-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
H0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc