

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025233.D
 Acq On : 19 Nov 2021 12:41
 Operator : JC/MD
 Sample : VX1119WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	53	rBV	91285	88929	16.59%	2.003%
2	1.666	91	95	105	rVB	61138	83993	15.67%	1.892%
3	2.306	193	200	210	rBV	126521	199544	37.22%	4.495%
4	2.532	229	237	244	rBV4	594	1508	0.28%	0.034%
5	2.782	274	278	283	rVB4	980	1726	0.32%	0.039%
6	2.940	297	304	315	rBV	3086	7018	1.31%	0.158%
7	3.093	328	329	333	rBV2	111	163	0.03%	0.004%
8	3.239	352	353	355	rBV	222	126	0.02%	0.003%
9	3.257	355	356	359	rVV	145	108	0.02%	0.002%
10	3.355	371	372	375	rBV2	104	103	0.02%	0.002%
11	3.513	396	398	399	rBV	146	114	0.02%	0.003%
12	3.788	442	443	447	rVB2	145	104	0.02%	0.002%
13	4.312	526	529	531	rBV	161	189	0.04%	0.004%
14	4.452	543	552	565	rBV2	42169	117961	22.01%	2.657%
15	5.062	639	652	668	rBV	66961	209607	39.10%	4.722%
16	5.214	675	677	678	rBV	163	148	0.03%	0.003%
17	5.336	695	697	701	rVB2	142	130	0.02%	0.003%
18	5.373	701	703	705	rBV2	258	292	0.05%	0.007%
19	5.544	728	731	732	rBV	256	280	0.05%	0.006%
20	5.867	780	784	789	rBV2	191	226	0.04%	0.005%
21	5.970	789	801	818	rBV2	182018	536055	100.00%	12.076%
22	6.245	844	846	848	rBV2	110	115	0.02%	0.003%
23	6.269	848	850	853	rBV	90	120	0.02%	0.003%
24	6.367	864	866	869	rVB2	88	101	0.02%	0.002%
25	6.434	875	877	878	rBV	151	109	0.02%	0.002%
26	6.464	878	882	885	rVV3	115	144	0.03%	0.003%
27	6.763	920	931	943	rBV	168379	397336	74.12%	8.951%
28	7.007	970	971	975	rBV2	101	139	0.03%	0.003%
29	7.110	981	988	995	rVB3	3121	6912	1.29%	0.156%
30	7.305	1011	1020	1034	rVV	108709	238469	44.49%	5.372%
31	7.403	1034	1036	1040	rVB2	161	159	0.03%	0.004%
32	7.470	1045	1047	1048	rBV2	274	244	0.05%	0.005%
33	7.805	1101	1102	1105	rVB	314	249	0.05%	0.006%
34	7.927	1118	1122	1129	rVV3	674	1235	0.23%	0.028%
35	8.000	1132	1134	1136	rBV2	118	127	0.02%	0.003%
36	8.086	1147	1148	1151	rBV2	117	111	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025233.D
 Acq On : 19 Nov 2021 12:41
 Operator : JC/MD
 Sample : VX1119WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

37	8.196	1163	1166	1167	rBV2	89	105	0.02%	0.002%
38	8.324	1181	1187	1202	rVV	80855	131289	24.49%	2.958%
39	8.470	1206	1211	1218	rBV3	521	942	0.18%	0.021%
40	8.573	1225	1228	1234	rVB2	241	366	0.07%	0.008%
41	8.647	1234	1240	1248	rBV	290084	460503	85.91%	10.374%
42	8.720	1248	1252	1257	rVB	4013	6313	1.18%	0.142%
43	8.951	1284	1290	1299	rBV	59740	86131	16.07%	1.940%
44	9.275	1341	1343	1346	rVB3	337	299	0.06%	0.007%
45	9.384	1355	1361	1374	rBV	185930	265603	49.55%	5.983%
46	9.531	1383	1385	1387	rBV2	128	103	0.02%	0.002%
47	9.665	1404	1407	1409	rVV2	111	160	0.03%	0.004%
48	9.701	1409	1413	1419	rVB	1722	2426	0.45%	0.055%
49	9.939	1450	1452	1454	rVB2	205	181	0.03%	0.004%
50	9.963	1454	1456	1457	rBV	190	113	0.02%	0.003%
51	10.000	1457	1462	1463	rBV2	140	214	0.04%	0.005%
52	10.055	1465	1471	1480	rBV	352002	469742	87.63%	10.582%
53	10.201	1491	1495	1497	rBV2	296	412	0.08%	0.009%
54	10.305	1510	1512	1515	rVB	473	430	0.08%	0.010%
55	10.427	1530	1532	1534	rBV	125	104	0.02%	0.002%
56	10.506	1543	1545	1552	rBV2	149	213	0.04%	0.005%
57	10.634	1564	1566	1568	rBV	205	225	0.04%	0.005%
58	10.811	1593	1595	1597	rVV2	169	153	0.03%	0.003%
59	10.957	1618	1619	1622	rVB2	238	219	0.04%	0.005%
60	11.122	1642	1646	1650	rVB2	2208	2876	0.54%	0.065%
61	11.195	1652	1658	1668	rBV	200681	257384	48.01%	5.798%
62	11.280	1668	1672	1673	rBV2	333	399	0.07%	0.009%
63	11.378	1686	1688	1689	rBV	195	117	0.02%	0.003%
64	11.457	1697	1701	1702	rVV3	323	392	0.07%	0.009%
65	11.475	1702	1704	1713	rVB3	623	1153	0.22%	0.026%
66	11.658	1732	1734	1736	rVV	167	129	0.02%	0.003%
67	11.719	1742	1744	1746	rBV	135	110	0.02%	0.002%
68	11.750	1746	1749	1753	rVB3	1866	2448	0.46%	0.055%
69	11.933	1776	1779	1784	rBV3	1076	1401	0.26%	0.032%
70	11.969	1784	1785	1788	rBV	252	247	0.05%	0.006%
71	12.024	1788	1794	1807	rBV	359677	456341	85.13%	10.280%
72	12.122	1808	1810	1812	rBV3	551	555	0.10%	0.013%
73	12.201	1821	1823	1826	rVB2	184	219	0.04%	0.005%
74	12.323	1836	1843	1853	rBV	303197	390080	72.77%	8.788%
75	12.426	1857	1860	1863	rBV2	560	622	0.12%	0.014%
76	12.481	1867	1869	1871	rVB2	343	193	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025233.D
 Acq On : 19 Nov 2021 12:41
 Operator : JC/MD
 Sample : VX1119WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	12.603	1886	1889	1890	rBV2	137	136	0.03%	0.003%
78	12.634	1890	1894	1896	rBV	200	272	0.05%	0.006%
79	12.664	1896	1899	1903	rVV2	297	332	0.06%	0.007%
80	12.762	1913	1915	1918	rVB	299	175	0.03%	0.004%
81	12.878	1931	1934	1936	rBV2	149	157	0.03%	0.004%
82	13.048	1961	1962	1964	rBV	239	237	0.04%	0.005%
83	13.121	1970	1974	1975	rVB	113	127	0.02%	0.003%
84	13.170	1981	1982	1985	rBV	153	98	0.02%	0.002%
85	13.329	2006	2008	2011	rBV	193	192	0.04%	0.004%
86	13.384	2015	2017	2021	rBV	130	142	0.03%	0.003%
87	13.530	2038	2041	2043	rBV	125	147	0.03%	0.003%
88	13.548	2043	2044	2047	rVB2	163	135	0.03%	0.003%
89	13.591	2049	2051	2052	rBV	178	144	0.03%	0.003%
90	13.780	2081	2082	2084	rVB2	168	116	0.02%	0.003%
91	14.036	2122	2124	2126	rBV2	127	129	0.02%	0.003%
92	14.097	2133	2134	2137	rBV2	144	135	0.03%	0.003%
93	14.127	2137	2139	2143	rVV3	310	378	0.07%	0.009%
94	14.194	2148	2150	2154	rVV3	113	124	0.02%	0.003%
95	14.475	2193	2196	2198	rVV2	146	159	0.03%	0.004%
96	14.585	2212	2214	2215	rBV	163	146	0.03%	0.003%
97	14.719	2233	2236	2238	rBV2	176	184	0.03%	0.004%
98	14.877	2260	2262	2265	rBV3	130	109	0.02%	0.002%
99	14.975	2276	2278	2281	rBV2	181	211	0.04%	0.005%
100	14.999	2281	2282	2285	rVB	284	163	0.03%	0.004%

Sum of corrected areas: 4438954




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025233.D
Acq On : 19 Nov 2021 12:41
Operator : JC/MD
Sample : VX1119WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK639

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

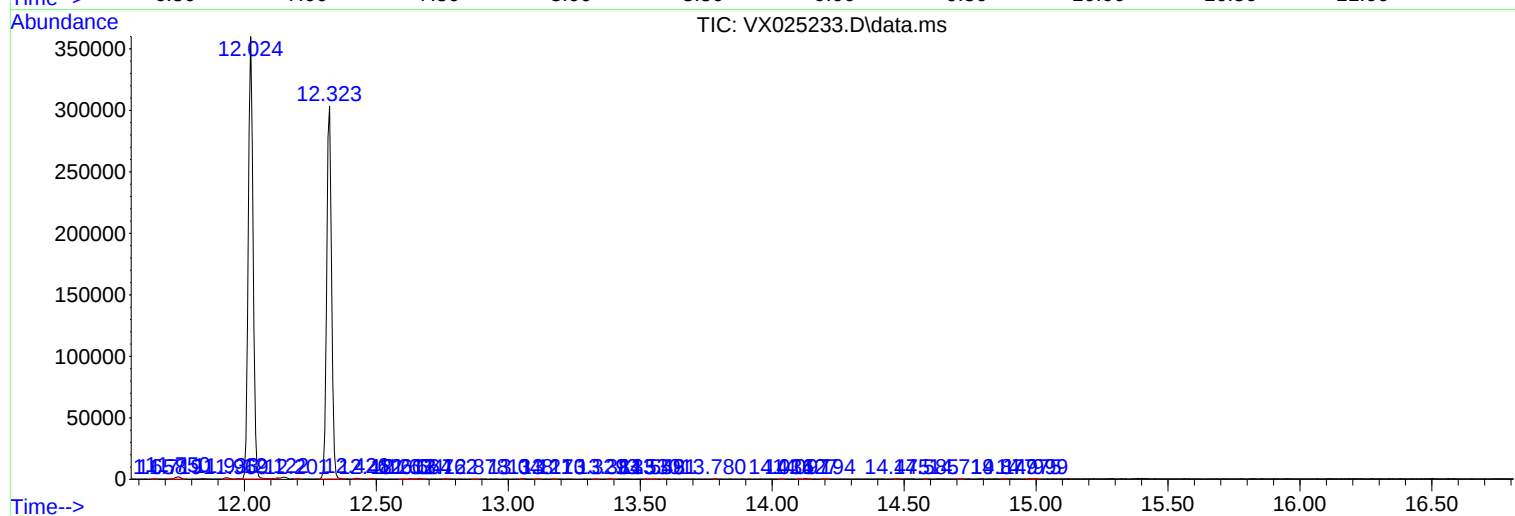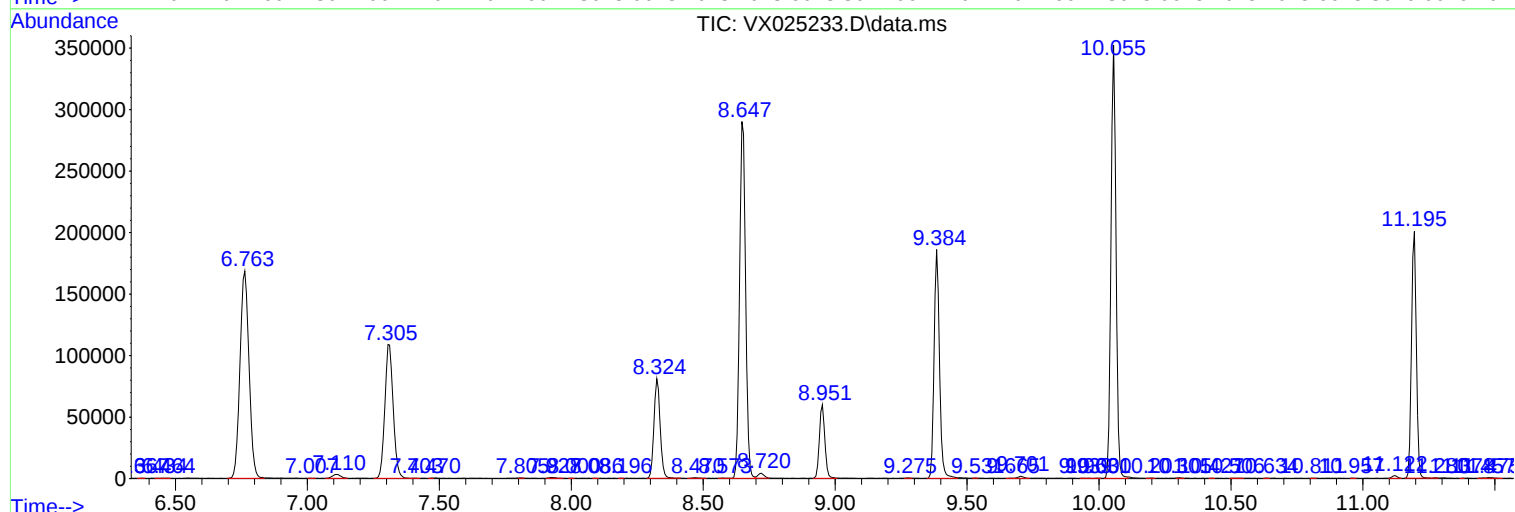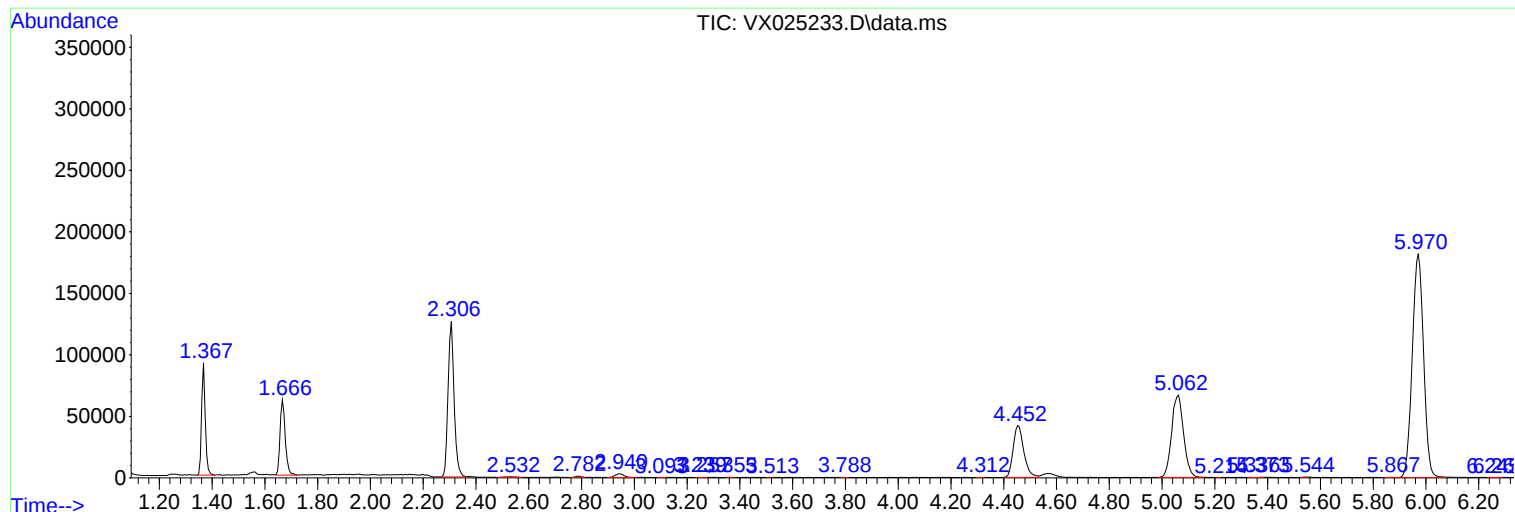

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025233.D
Acq On : 19 Nov 2021 12:41
Operator : JC/MD
Sample : VX1119WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK639

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025233.D
Acq On : 19 Nov 2021 12:41
Operator : JC/MD
Sample : VX1119WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK639

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc