

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025237.D
 Acq On : 19 Nov 2021 16:42
 Operator : JC/MD
 Sample : M4677-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

Signal : TIC: VX025237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rBV	112124	107699	15.60%	2.057%
2	1.660	90	94	104	rBV	77445	107312	15.55%	2.050%
3	2.306	194	200	212	rVB	145549	242760	35.17%	4.637%
4	2.514	232	234	236	rBV	204	198	0.03%	0.004%
5	2.654	256	257	260	rVB	189	154	0.02%	0.003%
6	2.691	260	263	264	rBV	317	288	0.04%	0.006%
7	2.788	275	279	284	rVB2	583	836	0.12%	0.016%
8	2.941	298	304	313	rBV	3444	7686	1.11%	0.147%
9	3.282	358	360	361	rBV	153	129	0.02%	0.002%
10	3.312	364	365	368	rVB	193	161	0.02%	0.003%
11	3.343	368	370	371	rBV2	197	169	0.02%	0.003%
12	3.392	375	378	380	rBV2	157	184	0.03%	0.004%
13	3.507	392	397	398	rBV2	99	157	0.02%	0.003%
14	3.617	414	415	418	rVB2	151	122	0.02%	0.002%
15	3.751	436	437	441	rBV	112	132	0.02%	0.003%
16	4.068	487	489	491	rBV2	130	155	0.02%	0.003%
17	4.087	491	492	495	rVV	182	168	0.02%	0.003%
18	4.117	495	497	499	rVB2	158	143	0.02%	0.003%
19	4.154	502	503	507	rBV2	157	178	0.03%	0.003%
20	4.452	543	552	565	rBV	53742	151265	21.91%	2.890%
21	4.769	603	604	608	rVB	185	187	0.03%	0.004%
22	4.806	608	610	613	rBV2	139	139	0.02%	0.003%
23	5.056	639	651	666	rBV	88428	271972	39.40%	5.195%
24	5.391	704	706	710	rVB	114	138	0.02%	0.003%
25	5.550	728	732	737	rVV2	323	579	0.08%	0.011%
26	5.592	737	739	742	rVB2	179	174	0.03%	0.003%
27	5.623	742	744	747	rBV	198	249	0.04%	0.005%
28	5.739	760	763	765	rBV	137	196	0.03%	0.004%
29	5.861	780	783	786	rBV	121	153	0.02%	0.003%
30	5.970	788	801	818	rBV2	234102	690250	100.00%	13.186%
31	6.239	843	845	847	rVV	154	123	0.02%	0.002%
32	6.452	878	880	882	rBV	152	137	0.02%	0.003%
33	6.763	921	931	944	rBV	159508	370379	53.66%	7.075%
34	6.976	964	966	969	rBV	213	194	0.03%	0.004%
35	7.110	980	988	996	rBV3	4204	8966	1.30%	0.171%
36	7.171	996	998	1001	rVB	179	136	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025237.D
 Acq On : 19 Nov 2021 16:42
 Operator : JC/MD
 Sample : M4677-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
 Title : VOC Analysis

37	7.312	1011	1021	1034	rBV	141136	307145	44.50%	5.867%
38	7.421	1037	1039	1040	rVB	212	138	0.02%	0.003%
39	7.476	1044	1048	1053	rBV3	374	712	0.10%	0.014%
40	7.720	1086	1088	1091	rVV2	142	141	0.02%	0.003%
41	7.787	1097	1099	1100	rBV	257	191	0.03%	0.004%
42	7.934	1118	1123	1128	rVB3	883	1692	0.25%	0.032%
43	8.196	1164	1166	1169	rVB2	149	141	0.02%	0.003%
44	8.324	1180	1187	1204	rBV	106759	172034	24.92%	3.286%
45	8.470	1208	1211	1218	rVV4	729	1206	0.17%	0.023%
46	8.543	1220	1223	1226	rVB2	139	170	0.02%	0.003%
47	8.647	1233	1240	1248	rBV	364713	583086	84.47%	11.138%
48	8.720	1248	1252	1264	rVB	5365	8736	1.27%	0.167%
49	8.952	1284	1290	1298	rBV	76721	110876	16.06%	2.118%
50	9.275	1341	1343	1347	rBV	283	230	0.03%	0.004%
51	9.384	1355	1361	1378	rBV	243876	346431	50.19%	6.618%
52	9.701	1410	1413	1419	rVB3	1049	1499	0.22%	0.029%
53	9.762	1419	1423	1426	rBV2	147	218	0.03%	0.004%
54	10.055	1465	1471	1483	rBV	329679	442945	64.17%	8.461%
55	10.201	1492	1495	1498	rBV3	180	225	0.03%	0.004%
56	10.305	1508	1512	1515	rBV2	541	686	0.10%	0.013%
57	10.470	1534	1539	1541	rBV	170	218	0.03%	0.004%
58	10.646	1564	1568	1570	rBV2	227	200	0.03%	0.004%
59	10.750	1583	1585	1588	rBV2	135	114	0.02%	0.002%
60	11.122	1640	1646	1652	rBV2	2091	2831	0.41%	0.054%
61	11.195	1652	1658	1666	rBV	258988	336941	48.81%	6.436%
62	11.323	1678	1679	1683	rVB2	340	247	0.04%	0.005%
63	11.378	1685	1688	1690	rBV3	189	283	0.04%	0.005%
64	11.476	1702	1704	1709	rBV4	541	843	0.12%	0.016%
65	11.549	1714	1716	1718	rVB	301	171	0.02%	0.003%
66	11.750	1744	1749	1755	rVB3	1890	2849	0.41%	0.054%
67	11.841	1759	1764	1770	rBB3	533	667	0.10%	0.013%
68	11.890	1770	1772	1775	rVB2	133	143	0.02%	0.003%
69	11.933	1775	1779	1783	rBV3	1008	1389	0.20%	0.027%
70	12.024	1789	1794	1804	rBV	339826	428351	62.06%	8.183%
71	12.128	1807	1811	1812	rBV	750	768	0.11%	0.015%
72	12.323	1835	1843	1851	rBV	395321	510051	73.89%	9.743%
73	12.421	1857	1859	1863	rVB2	656	747	0.11%	0.014%
74	12.469	1866	1867	1868	rBV	298	161	0.02%	0.003%
75	12.622	1889	1892	1893	rBV2	167	166	0.02%	0.003%
76	12.762	1912	1915	1918	rBV2	294	341	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025237.D
 Acq On : 19 Nov 2021 16:42
 Operator : JC/MD
 Sample : M4677-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis

77	13.109	1969	1972	1975	rBV2	130	192	0.03%	0.004%
78	13.244	1992	1994	1997	rVB	227	188	0.03%	0.004%
79	13.451	2027	2028	2031	rBV	200	164	0.02%	0.003%
80	13.609	2052	2054	2055	rBV2	175	130	0.02%	0.002%
81	13.743	2073	2076	2079	rVB	98	119	0.02%	0.002%
82	13.884	2097	2099	2102	rBV2	210	210	0.03%	0.004%
83	14.140	2135	2141	2144	rBV2	502	696	0.10%	0.013%
84	14.274	2162	2163	2166	rBV	132	161	0.02%	0.003%
85	14.335	2171	2173	2176	rBV2	98	148	0.02%	0.003%
86	14.396	2180	2183	2186	rBV2	157	158	0.02%	0.003%
87	14.445	2189	2191	2194	rVB	191	141	0.02%	0.003%
88	14.469	2194	2195	2197	rVB	184	116	0.02%	0.002%
89	14.499	2197	2200	2203	rBV2	205	334	0.05%	0.006%
90	14.688	2229	2231	2233	rBV2	214	180	0.03%	0.003%
91	14.768	2242	2244	2245	rBV	311	163	0.02%	0.003%
92	14.871	2259	2261	2264	rVB2	197	185	0.03%	0.004%
93	15.292	2324	2330	2332	rBV3	243	390	0.06%	0.007%
94	15.457	2355	2357	2358	rBV2	159	124	0.02%	0.002%
95	16.225	2481	2483	2484	rBV	284	135	0.02%	0.003%
96	16.286	2491	2493	2496	rVB2	357	297	0.04%	0.006%
97	16.389	2508	2510	2513	rVB	300	222	0.03%	0.004%
98	16.536	2530	2534	2536	rBV2	192	259	0.04%	0.005%
99	16.682	2557	2558	2560	rVB	373	167	0.02%	0.003%
100	16.700	2560	2561	2562	rBV	281	158	0.02%	0.003%


Sum of corrected areas: 5234888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025237.D
Acq On : 19 Nov 2021 16:42
Operator : JC/MD
Sample : M4677-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

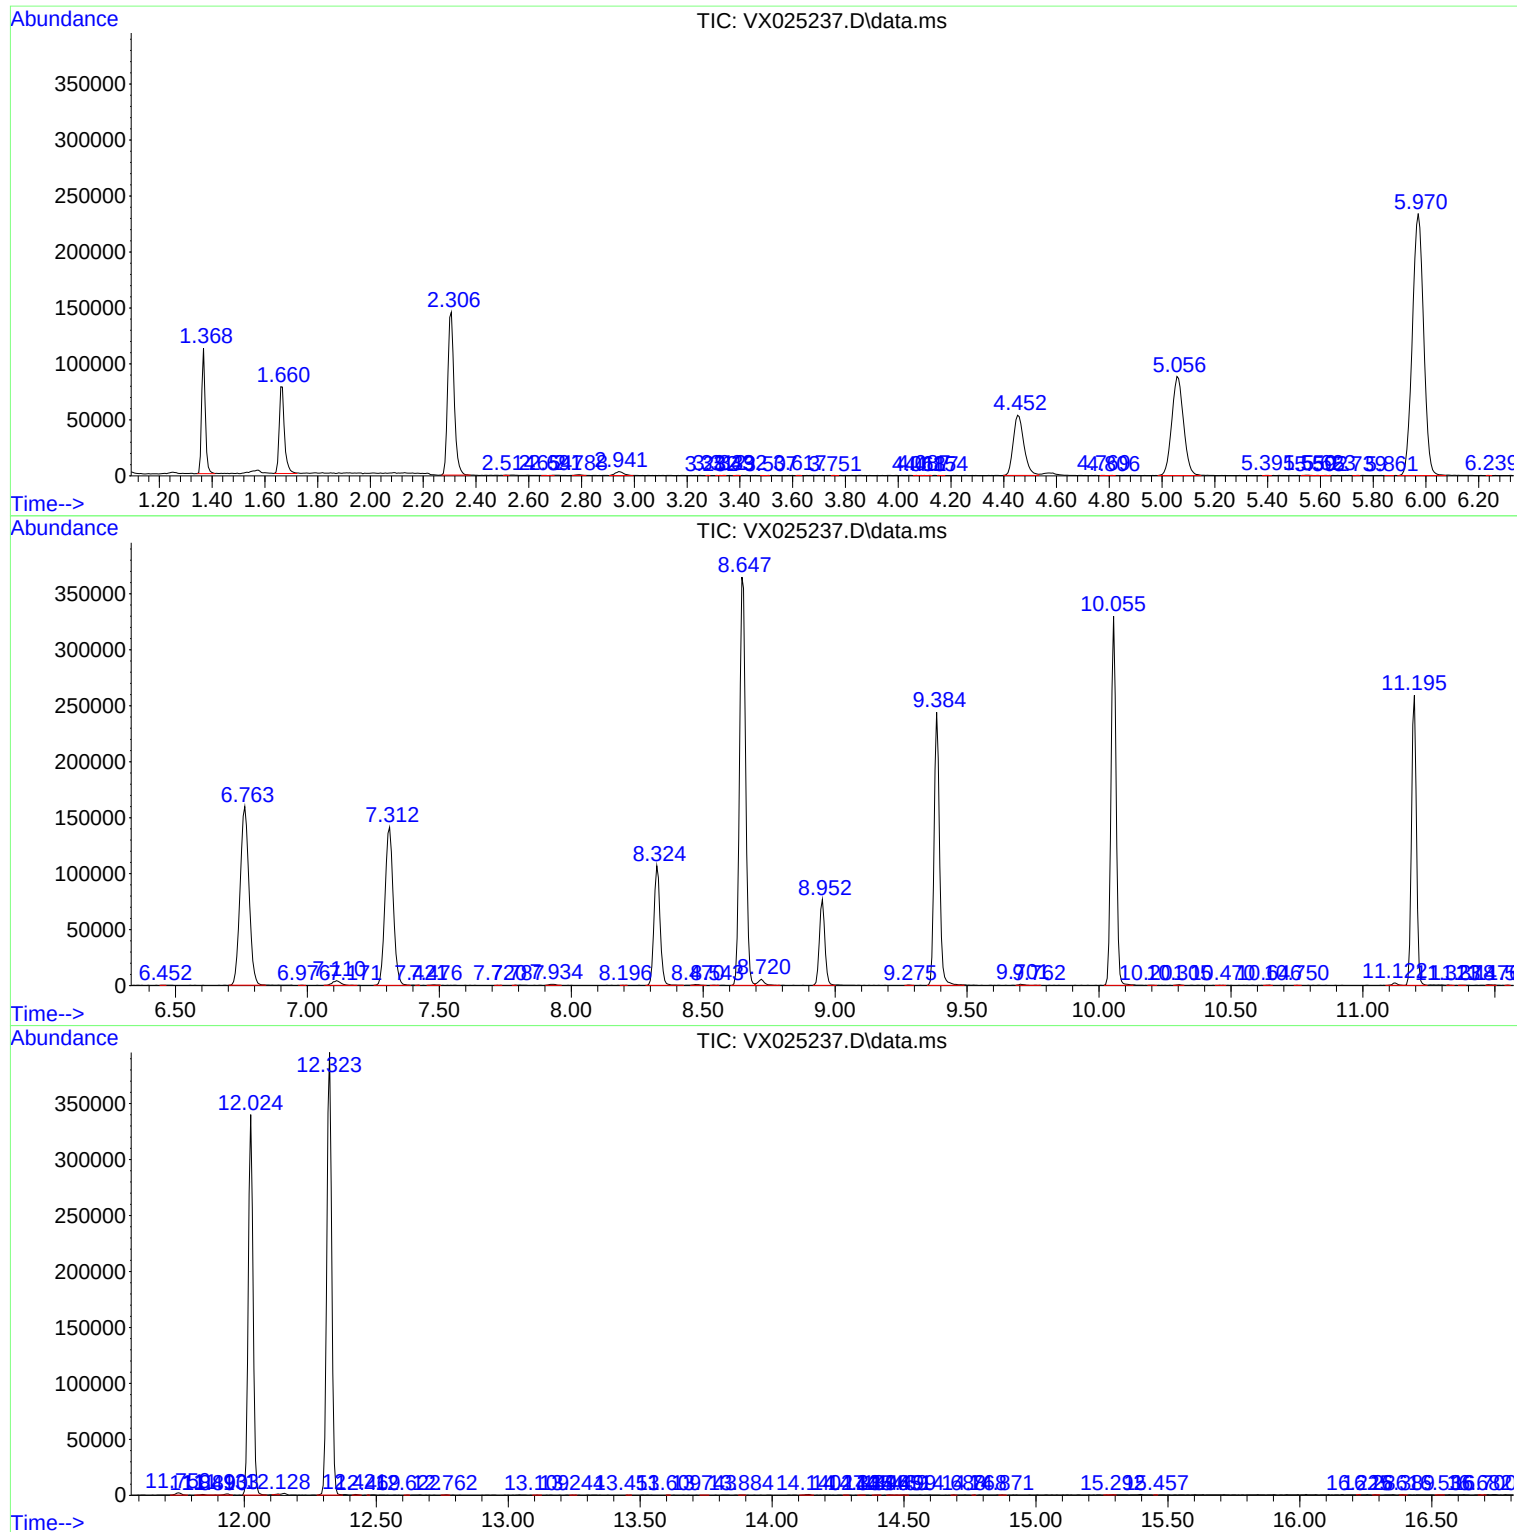

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025237.D
Acq On : 19 Nov 2021 16:42
Operator : JC/MD
Sample : M4677-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
Data File : VX025237.D
Acq On : 19 Nov 2021 16:42
Operator : JC/MD
Sample : M4677-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc