
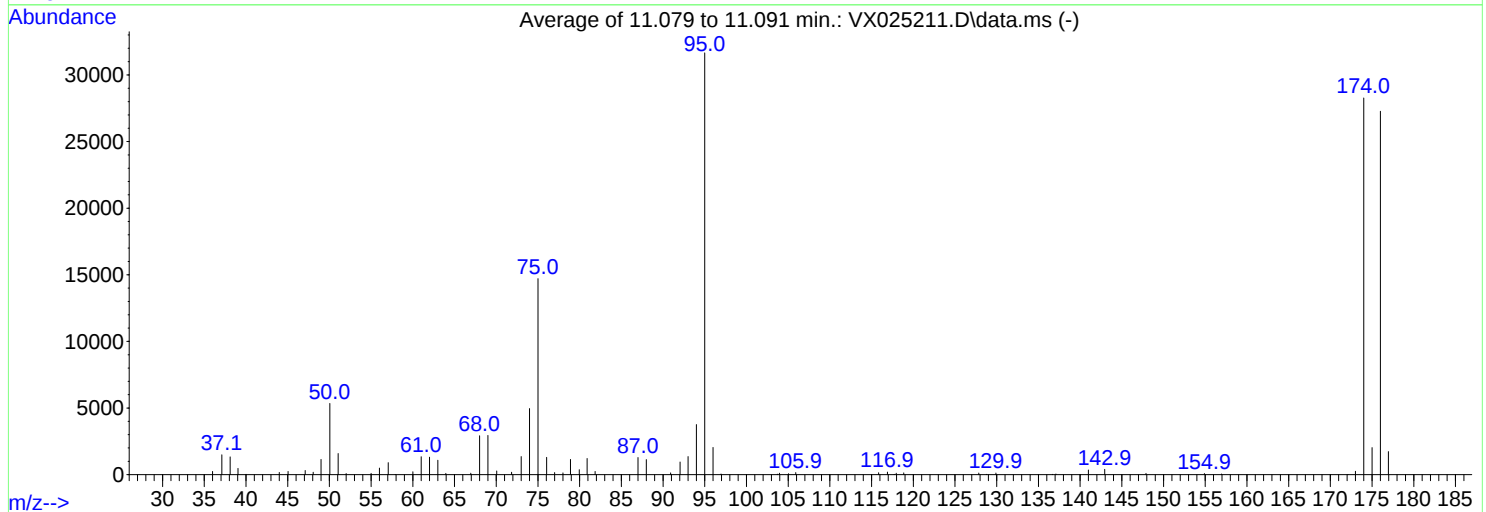


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025211.D
 Acq On : 18 Nov 2021 14:20
 Operator : JC/MD
 Sample : BFB615
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB615

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis
 Last Update : Mon Nov 22 00:11:59 2021

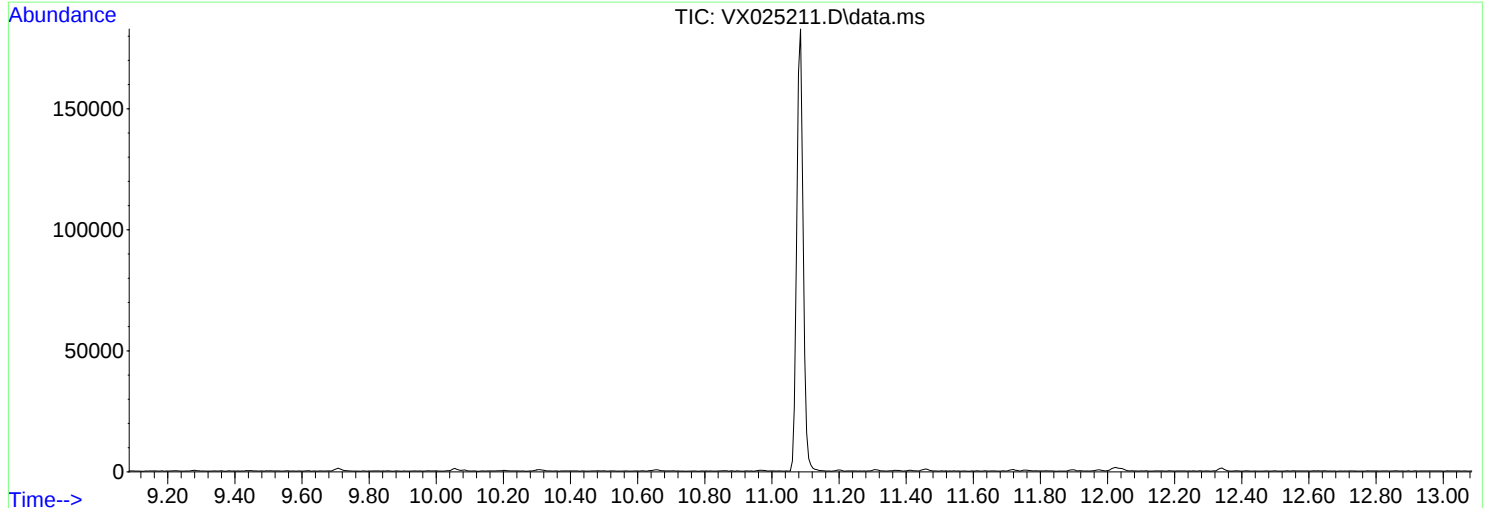

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	5345	PASS
75	95	30	80	46.5	14716	PASS
95	95	100	100	100.0	31659	PASS
96	95	5	9	6.5	2046	PASS
173	174	0.00	2	0.9	252	PASS
174	95	50	120	89.3	28275	PASS
175	174	5	9	7.2	2035	PASS
176	174	95	101	96.5	27272	PASS
177	176	5	9	6.4	1735	PASS

m/z	Abundance
36.00	293.0
37.10	1663.0
38.10	1536.0
39.00	481.0
40.00	268.0
44.00	412.0
45.10	281.0
47.10	315.0
48.00	209.0
49.00	1194.0
50.00	6105.0
51.00	1880.0
52.00	59.0
55.00	129.0
56.00	553.0
57.10	1011.0
60.10	232.0
61.00	1689.0
62.00	1489.0
63.00	1240.0
64.00	116.0
66.90	119.0
68.00	3245.0
69.00	3518.0
70.10	246.0
71.90	183.0
73.00	1578.0
74.00	5739.0
75.00	17168.0
76.00	1509.0
77.00	210.0
78.00	173.0
78.90	1336.0
80.00	421.0
80.90	1514.0
81.90	279.0
87.00	1516.0
88.00	1392.0
90.90	155.0
92.00	1036.0
93.00	1527.0
94.00	4422.0
95.00	37976.0
96.00	2507.0
97.00	63.0
103.90	186.0
105.10	85.0
105.90	157.0
115.80	164.0
116.90	266.0
117.90	209.0
118.90	144.0
127.80	144.0
128.80	71.0
129.90	152.0
136.70	74.0
137.10	86.0
140.00	54.0
141.00	462.0
142.90	489.0
147.90	116.0
154.80	91.0
156.90	72.0
172.10	54.0
173.00	292.0
174.00	33616.0
175.00	2336.0
176.00	32552.0
177.00	2074.0

Instrument :
MSVOA_X
ClientSampleId :
BFB615

m/z	Abundance
36.00	109.0
37.00	1040.0
38.10	817.0
39.10	370.0
40.10	199.0
44.10	277.0
45.00	183.0
47.10	206.0
48.10	120.0
49.10	779.0
50.10	3494.0
51.00	1103.0
52.00	94.0
54.90	63.0
56.00	321.0
57.00	588.0
59.90	129.0
61.00	911.0
62.00	778.0
63.10	761.0
63.80	64.0
67.00	89.0
68.00	1999.0
69.10	2030.0
70.00	193.0
71.80	155.0
73.00	1018.0
74.00	3452.0
75.00	9860.0
76.10	800.0
77.10	102.0
77.90	81.0
78.90	823.0
79.90	268.0
80.90	716.0
81.90	166.0
87.00	906.0
88.00	745.0
91.00	141.0
92.00	734.0
93.00	1075.0
94.00	2713.0
95.00	22992.0
96.10	1379.0
103.70	108.0
105.00	72.0
106.00	100.0
115.90	116.0
116.90	151.0
117.70	78.0
118.80	140.0
127.90	100.0
130.00	63.0
140.90	248.0
143.00	312.0
147.90	92.0
155.00	62.0
157.00	76.0
173.00	217.0
174.00	24120.0
175.00	1658.0
176.00	23120.0
176.90	1404.0

Instrument :
MSVOA_X
ClientSampleId :
BFB615

m/z	Abundance
40.00	200.0
44.00	194.0

Instrument :
MSVOA_X
ClientSampleId :
BFB615

m/z	Abundance
36.00	309.0
37.10	1755.0
38.10	1632.0
39.10	569.0
40.00	215.0
44.10	412.0
45.00	268.0
47.10	402.0
48.10	221.0
49.00	1465.0
50.10	6436.0
51.10	1773.0
52.00	87.0
55.00	104.0
56.00	614.0
57.00	1099.0
57.90	52.0
60.00	282.0
61.00	1436.0
62.00	1678.0
63.00	1233.0
64.00	117.0
67.00	130.0
68.00	3526.0
69.00	3299.0
70.00	376.0
71.90	215.0
73.00	1480.0
74.00	5698.0
75.00	17120.0
76.10	1596.0
77.00	173.0
78.00	135.0
78.90	1255.0
79.90	427.0
80.90	1413.0
81.80	288.0
87.00	1440.0
88.00	1268.0
90.80	115.0
92.10	1076.0
93.00	1459.0
94.00	4149.0
95.00	34008.0
96.00	2253.0
96.90	72.0
104.00	156.0
105.10	75.0
105.90	198.0
115.90	167.0
116.90	172.0
118.10	104.0
118.80	126.0
127.90	121.0
129.90	162.0
137.10	73.0
141.00	333.0
142.90	390.0
147.90	77.0
154.90	87.0
173.00	246.0
174.00	27088.0
175.00	2110.0
176.00	26144.0
177.00	1728.0

Instrument :
MSVOA_X
ClientSampleId :
BFB615