


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111921\
 Data File : VX025231.D
 Acq On : 19 Nov 2021 09:08
 Operator : JC/MD
 Sample : BFB616
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB616

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111121WMA.M
 Title : VOC Analysis
 Last Update : Mon Nov 22 00:11:59 2021

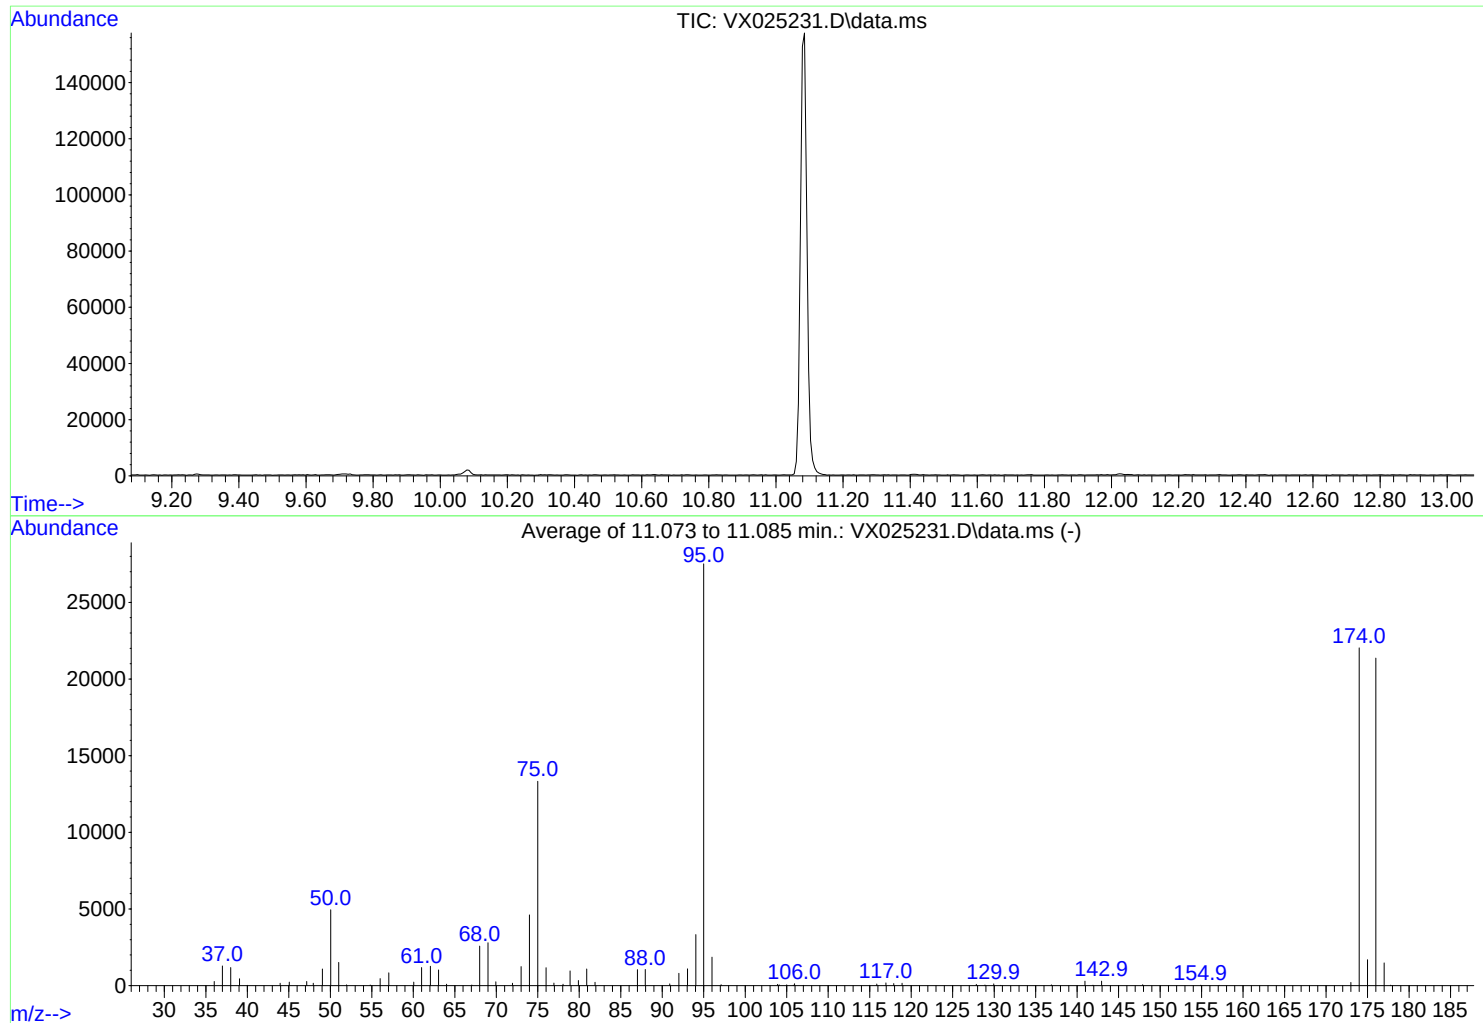

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	4944	PASS
75	95	30	80	48.4	13329	PASS
95	95	100	100	100.0	27512	PASS
96	95	5	9	6.8	1862	PASS
173	174	0.00	2	0.9	205	PASS
174	95	50	120	80.1	22029	PASS
175	174	5	9	7.7	1687	PASS
176	174	95	101	97.0	21359	PASS
177	176	5	9	6.9	1481	PASS

m/z	Abundance
36.00	266.0
37.00	1476.0
38.00	1449.0
39.10	453.0
40.00	216.0
44.00	360.0
45.10	253.0
47.20	252.0
47.90	172.0
49.10	1094.0
50.00	5222.0
51.00	1643.0
51.90	70.0
54.80	71.0
56.00	575.0
57.10	821.0
60.00	307.0
61.00	1324.0
62.10	1276.0
63.00	1026.0
64.00	117.0
67.00	70.0
68.00	2775.0
69.00	3210.0
69.90	288.0
71.90	160.0
73.00	1220.0
74.00	5127.0
75.00	14998.0
76.00	1323.0
77.00	202.0
78.00	113.0
78.90	1053.0
79.90	359.0
80.90	1120.0
81.90	277.0
87.00	1305.0
88.00	1167.0
91.00	148.0
92.00	933.0
93.00	1199.0
94.10	3788.0
95.00	31696.0
96.00	2083.0
97.10	63.0
103.90	157.0
105.00	76.0
105.90	157.0
115.00	68.0
115.90	115.0
116.90	218.0
117.90	161.0
119.00	176.0
127.80	108.0
128.90	53.0
130.00	157.0
136.90	79.0
140.90	368.0
141.90	51.0
142.90	425.0
147.90	67.0
154.90	85.0
157.10	72.0
173.00	260.0
174.00	29232.0
175.00	2188.0
176.00	28304.0
177.00	1893.0
177.80	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB616

Scan 1633 (11.042 min): VX025231.D\data.ms
BFB616

m/z	Abundance
40.00	184.0
44.00	156.0

Instrument :
MSVOA_X
ClientSampleId :
BFB616

m/z	Abundance
36.00	335.0
37.00	1409.0
38.00	1213.0
39.00	537.0
40.00	196.0
43.90	345.0
45.00	307.0
47.00	292.0
48.00	180.0
49.00	1289.0
50.00	6044.0
51.00	1820.0
52.00	86.0
54.80	67.0
56.00	446.0
57.00	1052.0
60.00	203.0
61.00	1381.0
62.00	1541.0
63.00	1328.0
64.00	91.0
67.10	58.0
68.00	3082.0
69.00	3171.0
69.90	282.0
72.00	209.0
73.00	1620.0
74.00	5265.0
75.00	15826.0
76.00	1273.0
76.90	188.0
78.00	99.0
78.90	1146.0
79.90	328.0
80.90	1306.0
81.90	222.0
87.00	1192.0
88.00	1289.0
90.90	129.0
92.00	967.0
93.00	1337.0
94.00	4009.0
95.00	32400.0
96.00	2161.0
97.10	72.0
104.10	169.0
105.00	90.0
106.00	209.0
107.00	72.0
115.90	104.0
116.90	211.0
117.80	139.0
118.90	186.0
127.80	87.0
128.90	61.0
129.90	124.0
130.80	57.0
136.90	85.0
141.00	339.0
141.90	56.0
142.90	311.0
147.90	65.0
173.00	256.0
174.00	24416.0
175.00	2003.0
176.00	24248.0
177.00	1739.0
177.80	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB616

m/z	Abundance
36.00	212.0
37.00	960.0
38.00	889.0
39.10	356.0
40.00	204.0
44.00	237.0
45.10	133.0
47.20	270.0
48.00	110.0
49.00	885.0
50.10	3565.0
51.00	1090.0
56.00	356.0
57.00	635.0
60.10	175.0
61.00	827.0
62.00	977.0
63.10	699.0
64.00	75.0
68.00	1867.0
69.00	1997.0
70.00	196.0
72.00	89.0
73.00	884.0
74.00	3450.0
75.00	9164.0
76.00	920.0
77.00	100.0
78.10	81.0
78.90	693.0
79.90	314.0
80.90	818.0
81.90	162.0
87.00	629.0
87.90	694.0
90.80	81.0
92.00	496.0
93.10	751.0
94.00	2180.0
95.00	18440.0
96.00	1341.0
97.10	59.0
103.90	83.0
105.80	97.0
115.80	93.0
117.00	101.0
118.00	94.0
118.80	114.0
128.00	69.0
129.90	70.0
140.90	179.0
143.00	148.0
147.90	67.0
173.00	98.0
174.00	12438.0
175.00	870.0
176.00	11526.0
177.00	810.0

Instrument :
MSVOA_X
ClientSampleId :
BFB616