

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043898.D
 Acq On : 19 Nov 2024 14:12
 Operator : JC/MD
 Sample : VX1119WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK730

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111924WMA.M
 Title : VOC Analysis

Signal : TIC: VX043898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	10102	10478	0.87%	0.122%
2	1.368	42	46	57	rBV	143944	179779	15.00%	2.087%
3	1.642	88	91	102	rVB	69050	101495	8.47%	1.178%
4	2.294	192	198	209	rVB	243949	388655	32.43%	4.511%
5	2.776	271	277	284	rBV5	1558	3598	0.30%	0.042%
6	2.934	297	303	310	rVV2	6679	14795	1.23%	0.172%
7	3.056	320	323	324	rBV	376	357	0.03%	0.004%
8	3.123	332	334	337	rVB2	425	360	0.03%	0.004%
9	3.270	353	358	360	rBV2	626	877	0.07%	0.010%
10	3.428	380	384	390	rBV5	1007	2341	0.20%	0.027%
11	3.806	444	446	451	rVV2	738	563	0.05%	0.007%
12	3.879	456	458	461	rVB2	453	428	0.04%	0.005%
13	4.288	523	525	528	rBV2	558	461	0.04%	0.005%
14	4.459	545	553	568	rBV	79315	239184	19.96%	2.776%
15	4.922	627	629	633	rVB2	501	712	0.06%	0.008%
16	5.050	638	650	669	rVV	154791	482599	40.27%	5.601%
17	5.190	671	673	676	rVB4	532	593	0.05%	0.007%
18	5.257	682	684	686	rBV3	513	482	0.04%	0.006%
19	5.318	692	694	697	rBV3	350	380	0.03%	0.004%
20	5.355	697	700	701	rBV3	456	457	0.04%	0.005%
21	5.397	701	707	709	rBV3	1123	1875	0.16%	0.022%
22	5.538	725	730	731	rBV	1210	1328	0.11%	0.015%
23	5.660	747	750	753	rBV2	362	504	0.04%	0.006%
24	5.708	756	758	761	rVV	623	402	0.03%	0.005%
25	5.958	787	799	814	rBV3	416198	1198401	100.00%	13.909%
26	6.361	861	865	866	rBV4	745	944	0.08%	0.011%
27	6.428	875	876	878	rBV	597	459	0.04%	0.005%
28	6.598	901	904	906	rBV2	523	574	0.05%	0.007%
29	6.629	906	909	912	rVB2	570	859	0.07%	0.010%
30	6.659	912	914	915	rBV2	427	344	0.03%	0.004%
31	6.678	915	917	920	rVB2	397	429	0.04%	0.005%
32	6.751	920	929	943	rBV	285874	691513	57.70%	8.026%
33	7.117	983	989	998	rVB6	6095	16370	1.37%	0.190%
34	7.184	998	1000	1001	rBV2	606	471	0.04%	0.005%
35	7.300	1011	1019	1037	rBV	239651	533147	44.49%	6.188%
36	7.476	1044	1048	1055	rVB6	944	2196	0.18%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043898.D
 Acq On : 19 Nov 2024 14:12
 Operator : JC/MD
 Sample : VX1119WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK730

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

37	7.964	1126	1128	1129	rBV2	425	343	0.03%	0.004%
38	8.074	1144	1146	1150	rVV2	312	370	0.03%	0.004%
39	8.177	1159	1163	1166	rBV2	621	908	0.08%	0.011%
40	8.324	1181	1187	1198	rBV	147267	255079	21.28%	2.960%
41	8.647	1233	1240	1256	rBV	582634	944851	78.84%	10.966%
42	8.860	1273	1275	1276	rBV2	432	361	0.03%	0.004%
43	8.915	1283	1284	1285	rBV	548	359	0.03%	0.004%
44	8.946	1285	1289	1304	rVV	106865	165006	13.77%	1.915%
45	9.275	1341	1343	1347	rVB4	1277	1401	0.12%	0.016%
46	9.336	1350	1353	1354	rBV2	424	491	0.04%	0.006%
47	9.384	1356	1361	1379	rBV	315121	510165	42.57%	5.921%
48	9.708	1410	1414	1417	rVB3	1344	2044	0.17%	0.024%
49	9.958	1453	1455	1458	rBV2	390	366	0.03%	0.004%
50	10.049	1465	1470	1482	rBV	586393	845813	70.58%	9.817%
51	10.293	1508	1510	1511	rBV2	882	575	0.05%	0.007%
52	10.360	1519	1521	1524	rVB2	515	496	0.04%	0.006%
53	10.482	1539	1541	1542	rBV	633	534	0.04%	0.006%
54	10.500	1542	1544	1548	rVB3	365	544	0.05%	0.006%
55	10.549	1548	1552	1554	rBV2	472	629	0.05%	0.007%
56	10.646	1566	1568	1569	rBV2	773	631	0.05%	0.007%
57	10.860	1602	1603	1606	rVV2	433	443	0.04%	0.005%
58	10.963	1618	1620	1621	rBV2	754	449	0.04%	0.005%
59	11.189	1652	1657	1665	rBV	425603	540645	45.11%	6.275%
60	11.415	1690	1694	1695	rVB2	432	470	0.04%	0.005%
61	11.451	1697	1700	1704	rVV3	1393	1650	0.14%	0.019%
62	11.494	1704	1707	1709	rVV2	526	511	0.04%	0.006%
63	11.628	1728	1729	1732	rBV2	391	434	0.04%	0.005%
64	11.671	1734	1736	1739	rBV2	455	500	0.04%	0.006%
65	11.762	1745	1751	1755	rBV3	1178	1863	0.16%	0.022%
66	11.805	1755	1758	1760	rVB	586	527	0.04%	0.006%
67	11.841	1760	1764	1765	rBV3	393	389	0.03%	0.005%
68	11.860	1765	1767	1769	rBV2	545	513	0.04%	0.006%
69	11.915	1773	1776	1779	rBV2	350	583	0.05%	0.007%
70	11.975	1782	1786	1788	rBV2	2121	2351	0.20%	0.027%
71	12.018	1788	1793	1802	rBV	560599	703544	58.71%	8.165%
72	12.232	1827	1828	1832	rVV3	454	468	0.04%	0.005%
73	12.317	1837	1842	1857	rBV	579098	733107	61.17%	8.508%
74	12.469	1865	1867	1870	rVB3	526	458	0.04%	0.005%
75	12.530	1875	1877	1879	rVB3	416	421	0.04%	0.005%
76	12.603	1887	1889	1891	rVB2	594	507	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043898.D
 Acq On : 19 Nov 2024 14:12
 Operator : JC/MD
 Sample : VX1119WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK730

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

77	12.634	1893	1894	1896	rBV2	677	358	0.03%	0.004%
78	12.719	1906	1908	1911	rBV2	483	466	0.04%	0.005%
79	12.756	1912	1914	1918	rVB2	914	785	0.07%	0.009%
80	12.878	1930	1934	1936	rBV3	486	736	0.06%	0.009%
81	13.079	1966	1967	1971	rBV2	520	406	0.03%	0.005%
82	13.116	1971	1973	1977	rVB3	910	1209	0.10%	0.014%
83	13.426	2022	2024	2026	rBV	370	393	0.03%	0.005%
84	13.567	2044	2047	2049	rVV	438	476	0.04%	0.006%
85	13.597	2049	2052	2056	rVB3	955	1266	0.11%	0.015%
86	13.640	2056	2059	2061	rVB2	425	384	0.03%	0.004%
87	13.676	2061	2065	2066	rVB2	334	362	0.03%	0.004%
88	13.774	2079	2081	2083	rBV3	841	796	0.07%	0.009%
89	13.890	2096	2100	2104	rBV3	431	685	0.06%	0.008%
90	13.969	2109	2113	2115	rBV4	839	1007	0.08%	0.012%
91	14.073	2129	2130	2134	rVV2	521	480	0.04%	0.006%
92	14.128	2134	2139	2144	rVV2	1838	2767	0.23%	0.032%
93	14.170	2144	2146	2148	rVV2	634	367	0.03%	0.004%
94	14.231	2155	2156	2159	rVB2	626	469	0.04%	0.005%
95	14.560	2208	2210	2212	rVB2	511	479	0.04%	0.006%
96	14.585	2212	2214	2217	rBV2	507	662	0.06%	0.008%
97	14.902	2264	2266	2269	rBV	524	501	0.04%	0.006%
98	15.164	2307	2309	2311	rBV2	500	473	0.04%	0.005%
99	16.127	2465	2467	2469	rVB3	812	708	0.06%	0.008%
100	16.597	2542	2544	2547	rBV3	767	785	0.07%	0.009%

Sum of corrected areas: 8616229




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043898.D
Acq On : 19 Nov 2024 14:12
Operator : JC/MD
Sample : VX1119WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK730

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

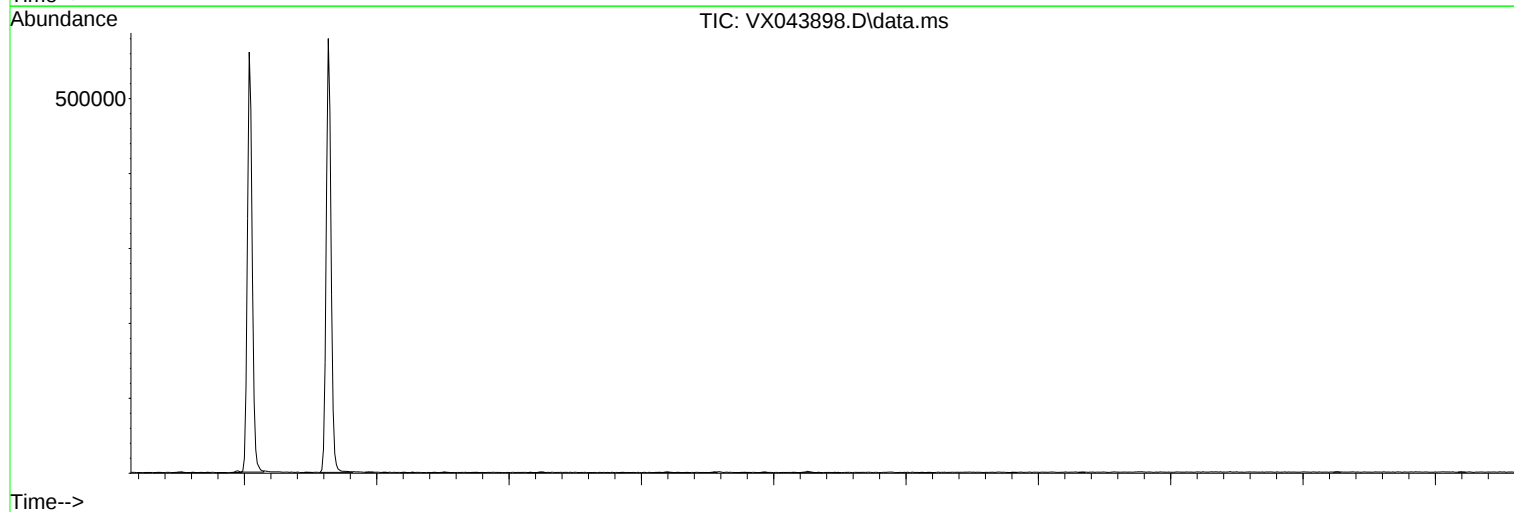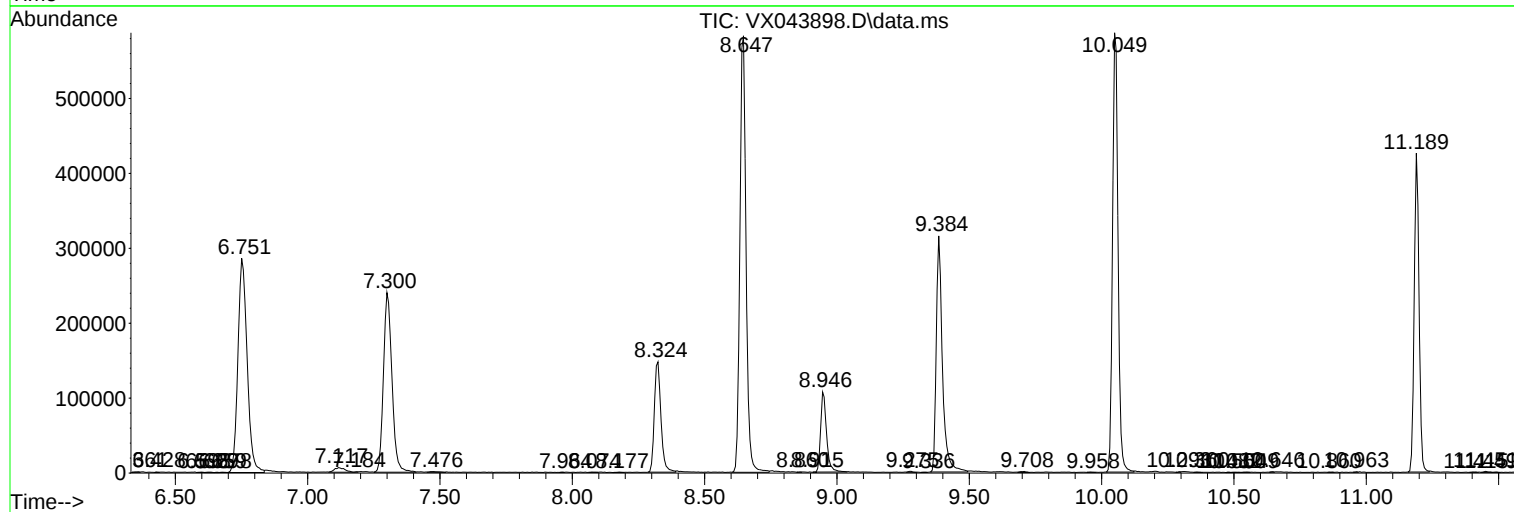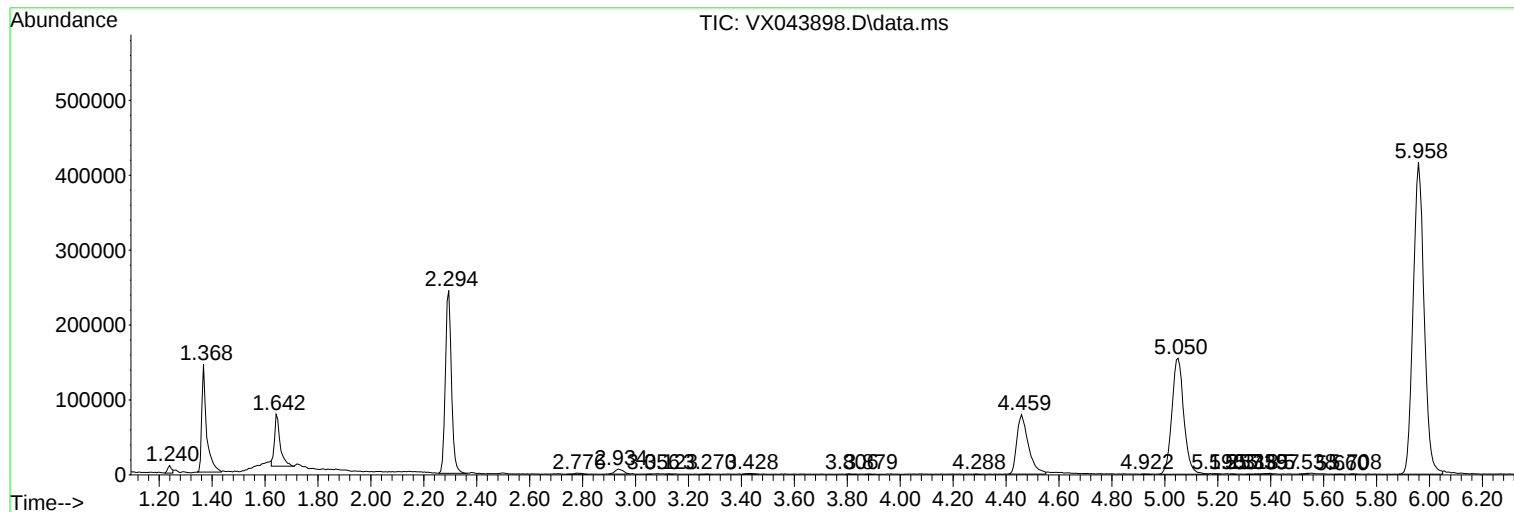

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043898.D
Acq On : 19 Nov 2024 14:12
Operator : JC/MD
Sample : VX1119WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK730

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043898.D
Acq On : 19 Nov 2024 14:12
Operator : JC/MD
Sample : VX1119WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK730

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc