

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043900.D
 Acq On : 19 Nov 2024 14:59
 Operator : JC/MD
 Sample : P4782-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

Signal : TIC: VX043900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV2	8881	13431	1.10%	0.155%
2	1.368	42	46	58	rBV	142132	173682	14.28%	2.002%
3	1.642	88	91	101	rVB	75920	106894	8.79%	1.232%
4	2.294	192	198	212	rBV	221844	352560	28.99%	4.063%
5	2.563	241	242	244	rBV2	387	365	0.03%	0.004%
6	2.782	271	278	279	rBV4	1155	1842	0.15%	0.021%
7	2.867	290	292	295	rVB3	410	406	0.03%	0.005%
8	2.941	295	304	310	rBV	12452	28521	2.35%	0.329%
9	3.172	340	342	343	rVB2	597	384	0.03%	0.004%
10	3.270	357	358	365	rVB3	393	576	0.05%	0.007%
11	3.422	379	383	386	rBV3	721	1197	0.10%	0.014%
12	3.605	410	413	416	rBV3	317	420	0.03%	0.005%
13	4.391	540	542	544	rVB	540	384	0.03%	0.004%
14	4.459	545	553	571	rBV	81863	253600	20.85%	2.923%
15	4.861	618	619	621	rBV	439	410	0.03%	0.005%
16	5.056	637	651	667	rBV	154980	489987	40.29%	5.647%
17	5.361	697	701	702	rBV2	561	650	0.05%	0.007%
18	5.501	721	724	726	rBV2	300	338	0.03%	0.004%
19	5.550	726	732	733	rBV3	1062	1856	0.15%	0.021%
20	5.641	744	747	750	rVB3	407	419	0.03%	0.005%
21	5.800	770	773	774	rVB2	352	338	0.03%	0.004%
22	5.824	774	777	778	rBV	371	334	0.03%	0.004%
23	5.849	778	781	782	rVB	465	334	0.03%	0.004%
24	5.964	788	800	820	rBV2	404257	1216095	100.00%	14.016%
25	6.312	855	857	859	rVB2	551	467	0.04%	0.005%
26	6.434	875	877	880	rBV2	624	691	0.06%	0.008%
27	6.592	898	903	905	rBV3	472	849	0.07%	0.010%
28	6.757	921	930	946	rBV	314824	770424	63.35%	8.880%
29	7.123	983	990	1001	rVB9	4832	13003	1.07%	0.150%
30	7.202	1001	1003	1004	rBV2	576	457	0.04%	0.005%
31	7.306	1012	1020	1035	rBV	242030	546826	44.97%	6.302%
32	7.574	1061	1064	1065	rBV2	414	436	0.04%	0.005%
33	7.671	1078	1080	1082	rBV2	256	321	0.03%	0.004%
34	8.019	1136	1137	1142	rVB3	629	854	0.07%	0.010%
35	8.110	1148	1152	1155	rBV3	405	566	0.05%	0.007%
36	8.324	1180	1187	1204	rVV	158267	267460	21.99%	3.083%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043900.D
 Acq On : 19 Nov 2024 14:59
 Operator : JC/MD
 Sample : P4782-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

37	8.647	1233	1240	1250	rBV	568139	893302	73.46%	10.296%
38	8.891	1277	1280	1282	rBV3	291	330	0.03%	0.004%
39	8.952	1284	1290	1300	rBV	104763	166620	13.70%	1.920%
40	9.128	1317	1319	1320	rBV2	384	369	0.03%	0.004%
41	9.177	1325	1327	1330	rVB3	510	503	0.04%	0.006%
42	9.384	1356	1361	1379	rBV	313648	504534	41.49%	5.815%
43	9.695	1410	1412	1418	rBV4	1748	2885	0.24%	0.033%
44	9.854	1435	1438	1439	rBV	588	408	0.03%	0.005%
45	9.945	1452	1453	1456	rBV4	519	381	0.03%	0.004%
46	10.055	1465	1471	1490	rVB	553924	795259	65.39%	9.166%
47	10.311	1509	1513	1518	rBV4	1423	2027	0.17%	0.023%
48	10.433	1531	1533	1535	rVB2	450	405	0.03%	0.005%
49	10.457	1535	1537	1540	rVB2	465	358	0.03%	0.004%
50	10.500	1542	1544	1546	rVB2	529	436	0.04%	0.005%
51	10.525	1546	1548	1550	rBV2	489	609	0.05%	0.007%
52	10.653	1566	1569	1570	rBV2	675	623	0.05%	0.007%
53	10.738	1582	1583	1587	rBV2	552	777	0.06%	0.009%
54	10.805	1589	1594	1600	rVV3	467	1011	0.08%	0.012%
55	10.854	1600	1602	1605	rVB	683	675	0.06%	0.008%
56	10.896	1608	1609	1613	rBV2	310	447	0.04%	0.005%
57	10.927	1613	1614	1617	rVV	519	441	0.04%	0.005%
58	10.970	1617	1621	1624	rVB4	819	1154	0.09%	0.013%
59	10.994	1624	1625	1627	rBV	547	397	0.03%	0.005%
60	11.073	1636	1638	1641	rVB3	391	461	0.04%	0.005%
61	11.189	1652	1657	1672	rVV	432710	543197	44.67%	6.261%
62	11.378	1685	1688	1691	rBV2	674	806	0.07%	0.009%
63	11.409	1691	1693	1695	rBV2	612	487	0.04%	0.006%
64	11.457	1698	1701	1702	rBV2	771	1026	0.08%	0.012%
65	11.555	1715	1717	1720	rBV2	528	409	0.03%	0.005%
66	11.610	1725	1726	1728	rVB	636	344	0.03%	0.004%
67	11.640	1728	1731	1732	rBV2	510	489	0.04%	0.006%
68	11.665	1732	1735	1738	rVV3	313	381	0.03%	0.004%
69	11.756	1748	1750	1753	rVV2	791	853	0.07%	0.010%
70	11.890	1770	1772	1775	rBV2	301	331	0.03%	0.004%
71	11.975	1783	1786	1788	rBV3	1082	1065	0.09%	0.012%
72	12.018	1788	1793	1804	rVV	558384	732994	60.27%	8.448%
73	12.317	1837	1842	1854	rVV	591611	756416	62.20%	8.718%
74	12.683	1900	1902	1904	rVB2	444	395	0.03%	0.005%
75	12.762	1912	1915	1918	rBV2	1232	1476	0.12%	0.017%
76	12.957	1946	1947	1950	rVV2	390	395	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043900.D
 Acq On : 19 Nov 2024 14:59
 Operator : JC/MD
 Sample : P4782-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

77	12.988	1950	1952	1953	rVV	361	309	0.03%	0.004%
78	13.122	1970	1974	1976	rBV2	529	578	0.05%	0.007%
79	13.146	1976	1978	1981	rBV	270	388	0.03%	0.004%
80	13.323	2005	2007	2009	rVV2	432	315	0.03%	0.004%
81	13.445	2024	2027	2032	rVB4	506	860	0.07%	0.010%
82	13.554	2043	2045	2047	rBV2	344	417	0.03%	0.005%
83	13.597	2051	2052	2054	rBV2	369	333	0.03%	0.004%
84	13.658	2059	2062	2063	rBV2	409	395	0.03%	0.005%
85	13.719	2070	2072	2073	rBV	480	319	0.03%	0.004%
86	13.786	2080	2083	2084	rBV2	822	699	0.06%	0.008%
87	14.134	2135	2140	2144	rBV	1342	1878	0.15%	0.022%
88	14.219	2152	2154	2155	rBV	429	357	0.03%	0.004%
89	14.359	2175	2177	2178	rVB	673	330	0.03%	0.004%
90	14.487	2196	2198	2200	rBV2	497	600	0.05%	0.007%
91	14.554	2207	2209	2210	rVB2	621	361	0.03%	0.004%
92	14.951	2269	2274	2277	rBV4	808	1268	0.10%	0.015%
93	15.164	2307	2309	2311	rBV2	755	631	0.05%	0.007%
94	15.298	2329	2331	2332	rBV2	587	454	0.04%	0.005%
95	15.505	2363	2365	2367	rBV2	692	564	0.05%	0.007%
96	15.707	2396	2398	2399	rBV	797	425	0.03%	0.005%
97	15.810	2413	2415	2420	rBV4	474	617	0.05%	0.007%
98	15.932	2433	2435	2439	rBV4	397	505	0.04%	0.006%
99	16.481	2523	2525	2526	rBV2	842	467	0.04%	0.005%
100	16.499	2526	2528	2530	rVV	715	438	0.04%	0.005%

Sum of corrected areas: 8676361




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043900.D
Acq On : 19 Nov 2024 14:59
Operator : JC/MD
Sample : P4782-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

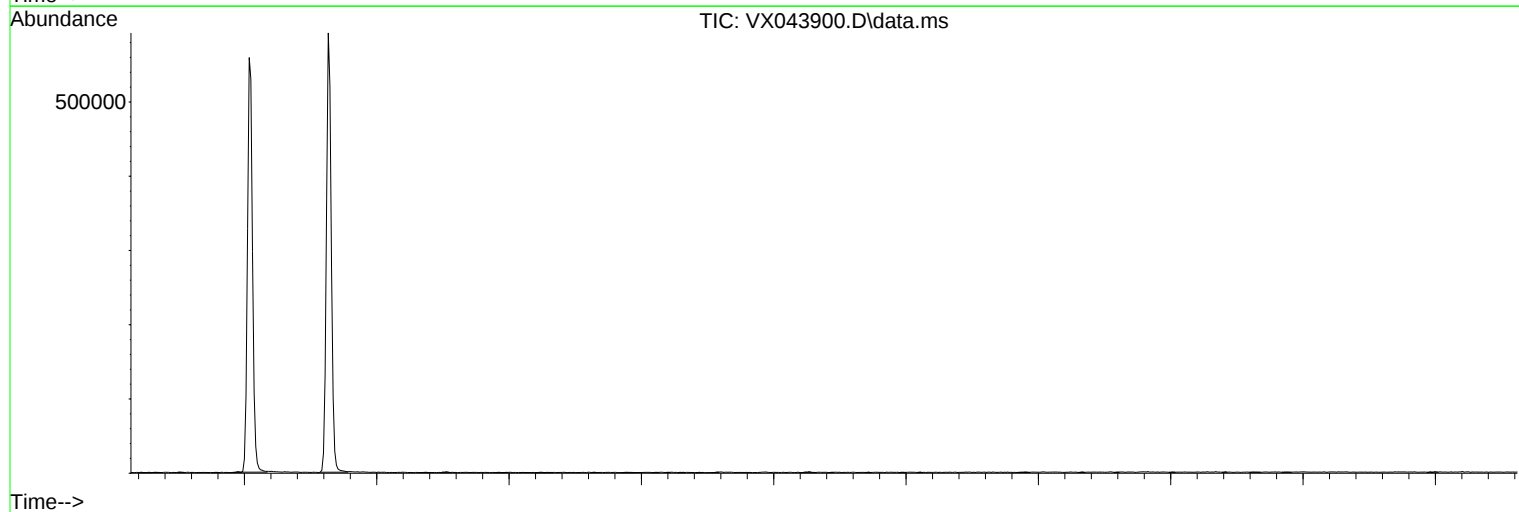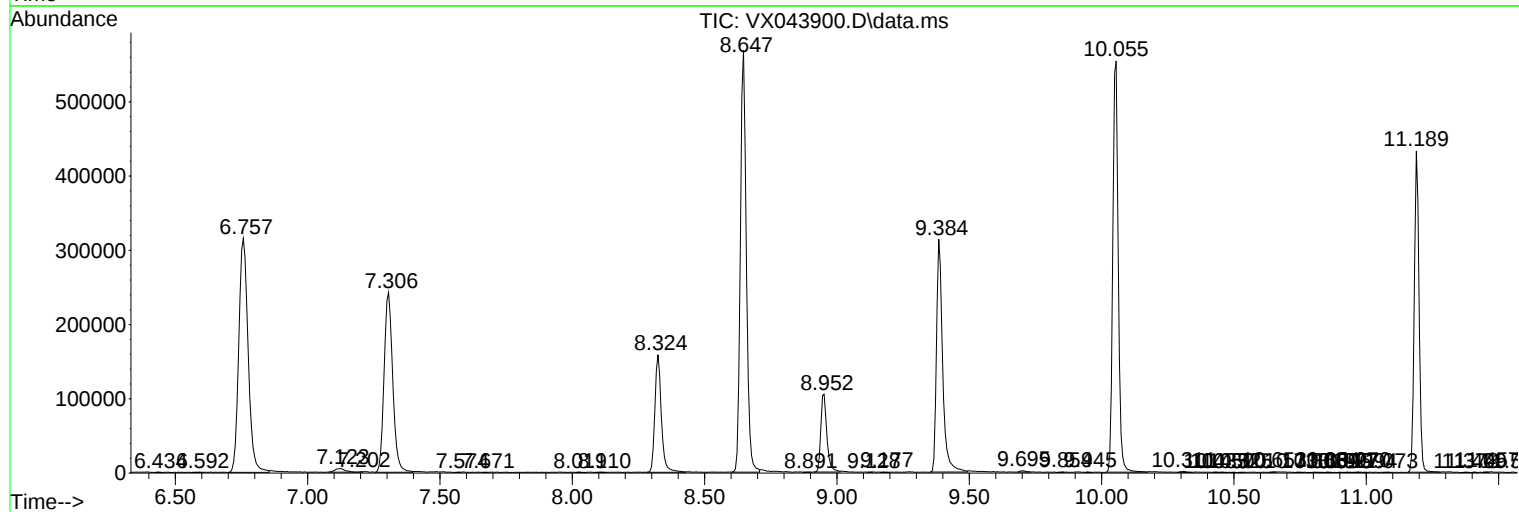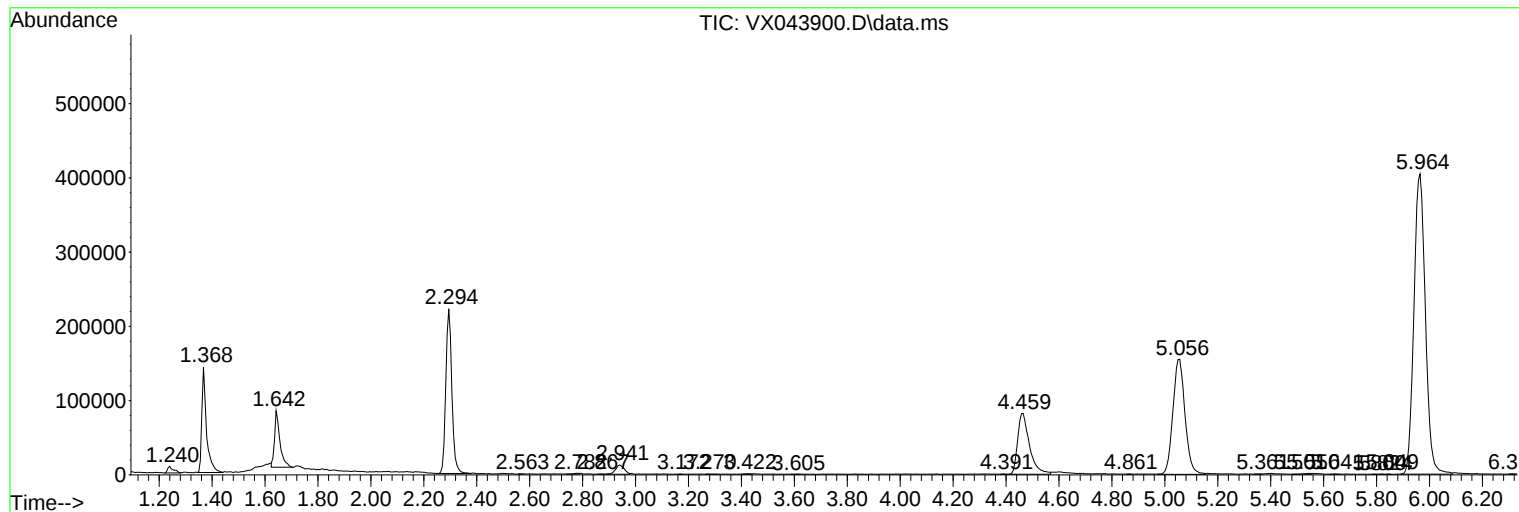

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043900.D
Acq On : 19 Nov 2024 14:59
Operator : JC/MD
Sample : P4782-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043900.D
Acq On : 19 Nov 2024 14:59
Operator : JC/MD
Sample : P4782-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
