

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043904.D
 Acq On : 19 Nov 2024 16:43
 Operator : JC/MD
 Sample : VIBLK682
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

Signal : TIC: VX043904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	9489	9078	0.74%	0.110%
2	1.368	42	46	56	rVB	131783	157751	12.92%	1.903%
3	1.648	88	92	101	rVB	78968	113857	9.32%	1.374%
4	2.294	192	198	208	rBV	225276	353806	28.98%	4.269%
5	2.447	222	223	225	rVB	619	353	0.03%	0.004%
6	2.489	228	230	231	rBV2	639	330	0.03%	0.004%
7	2.617	247	251	252	rBV2	401	435	0.04%	0.005%
8	2.776	275	277	279	rBV3	734	725	0.06%	0.009%
9	2.940	296	304	315	rBV	11339	26659	2.18%	0.322%
10	3.178	341	343	345	rBV2	465	332	0.03%	0.004%
11	3.203	345	347	350	rBV3	359	412	0.03%	0.005%
12	3.300	362	363	366	rBV	484	358	0.03%	0.004%
13	3.434	380	385	389	rVV4	828	1600	0.13%	0.019%
14	3.648	418	420	422	rBV2	404	329	0.03%	0.004%
15	3.703	425	429	430	rBV2	412	364	0.03%	0.004%
16	3.745	435	436	439	rBV2	467	340	0.03%	0.004%
17	3.959	467	471	473	rBV3	373	488	0.04%	0.006%
18	4.465	545	554	570	rBV2	76641	245257	20.09%	2.959%
19	4.910	625	627	630	rBV2	314	404	0.03%	0.005%
20	5.050	639	650	670	rVB	155186	485636	39.77%	5.860%
21	5.385	700	705	708	rBV3	946	1341	0.11%	0.016%
22	5.477	718	720	721	rBV2	413	330	0.03%	0.004%
23	5.958	786	799	817	rBV2	406278	1221024	100.00%	14.733%
24	6.220	840	842	844	rBV2	474	330	0.03%	0.004%
25	6.263	847	849	852	rBV3	373	379	0.03%	0.005%
26	6.342	860	862	863	rBV2	467	452	0.04%	0.005%
27	6.367	864	866	870	rVV4	861	805	0.07%	0.010%
28	6.397	870	871	874	rVB2	418	332	0.03%	0.004%
29	6.476	881	884	887	rVB2	468	507	0.04%	0.006%
30	6.617	903	907	908	rBV2	495	563	0.05%	0.007%
31	6.659	911	914	918	rVB2	529	748	0.06%	0.009%
32	6.757	918	930	948	rBV	306860	736775	60.34%	8.890%
33	7.117	983	989	1000	rVB9	4710	12374	1.01%	0.149%
34	7.214	1002	1005	1008	rBV3	992	1098	0.09%	0.013%
35	7.306	1011	1020	1038	rBV	246353	547468	44.84%	6.606%
36	7.482	1047	1049	1050	rBV	825	645	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043904.D
 Acq On : 19 Nov 2024 16:43
 Operator : JC/MD
 Sample : VIBLK682
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

37	7.604	1067	1069	1072	rVB2	564	525	0.04%	0.006%
38	7.641	1072	1075	1077	rBV3	370	409	0.03%	0.005%
39	7.671	1079	1080	1083	rVB	568	491	0.04%	0.006%
40	7.702	1083	1085	1088	rBV2	372	472	0.04%	0.006%
41	7.775	1094	1097	1099	rVB2	534	494	0.04%	0.006%
42	7.927	1118	1122	1124	rVV2	596	672	0.06%	0.008%
43	7.976	1128	1130	1132	rVV2	485	359	0.03%	0.004%
44	8.025	1136	1138	1141	rVV2	588	510	0.04%	0.006%
45	8.232	1168	1172	1175	rVV	319	399	0.03%	0.005%
46	8.324	1181	1187	1200	rBV	156105	270375	22.14%	3.262%
47	8.482	1211	1213	1217	rBV3	483	611	0.05%	0.007%
48	8.537	1219	1222	1228	rBV4	525	1174	0.10%	0.014%
49	8.647	1233	1240	1255	rBV	576399	888995	72.81%	10.726%
50	8.872	1276	1277	1280	rBV2	514	389	0.03%	0.005%
51	8.945	1284	1289	1303	rBV	109085	173279	14.19%	2.091%
52	9.232	1334	1336	1338	rBV2	433	404	0.03%	0.005%
53	9.269	1340	1342	1345	rVB2	577	615	0.05%	0.007%
54	9.384	1356	1361	1375	rBV	322051	502200	41.13%	6.059%
55	9.622	1398	1400	1402	rBV2	409	345	0.03%	0.004%
56	10.049	1465	1470	1479	rBV	517733	740272	60.63%	8.932%
57	10.354	1519	1520	1524	rBV4	623	453	0.04%	0.005%
58	10.427	1530	1532	1536	rVB3	677	562	0.05%	0.007%
59	10.573	1553	1556	1560	rVB2	492	559	0.05%	0.007%
60	10.750	1583	1585	1587	rBV3	546	470	0.04%	0.006%
61	10.787	1590	1591	1594	rBV2	545	488	0.04%	0.006%
62	10.878	1602	1606	1607	rBV3	442	473	0.04%	0.006%
63	10.963	1619	1620	1622	rBV	466	465	0.04%	0.006%
64	11.024	1628	1630	1631	rBV2	493	385	0.03%	0.005%
65	11.189	1652	1657	1666	rVV	401889	510716	41.83%	6.162%
66	11.408	1690	1693	1696	rBV2	474	657	0.05%	0.008%
67	11.457	1699	1701	1704	rVB3	507	412	0.03%	0.005%
68	11.524	1709	1712	1715	rVV2	570	650	0.05%	0.008%
69	11.573	1718	1720	1723	rVV3	466	438	0.04%	0.005%
70	11.616	1723	1727	1728	rVB3	365	407	0.03%	0.005%
71	11.695	1739	1740	1742	rBV2	505	345	0.03%	0.004%
72	11.969	1783	1785	1788	rBV3	844	1158	0.09%	0.014%
73	12.018	1788	1793	1803	rBV	464354	606466	49.67%	7.318%
74	12.317	1837	1842	1857	rBV	500315	641239	52.52%	7.737%
75	12.616	1889	1891	1895	rBV3	512	463	0.04%	0.006%
76	12.762	1912	1915	1917	rVV	883	958	0.08%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
 Data File : VX043904.D
 Acq On : 19 Nov 2024 16:43
 Operator : JC/MD
 Sample : VIBLK682
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK682

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

77	12.890	1934	1936	1940	rVB3	564	668	0.05%	0.008%
78	12.963	1946	1948	1949	rVV2	445	326	0.03%	0.004%
79	13.036	1956	1960	1963	rBV3	439	474	0.04%	0.006%
80	13.274	1997	1999	2001	rVV2	376	380	0.03%	0.005%
81	13.323	2004	2007	2008	rVB2	536	448	0.04%	0.005%
82	13.353	2008	2012	2015	rBV2	468	792	0.06%	0.010%
83	13.378	2015	2016	2019	rBV2	368	365	0.03%	0.004%
84	13.426	2022	2024	2028	rVV2	341	380	0.03%	0.005%
85	13.530	2039	2041	2044	rVB3	557	378	0.03%	0.005%
86	13.573	2047	2048	2052	rBV2	557	550	0.05%	0.007%
87	13.646	2059	2060	2062	rBV2	526	398	0.03%	0.005%
88	13.689	2064	2067	2069	rVB	527	558	0.05%	0.007%
89	13.926	2104	2106	2109	rBV2	395	450	0.04%	0.005%
90	13.969	2111	2113	2116	rVV3	505	558	0.05%	0.007%
91	14.134	2136	2140	2143	rVB2	1214	1732	0.14%	0.021%
92	14.377	2178	2180	2181	rBV2	388	342	0.03%	0.004%
93	14.591	2213	2215	2218	rBV	585	373	0.03%	0.005%
94	14.798	2246	2249	2250	rBV2	356	383	0.03%	0.005%
95	14.926	2268	2270	2272	rVB3	461	415	0.03%	0.005%
96	15.018	2281	2285	2290	rBV3	619	1216	0.10%	0.015%
97	15.103	2297	2299	2300	rBV2	498	397	0.03%	0.005%
98	15.627	2383	2385	2390	rBV4	631	761	0.06%	0.009%
99	16.371	2506	2507	2509	rBV	468	381	0.03%	0.005%
100	16.651	2551	2553	2556	rBV2	669	711	0.06%	0.009%

Sum of corrected areas: 8287875




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043904.D
Acq On : 19 Nov 2024 16:43
Operator : JC/MD
Sample : VIBLK682
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK682

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

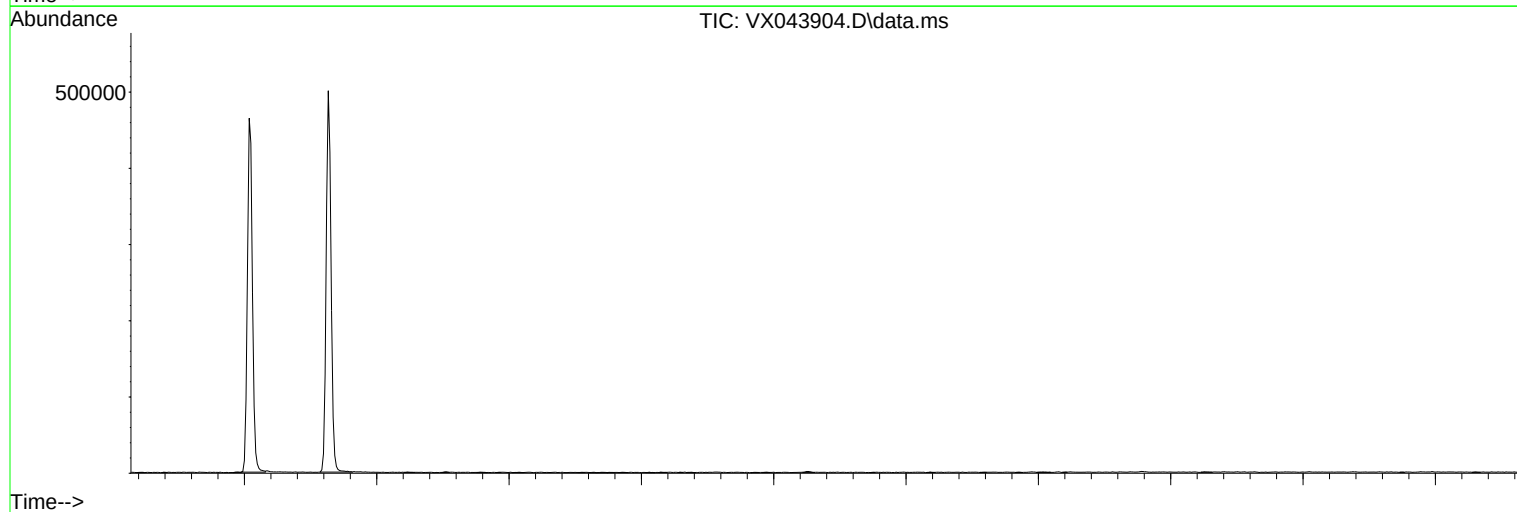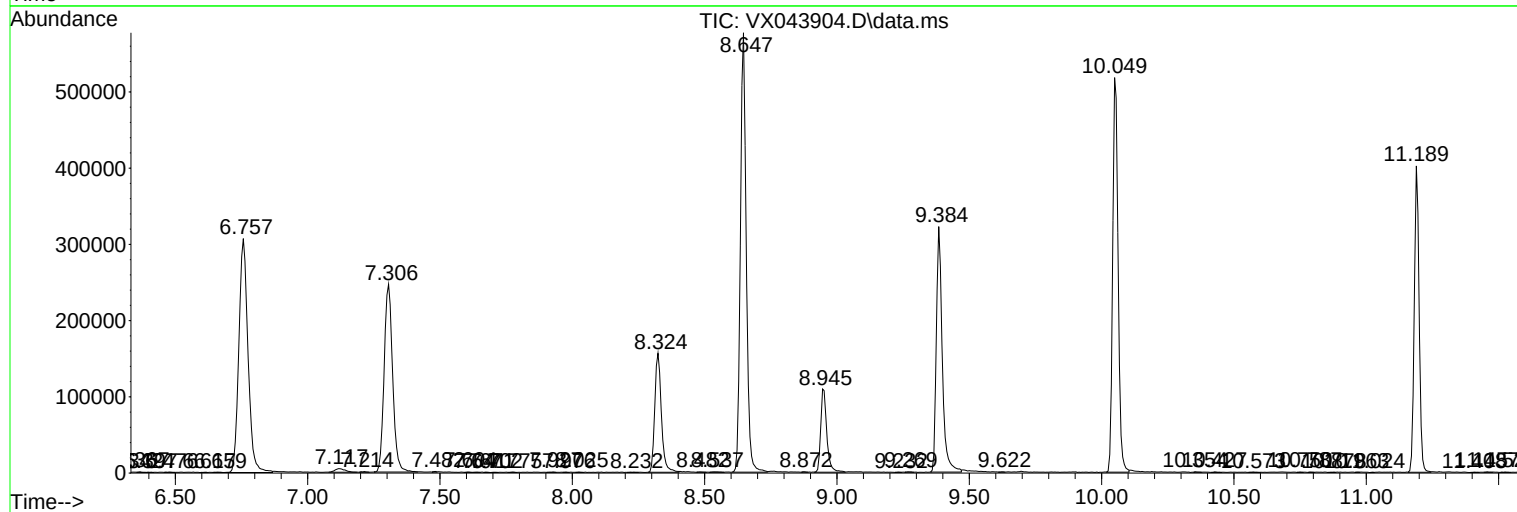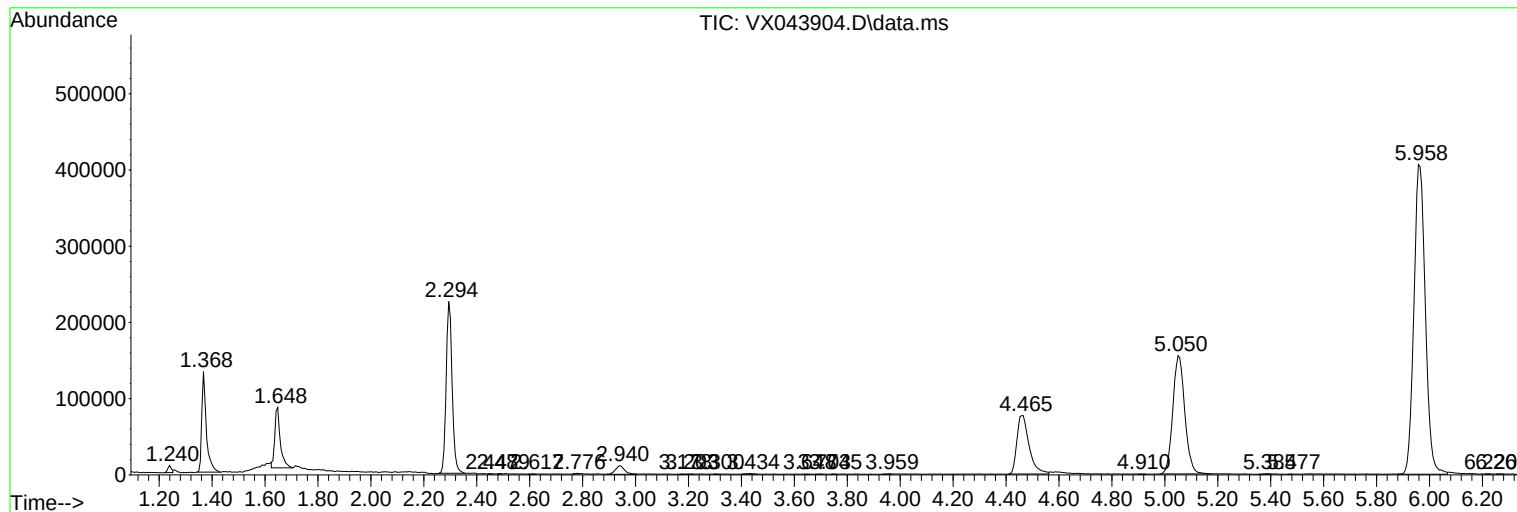

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043904.D
Acq On : 19 Nov 2024 16:43
Operator : JC/MD
Sample : VIBLK682
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK682

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043904.D
Acq On : 19 Nov 2024 16:43
Operator : JC/MD
Sample : VIBLK682
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK682

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
