
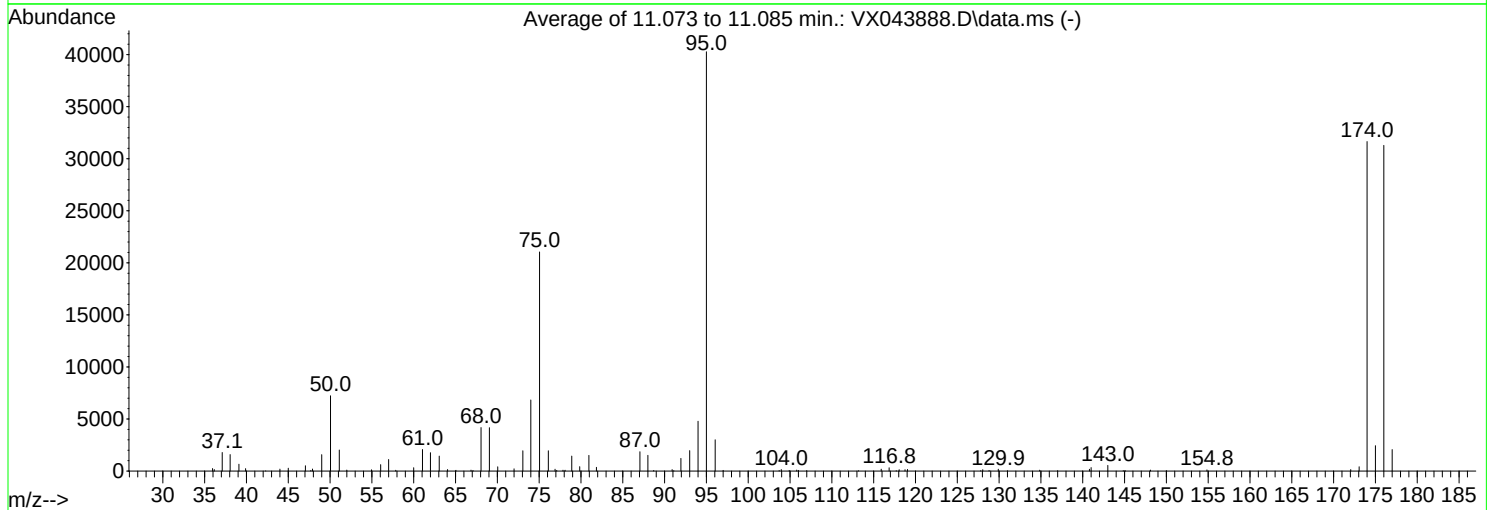


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111924\
Data File : VX043888.D
Acq On : 19 Nov 2024 08:05
Operator : JC/MD
Sample : BFB701
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB701

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111924WMA.M
Title : VOC Analysis
Last Update : Tue Nov 19 23:30:03 2024

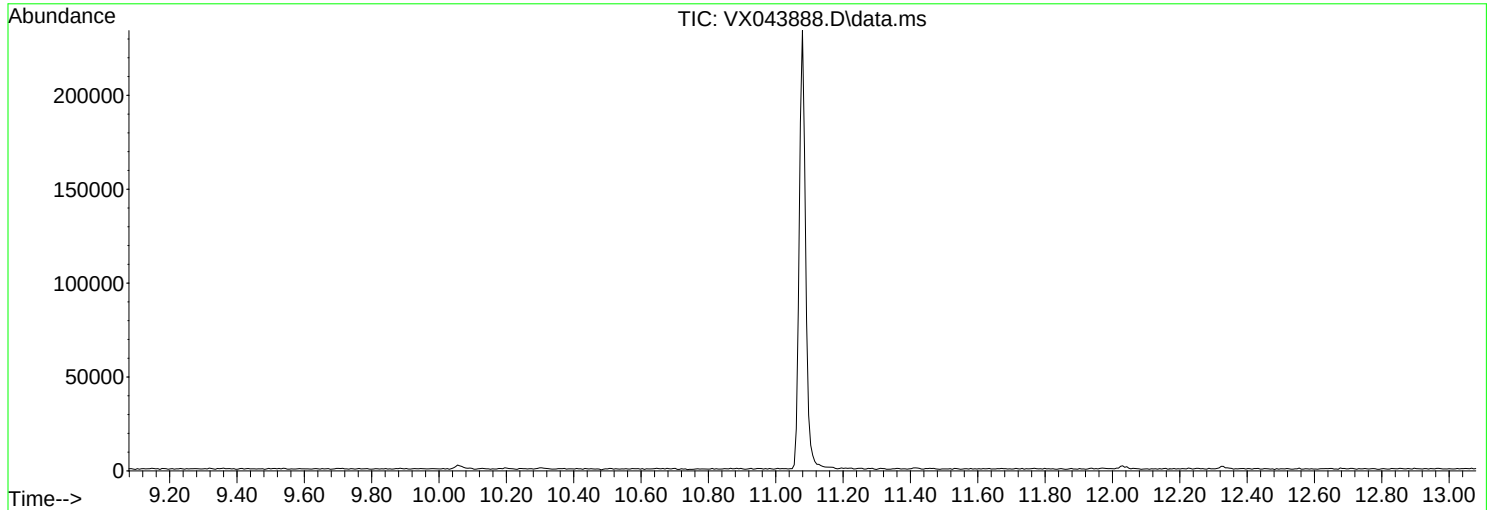

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	7233	PASS
75	95	30	80	52.3	21048	PASS
95	95	100	100	100.0	40277	PASS
96	95	5	9	7.5	3004	PASS
173	174	0.00	2	1.3	415	PASS
174	95	50	120	78.6	31648	PASS
175	174	5	9	7.7	2439	PASS
176	174	95	101	98.8	31280	PASS
177	176	5	9	6.6	2064	PASS

Scan 1633 (11.043 min): VX043888.D\data.ms
BFB701

m/z	Abundance
39.20	121.0
40.00	759.0
44.00	289.0

Instrument :
MSVOA_X
ClientSampleId :
BFB701

m/z	Abundance
36.00	465.0
37.10	2004.0
38.00	1488.0
39.10	906.0
39.90	705.0
44.00	424.0
44.90	267.0
47.10	601.0
47.70	177.0
49.00	1615.0
50.10	7335.0
51.10	2521.0
52.00	100.0
54.90	111.0
56.10	453.0
57.00	1094.0
57.90	101.0
60.00	353.0
61.10	2178.0
62.00	1659.0
63.10	1637.0
64.00	186.0
65.10	65.0
66.80	96.0
67.10	59.0
68.10	4239.0
69.10	4146.0
70.10	458.0
72.00	224.0
73.00	2050.0
74.00	6838.0
75.10	21576.0
76.10	2011.0
76.90	277.0
77.90	213.0
78.90	1549.0
79.90	422.0
81.00	1532.0
81.80	349.0
87.00	1574.0
88.00	1569.0
90.90	206.0
91.90	1262.0
93.00	2052.0
94.00	4884.0
95.00	37960.0
96.10	3106.0
97.00	99.0
103.90	242.0
105.80	119.0
107.00	63.0
113.20	112.0
115.80	178.0
116.80	364.0
118.10	133.0
118.80	216.0
127.80	109.0
128.80	53.0
129.90	202.0
134.90	104.0
140.80	521.0
143.10	373.0
144.90	60.0
148.10	91.0
154.90	114.0
172.00	72.0
173.00	258.0
174.00	26512.0
175.00	2345.0
176.00	26024.0
177.00	2015.0

Instrument :
MSVOA_X
ClientSampleId :
BFB701

m/z	Abundance
35.90	267.0
36.20	238.0
37.10	2235.0
38.10	2111.0
39.10	768.0
40.10	566.0
44.10	546.0
45.00	306.0
47.00	541.0
47.90	391.0
49.00	1915.0
50.00	9161.0
51.10	2266.0
52.00	122.0
55.00	111.0
56.00	819.0
57.00	1505.0
57.80	55.0
60.00	380.0
61.00	2369.0
62.00	2116.0
63.00	1464.0
64.00	128.0
65.10	91.0
66.90	184.0
68.00	5005.0
69.00	4943.0
70.00	436.0
72.00	247.0
73.10	2410.0
74.00	8296.0
75.10	24816.0
76.10	2385.0
76.90	270.0
78.10	174.0
78.90	1547.0
79.80	537.0
80.90	1712.0
81.90	407.0
87.00	2371.0
87.90	1933.0
90.90	224.0
91.90	1352.0
93.00	2040.0
94.00	5269.0
95.00	48704.0
96.00	3520.0
97.00	102.0
104.00	203.0
104.90	71.0
105.80	173.0
107.00	56.0
115.90	243.0
116.90	395.0
117.70	117.0
118.00	100.0
119.00	291.0
128.00	296.0
128.80	136.0
129.90	181.0
134.80	82.0
141.00	570.0
143.10	652.0
145.10	88.0
148.10	149.0
150.00	81.0
154.80	172.0
172.10	187.0
173.00	501.0
174.00	38400.0
175.00	3000.0
176.00	36576.0
177.00	2384.0

Instrument :
MSVOA_X
ClientSampleId :
BFB701

m/z	Abundance
36.10	203.0
37.10	1122.0
38.10	1165.0
39.10	669.0
40.00	683.0
42.30	57.0
44.10	465.0
45.10	257.0
47.10	404.0
47.90	204.0
49.00	1203.0
50.10	5204.0
51.00	1294.0
52.00	72.0
54.90	151.0
56.00	581.0
57.00	735.0
57.80	81.0
60.00	240.0
61.00	1667.0
62.00	1517.0
63.00	1216.0
64.10	134.0
64.90	72.0
67.10	81.0
68.00	3296.0
69.00	3425.0
70.10	335.0
72.00	181.0
73.00	1397.0
74.00	5350.0
75.00	16752.0
76.00	1448.0
77.10	201.0
77.70	52.0
78.10	82.0
78.90	1222.0
79.80	321.0
80.90	1273.0
81.90	332.0
87.10	1631.0
88.10	1040.0
88.70	190.0
91.10	122.0
92.00	1039.0
93.00	1805.0
94.00	4203.0
95.00	34168.0
96.10	2387.0
103.70	182.0
104.90	91.0
106.00	194.0
116.00	140.0
116.90	201.0
118.00	166.0
118.70	196.0
119.10	187.0
128.10	112.0
129.90	152.0
131.00	83.0
134.90	76.0
137.00	103.0
141.00	446.0
142.90	616.0
144.80	63.0
148.10	53.0
154.90	61.0
172.10	167.0
173.10	487.0
174.00	30032.0
175.00	1973.0
176.00	31240.0
177.00	1793.0

Instrument :
MSVOA_X
ClientSampleId :
BFB701