



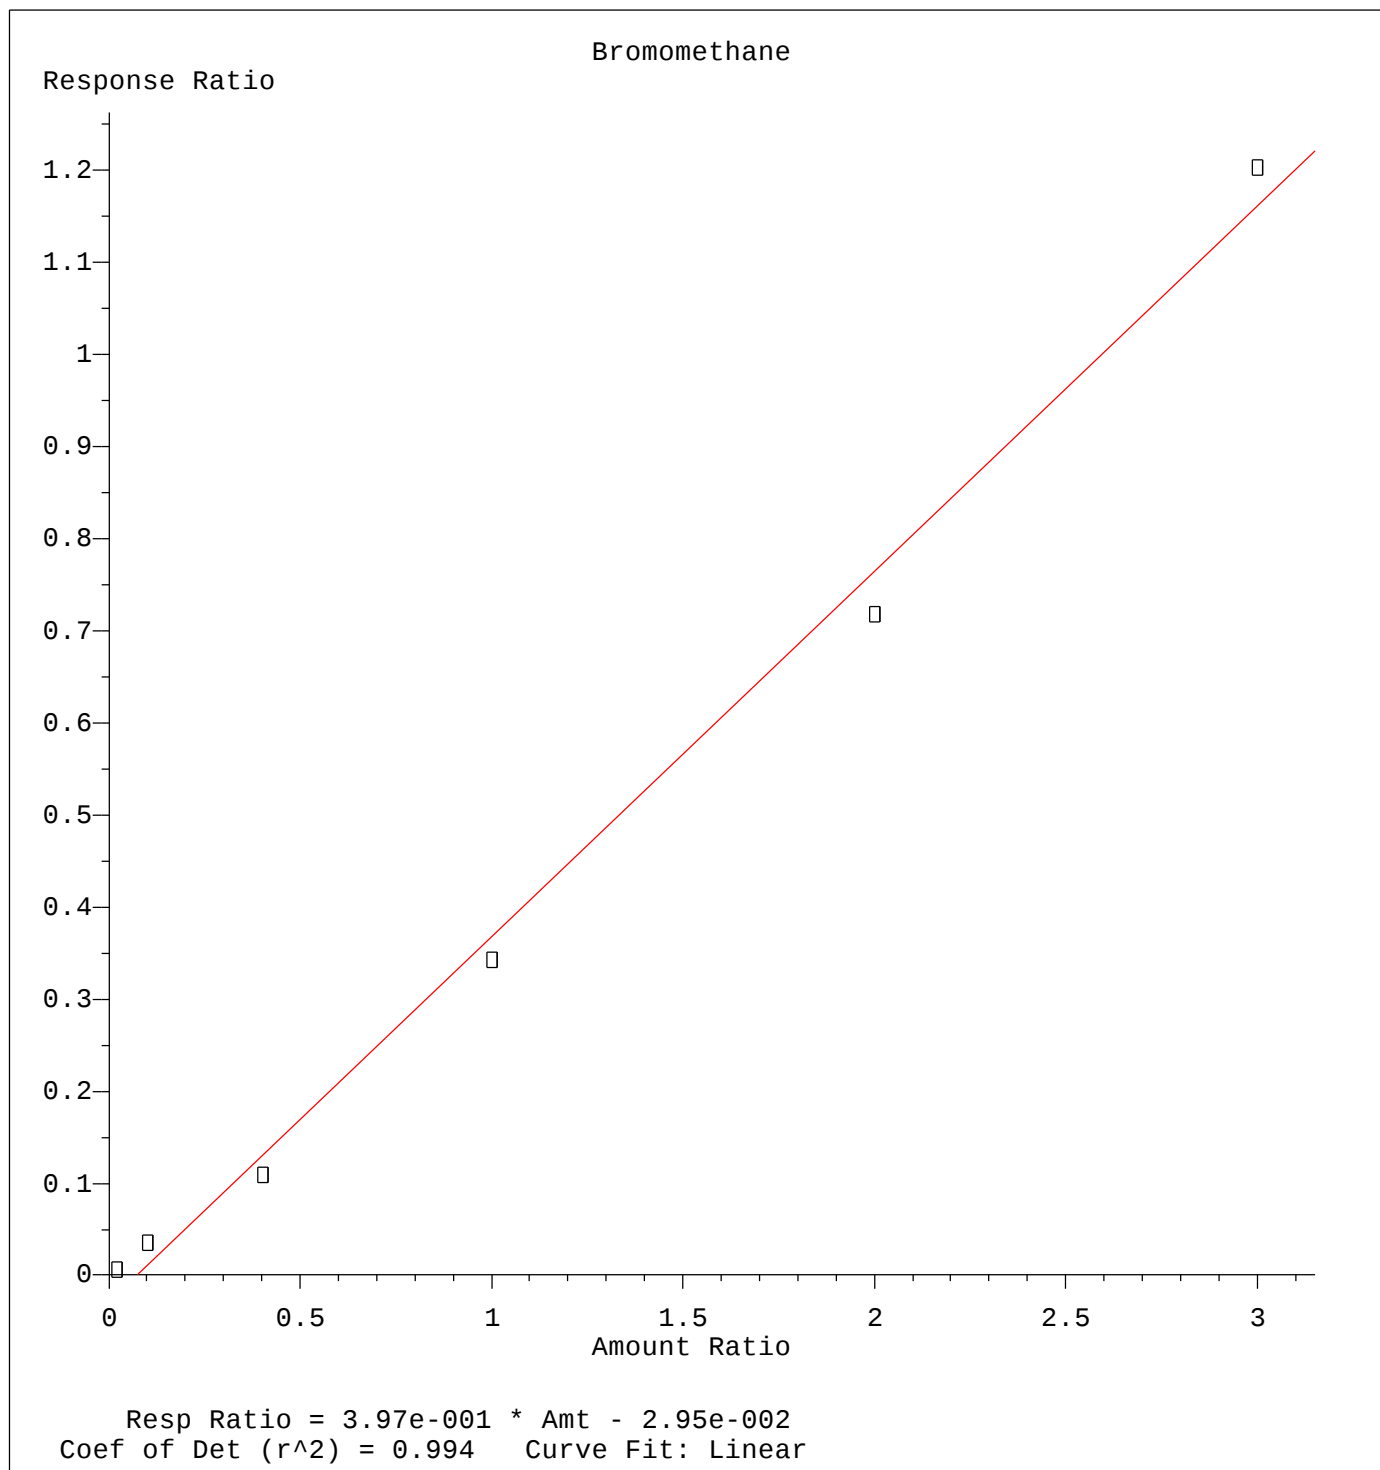

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Calibration Table Last Updated: Wed Nov 21 08:15:54 2018

Methylene Chloride

Response Ratio

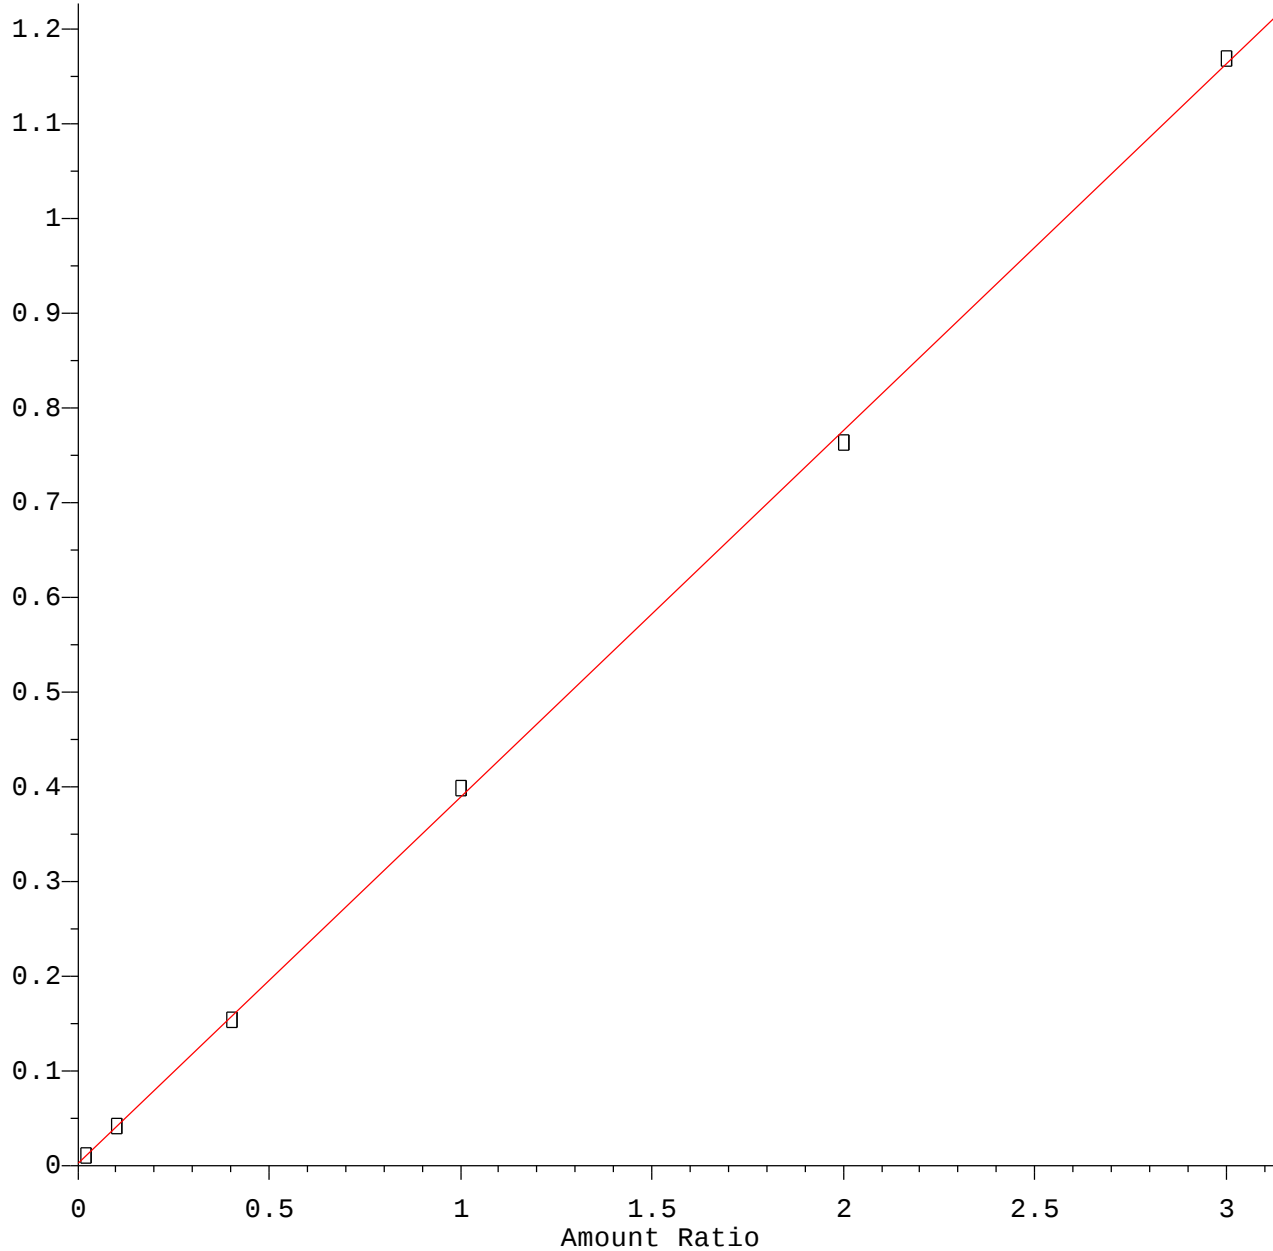


Resp Ratio = 3.86e-001 * Amt + 2.71e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Calibration Table Last Updated: Wed Nov 21 08:15:54 2018


Chloroethane

Response Ratio

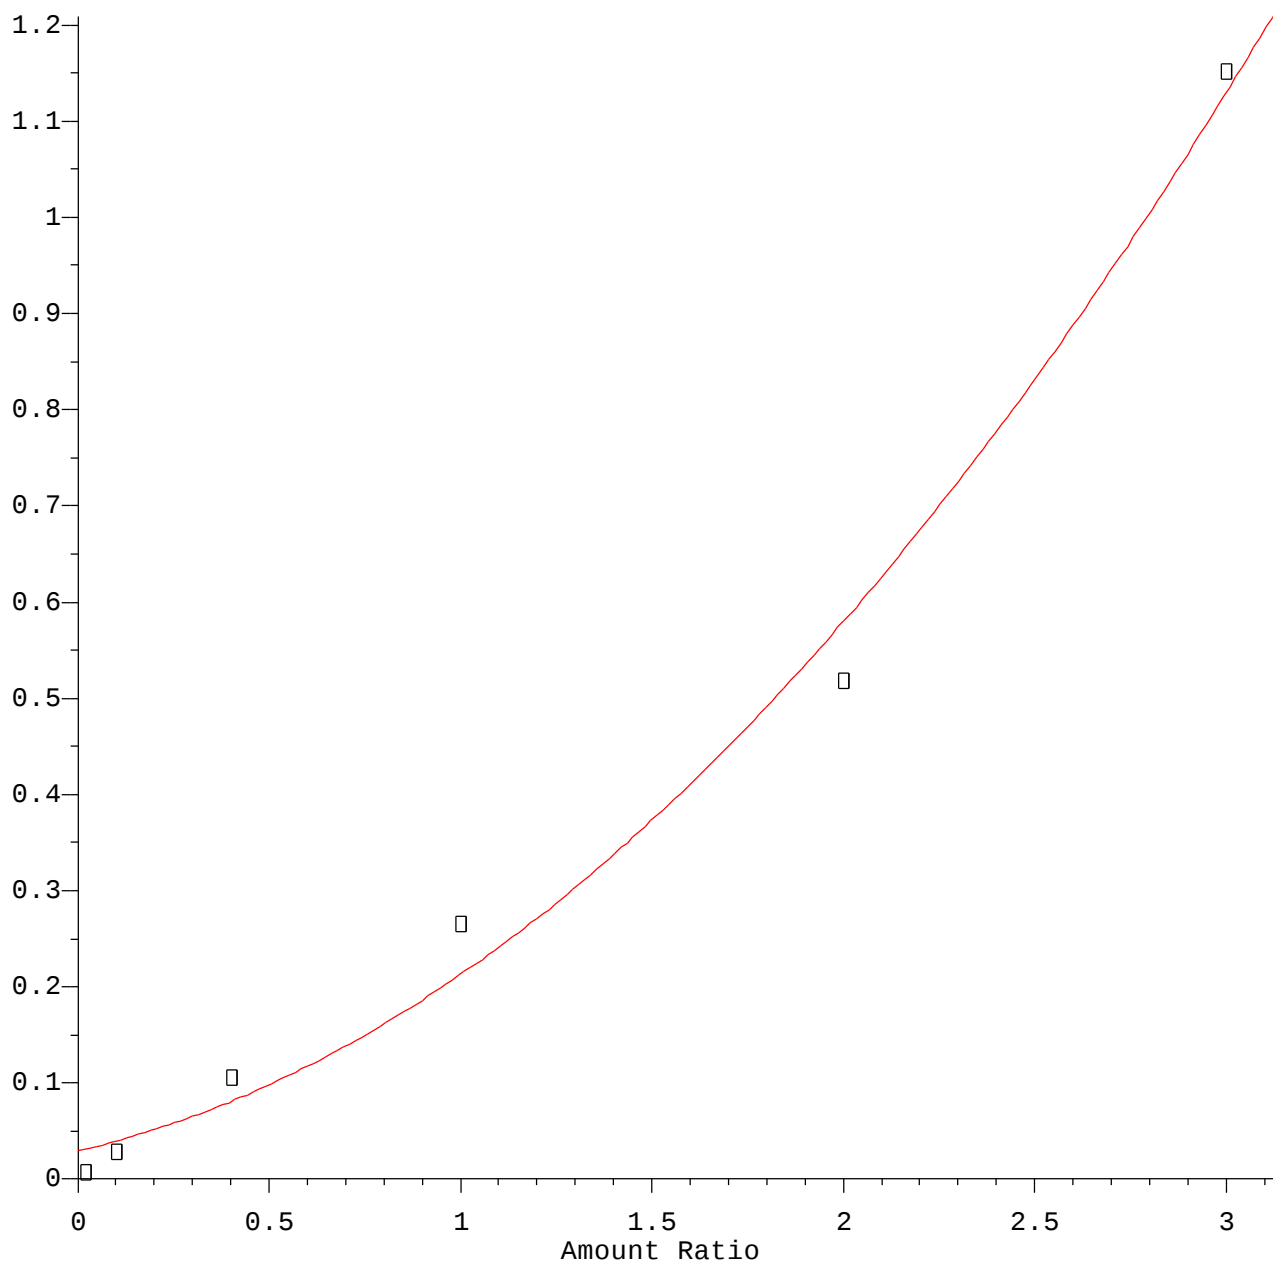

$R = 9.16e-002 A^2 + 9.21e-002 A + 2.89e-002$
Coef of Det (r^2) = 0.991 Curve Fit: Quadratic


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Calibration Table Last Updated: Wed Nov 21 08:15:54 2018

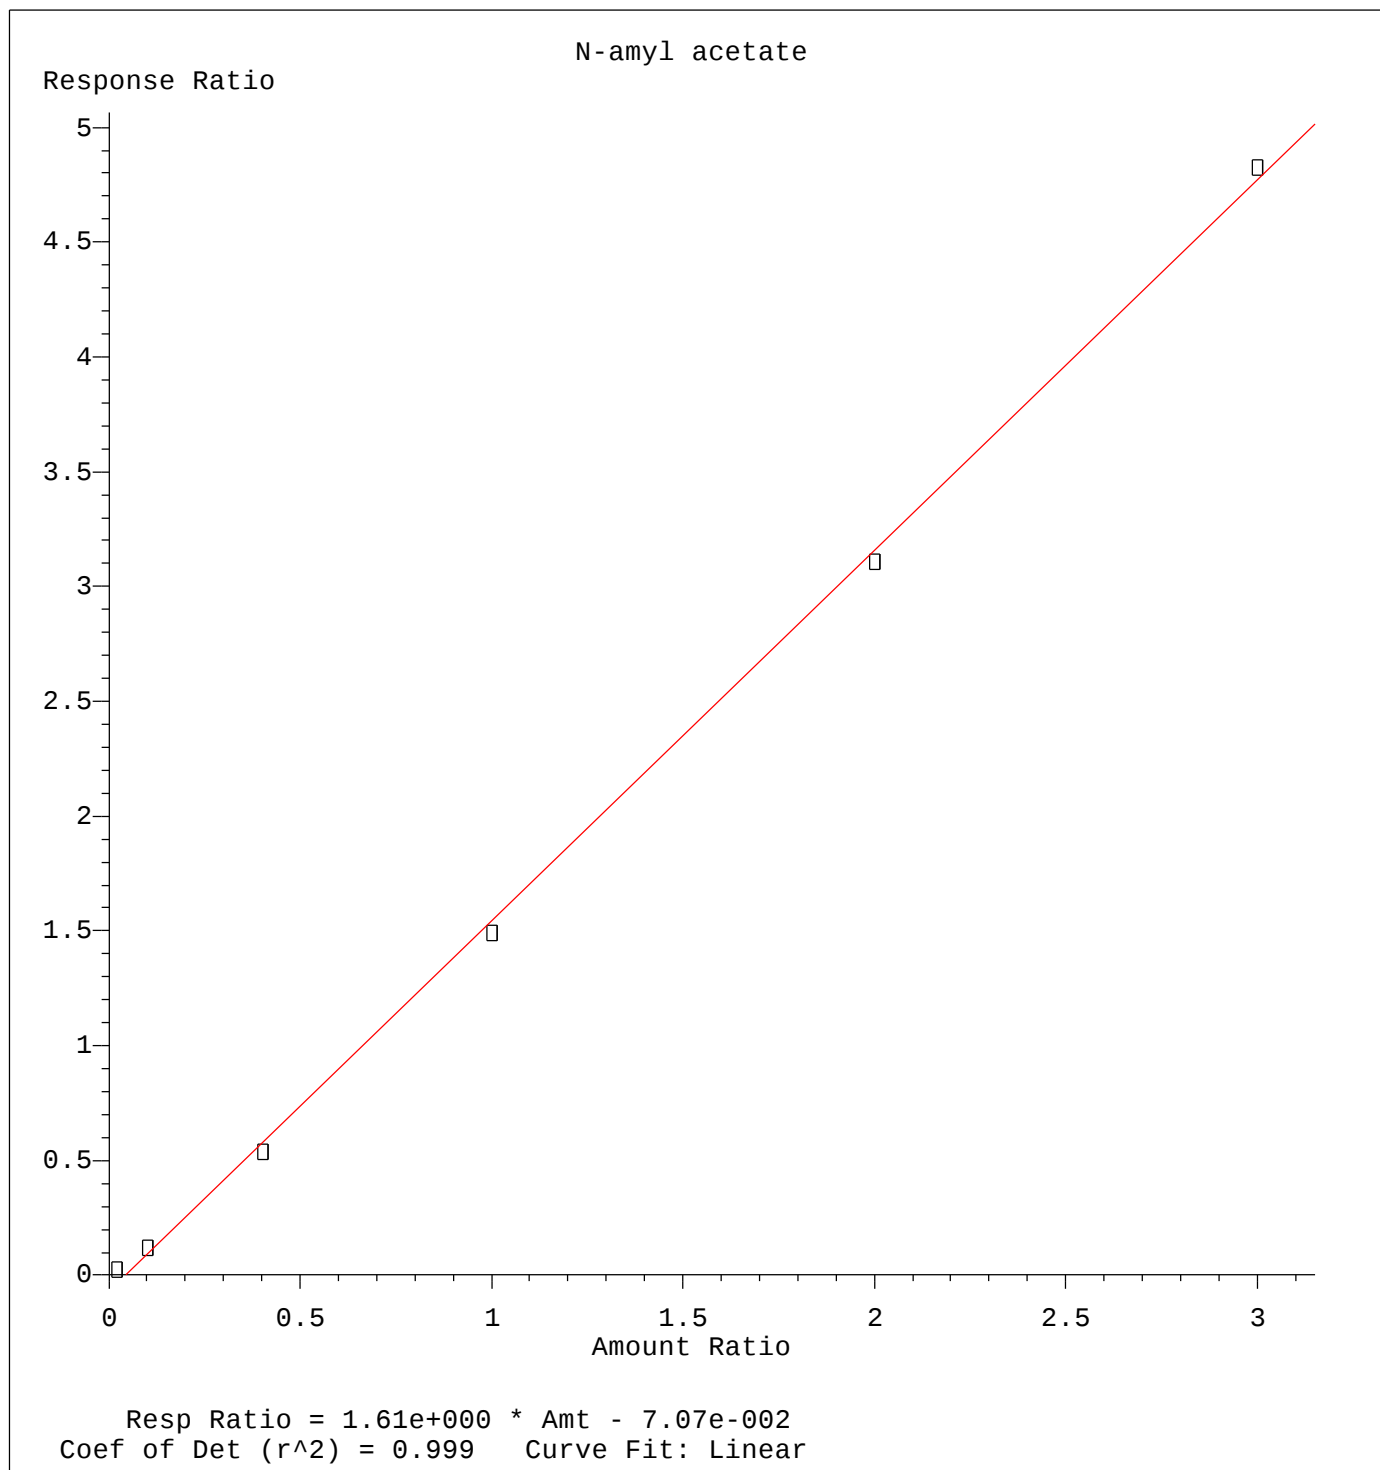

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Calibration Table Last Updated: Wed Nov 21 08:15:54 2018

2-Chloroethyl Vinyl ether

Response Ratio

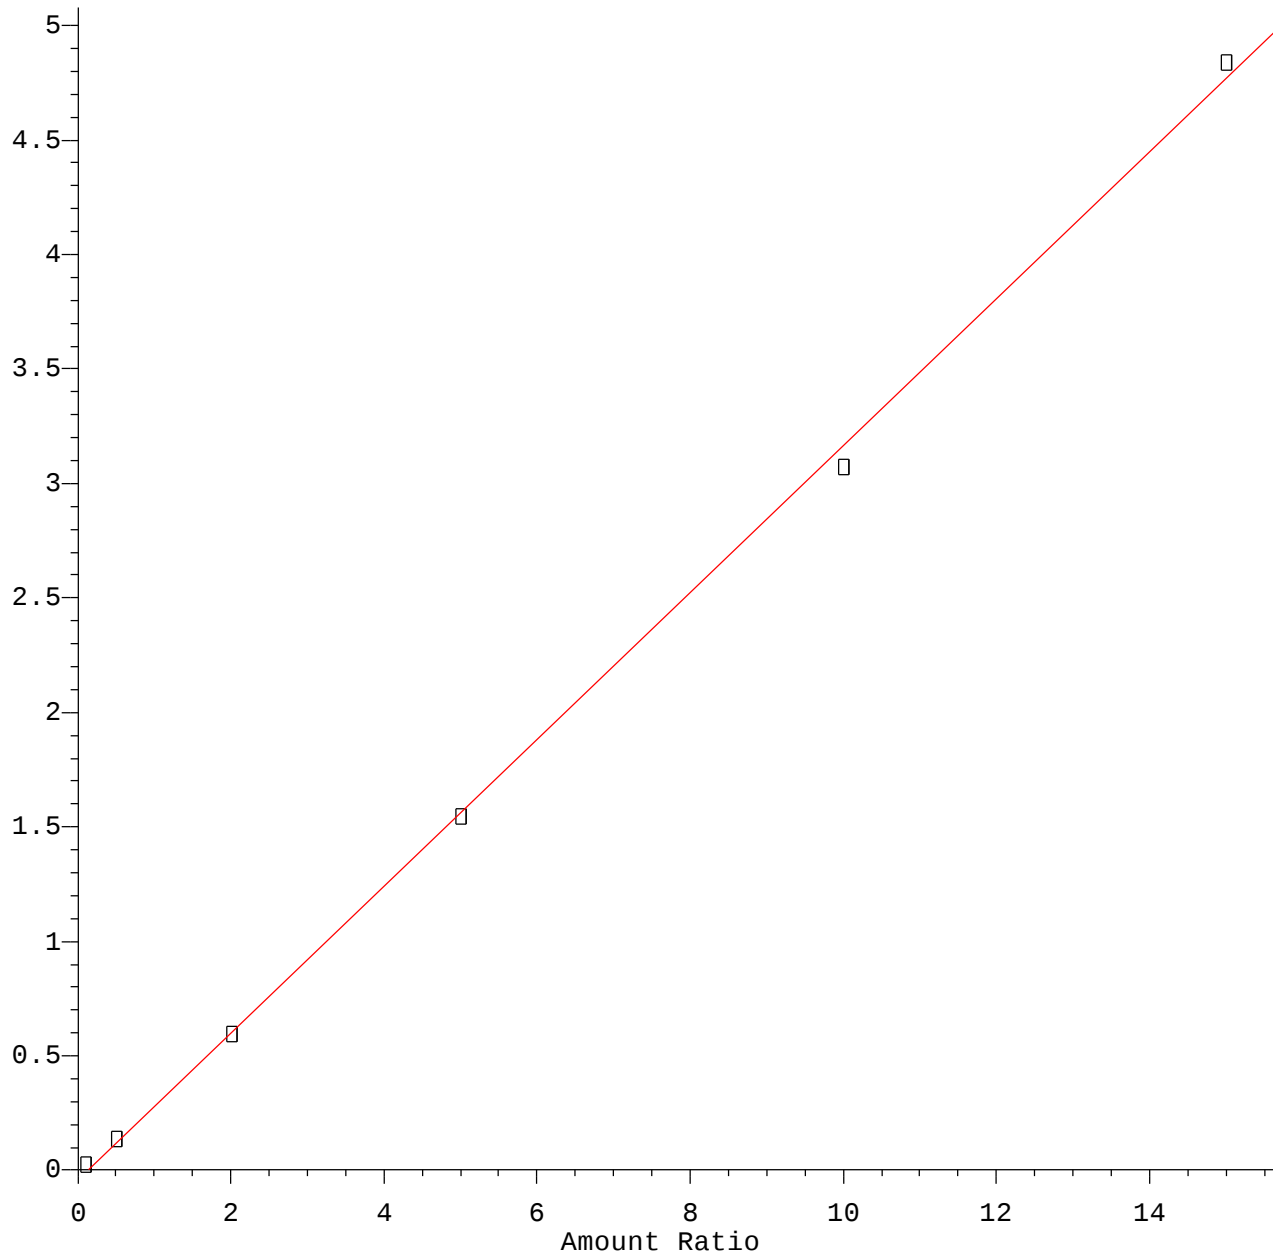


Resp Ratio = $3.21 \times 10^{-1} \times \text{Amt} - 4.31 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Calibration Table Last Updated: Wed Nov 21 08:15:54 2018

Ethyl methacrylate

Response Ratio

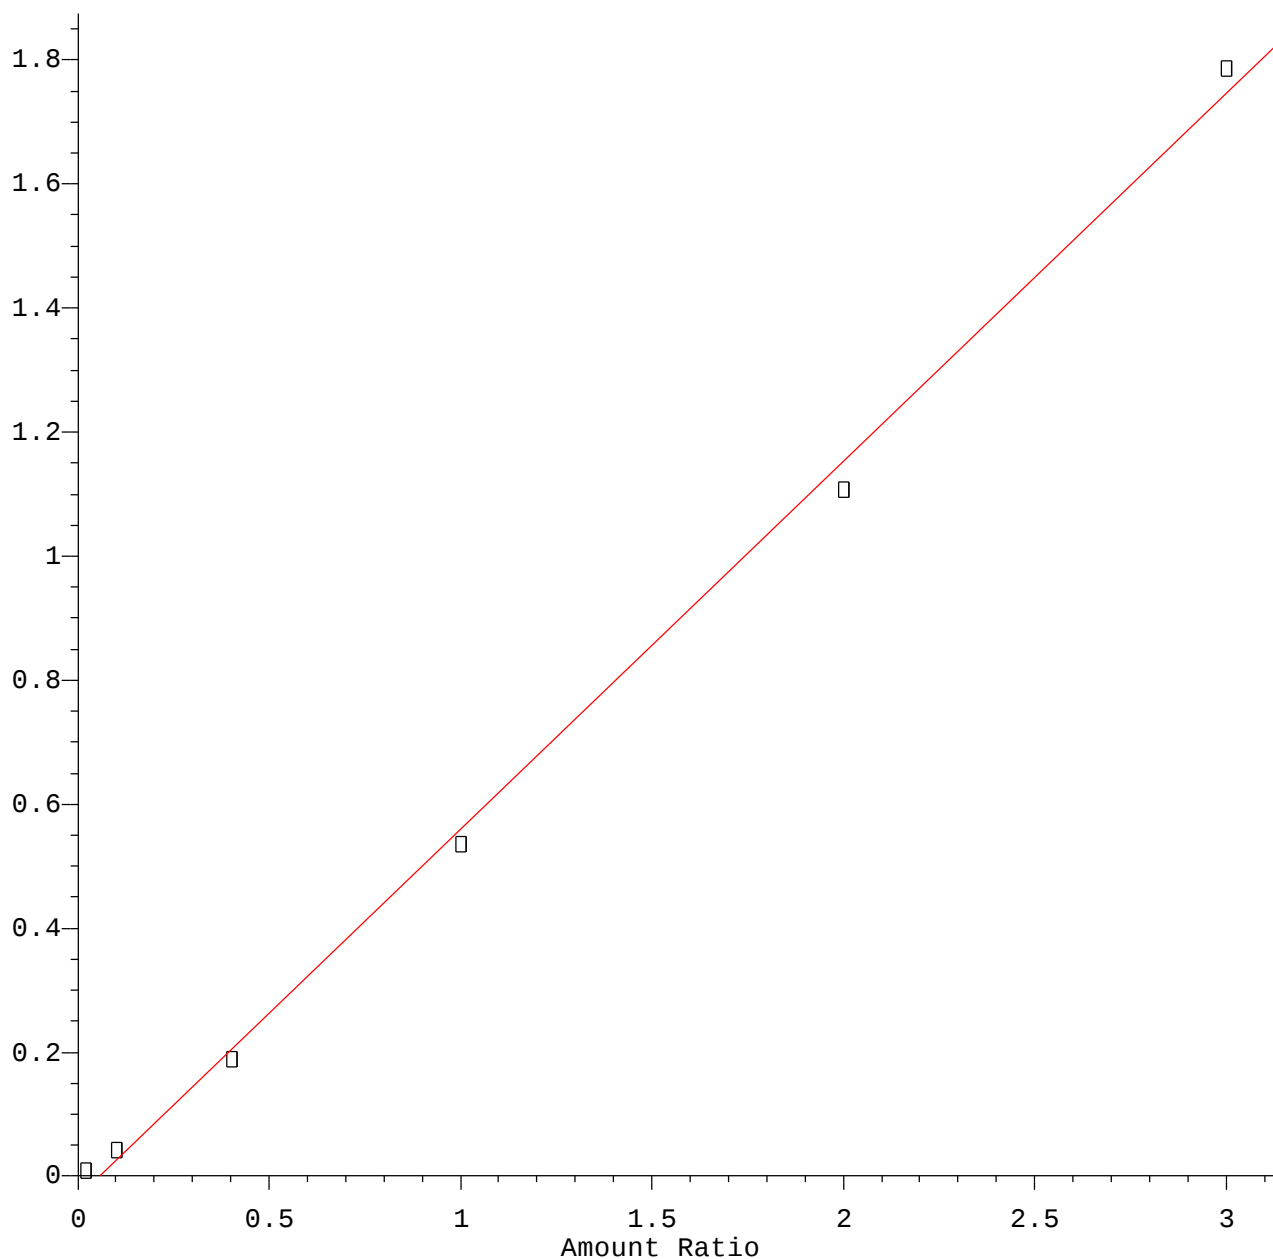

Resp Ratio = $5.93 \times 10^{-1} \times \text{Amt} - 3.40 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Calibration Table Last Updated: Wed Nov 21 08:15:54 2018