

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112019\
 Data File : VX013469.D
 Acq On : 20 Nov 2019 10:35
 Operator : JC/SP
 Sample : VX1120WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1120WBL01

Quant Time: Nov 21 01:03:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 02 07:06:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	668180	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	1096035	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	964853	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	436231	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	398791	50.38	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.76%	
35) Dibromofluoromethane	5.48	113	334365	48.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.28%	
50) Toluene-d8	8.71	98	1300539	50.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.36%	
62) 4-Bromofluorobenzene	11.13	95	431995	46.19	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.38%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112019\
Data File : VX013469.D
Acq On : 20 Nov 2019 10:35
Operator : JC/SP
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120WBL01

Quant Time: Nov 21 01:03:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 02 07:06:38 2019
Response via : Initial Calibration

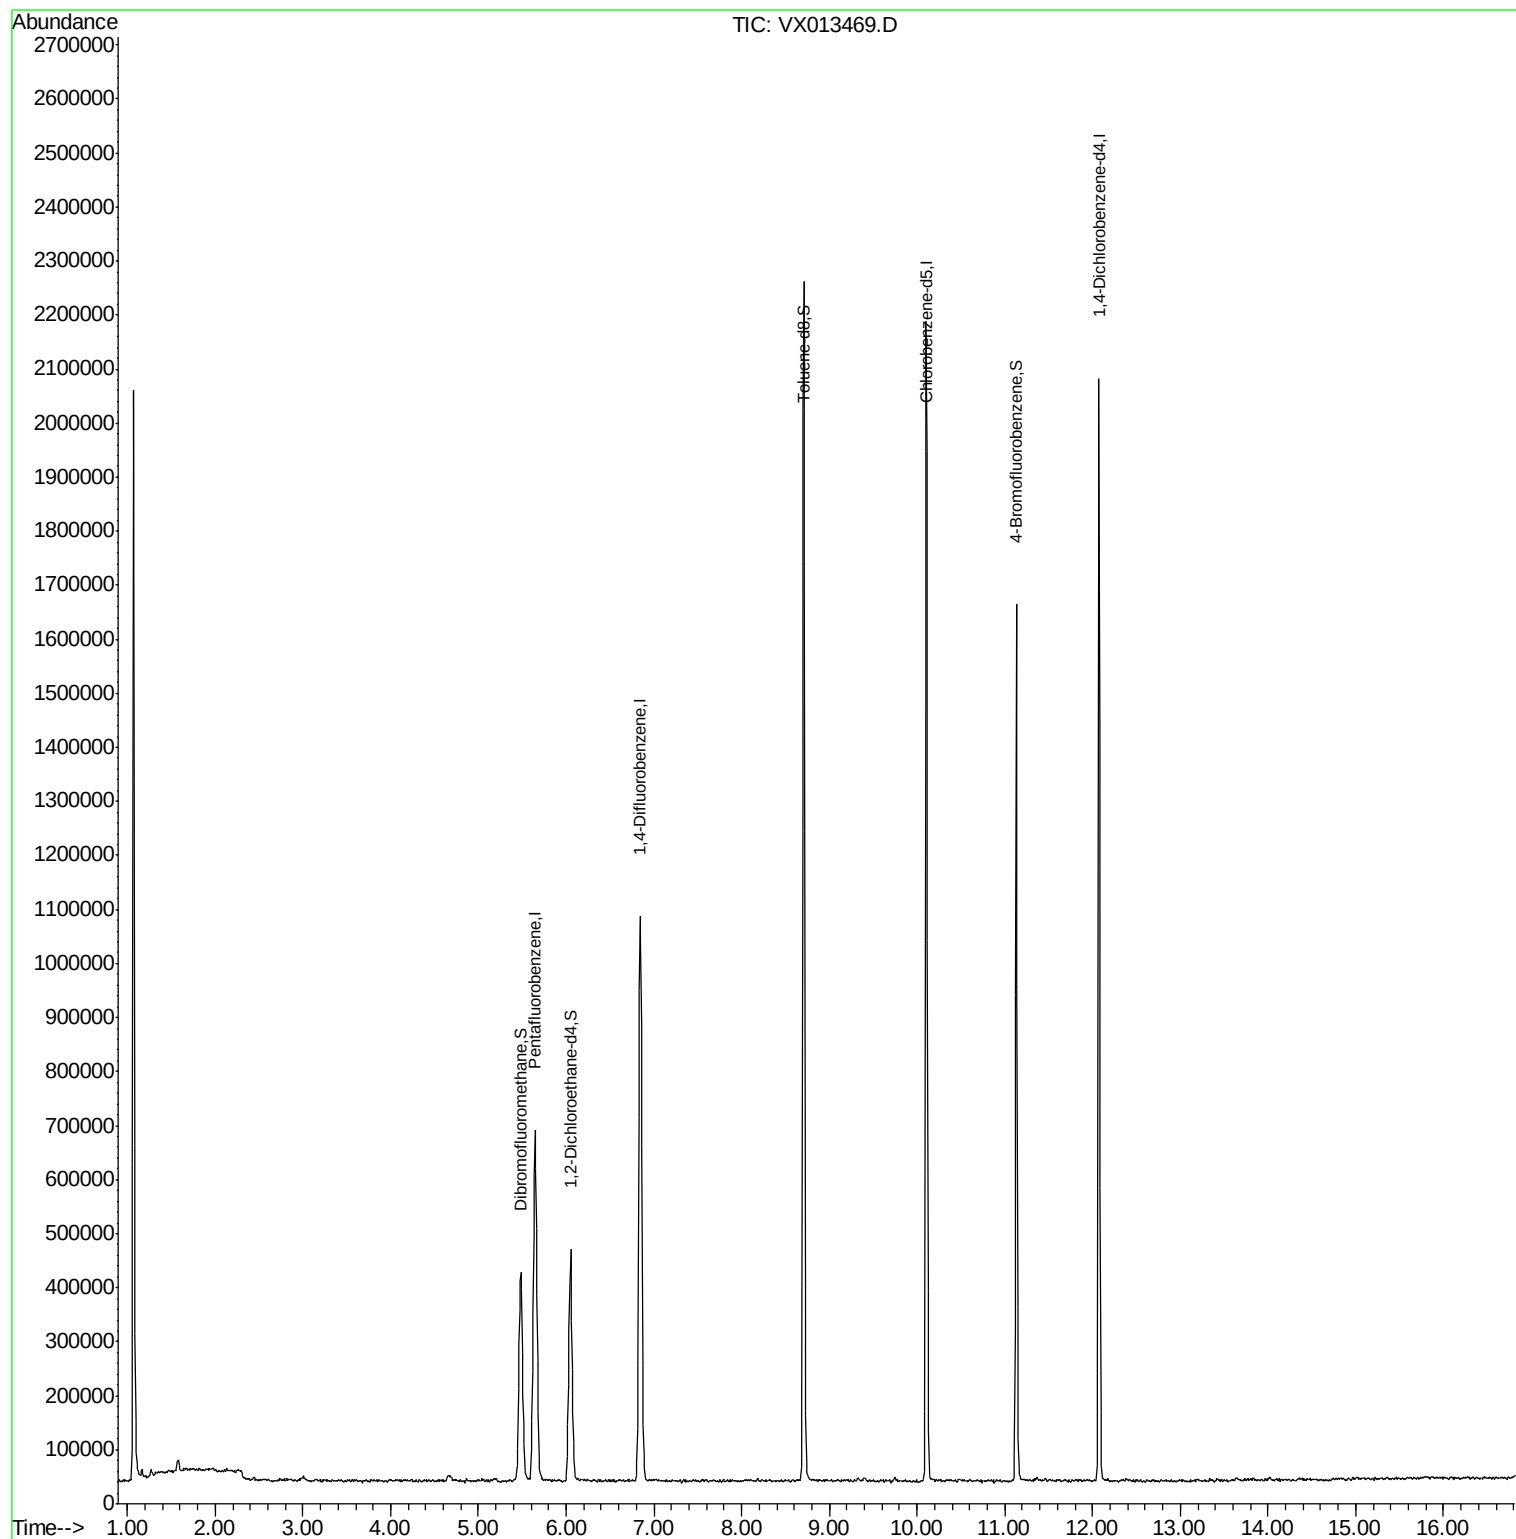

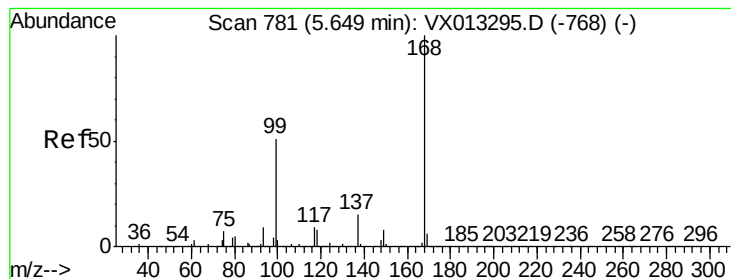

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. 0.00 min

Lab File: VX013469.D

Acq: 20 Nov 2019 10:35

Instrument :

MSVOA_X

ClientSampleId :


VX1120WBL01

Tot Ion:168 Resp: 668180

Ion Ratio Lower Upper




168 100

99 48.8 40.8 61.2

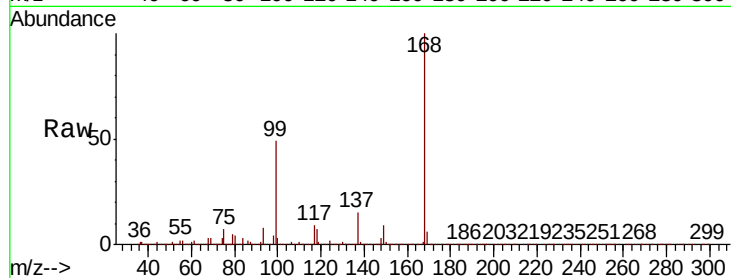

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

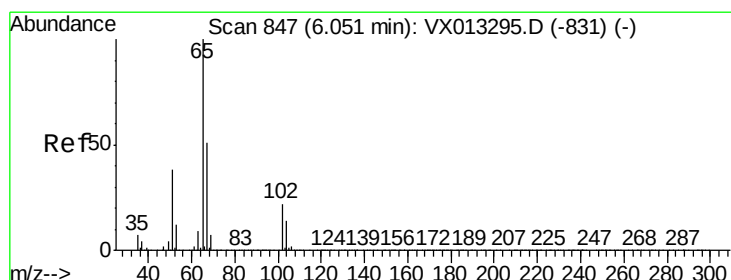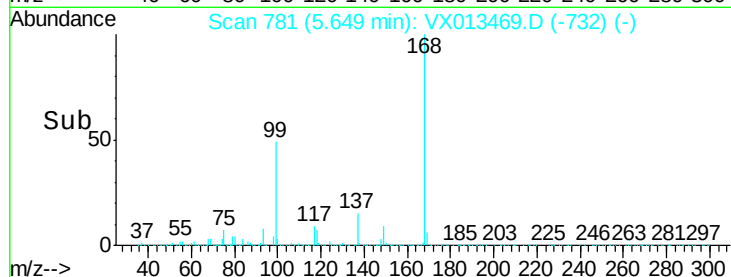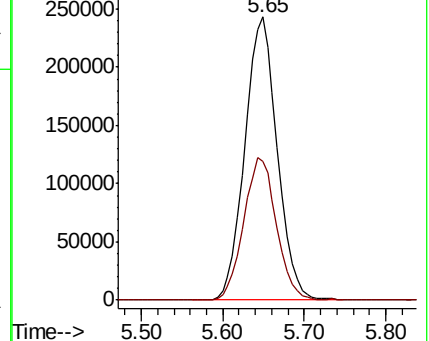

#33

1,2-Dichloroethane-d4

Concen: 50.378 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX013469.D


Acq: 20 Nov 2019 10:35

Tgt Ion: 65 Resp: 398791

Ion Ratio Lower Upper



65 100


67 53.0 0.0 104.2

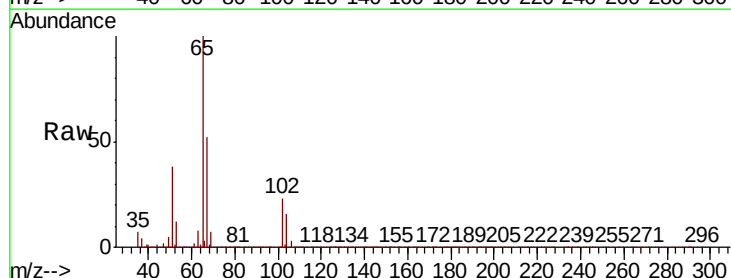

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

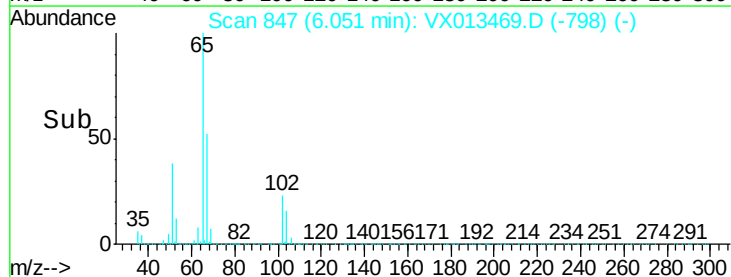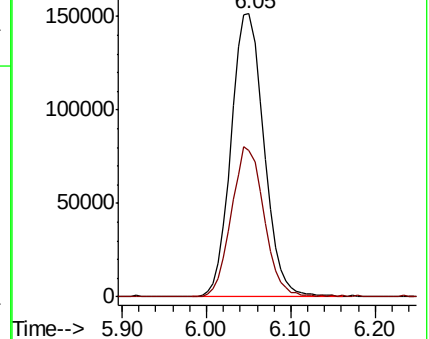

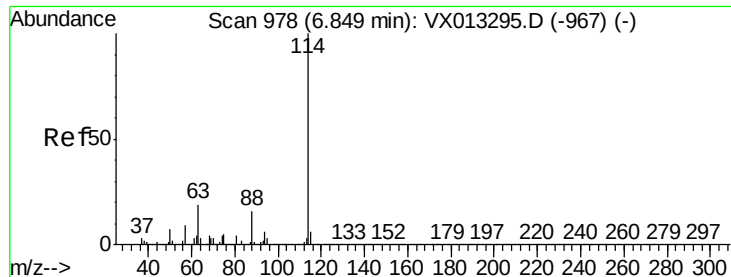

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 977

Delta R.T. -0.01 min

Lab File: VX013469.D

Acq: 20 Nov 2019 10:35

Instrument :

MSVOA_X

ClientSampleId :

VX1120WBL01


Tot Ion:114 Resp: 1096035

Ion Ratio Lower Upper

114 100

63 20.7 0.0 38.4




88 15.9 0.0 32.2

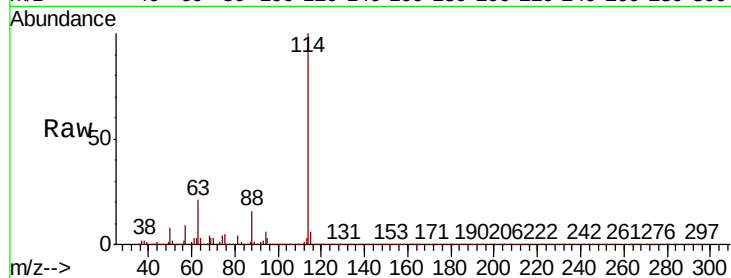

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

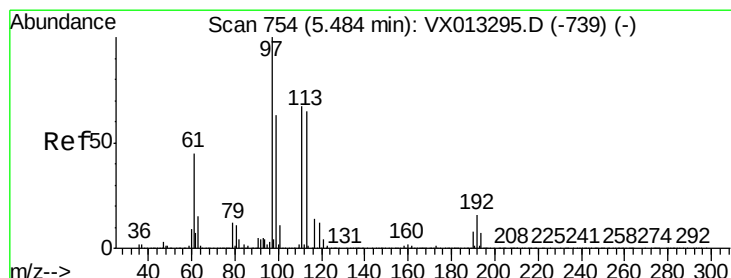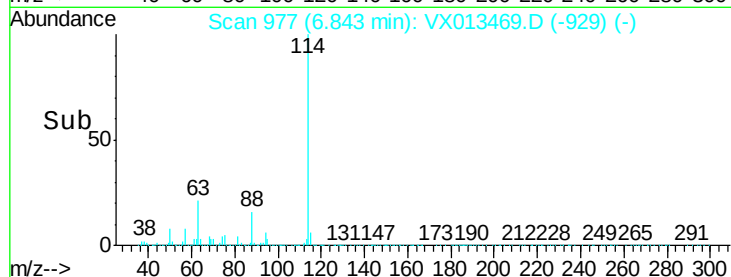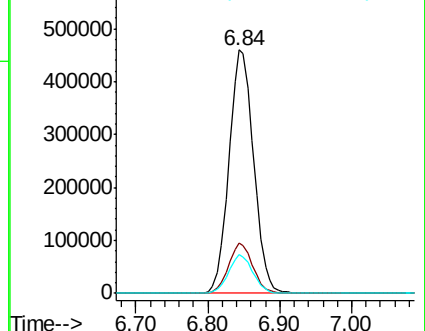

#35

Dibromofluoromethane

Concen: 48.639 ug/l

RT: 5.48 min Scan# 754

Delta R.T. 0.00 min

Lab File: VX013469.D

Acq: 20 Nov 2019 10:35


Tgt Ion:113 Resp: 334365

Ion Ratio Lower Upper

113 100

111 102.5 81.9 122.9



192 23.5 19.1 28.7

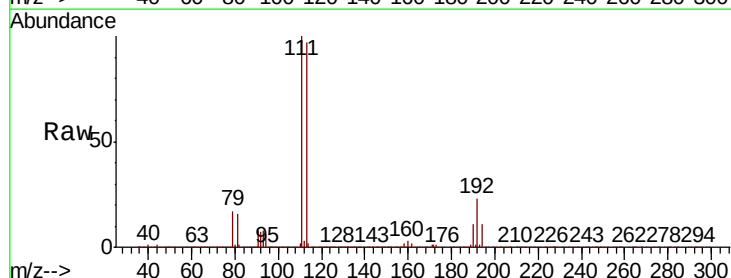


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



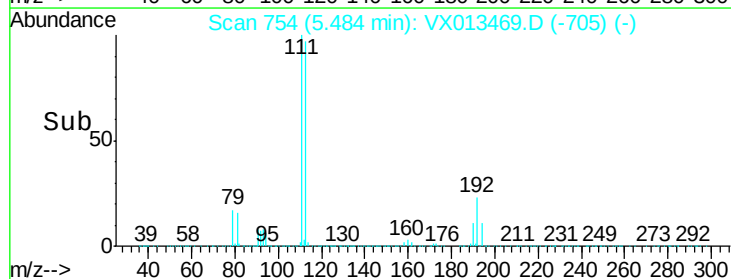
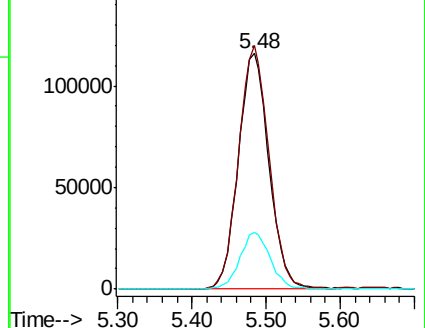


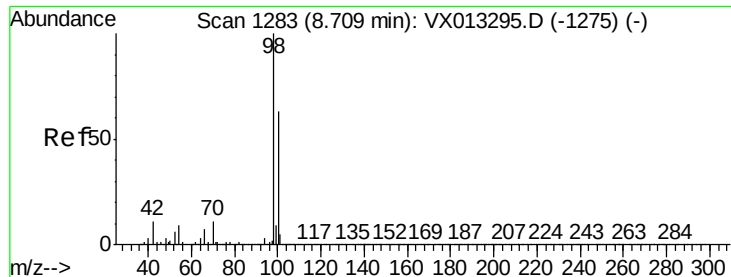

#50
Toluene-d8
Concen: 50.183 ug/l
RT: 8.71 min Scan# 1283
Delta R.T. 0.00 min
Lab File: VX013469.D
Acq: 20 Nov 2019 10:35




Instrument :
MSVOA_X
ClientSampleId :
VX1120WBL01


Tot Ion: 98 Resp: 1300539
Ion Ratio Lower Upper
98 100
100 65.5 52.2 78.2

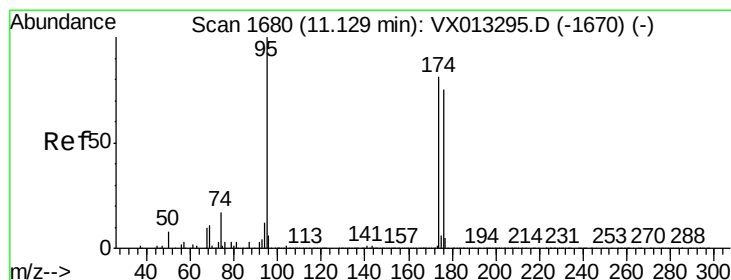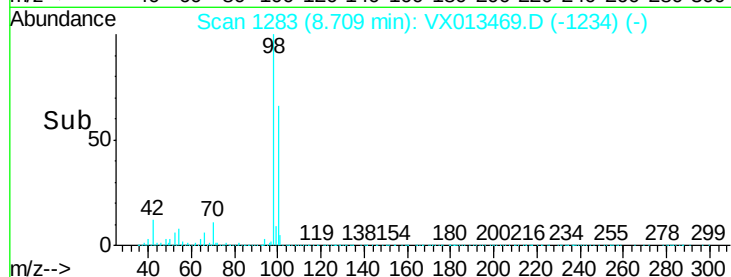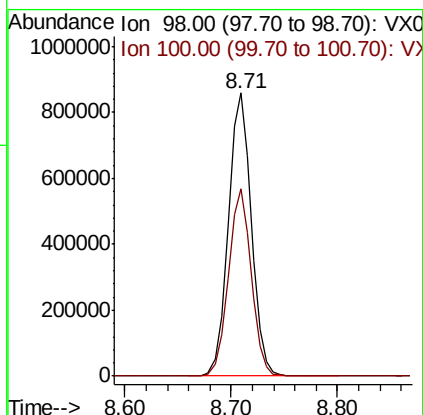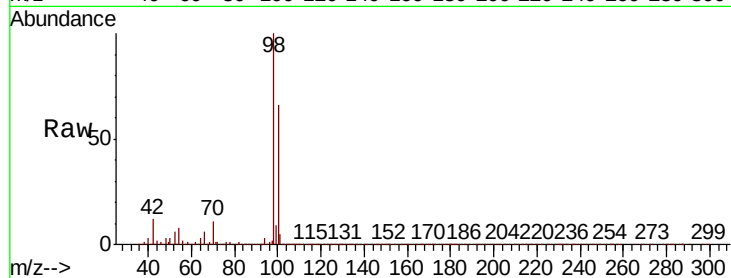

#62
4-Bromofluorobenzene
Concen: 46.187 ug/l
RT: 11.13 min Scan# 1680
Delta R.T. -0.00 min
Lab File: VX013469.D
Acq: 20 Nov 2019 10:35

Tgt Ion: 95 Resp: 431995
Ion Ratio Lower Upper
95 100
174 88.6 0.0 179.8
176 86.3 0.0 173.0


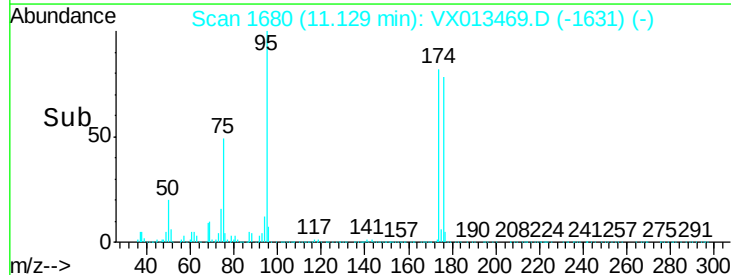
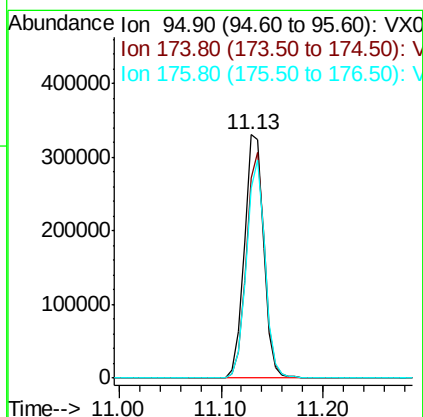
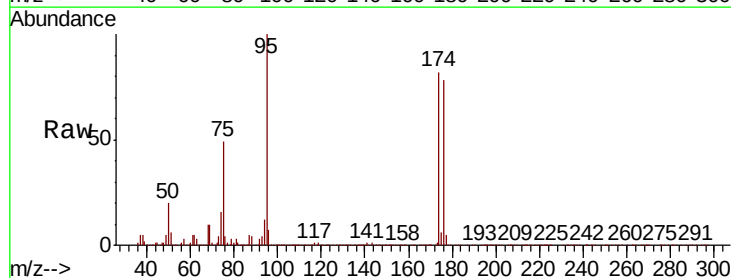


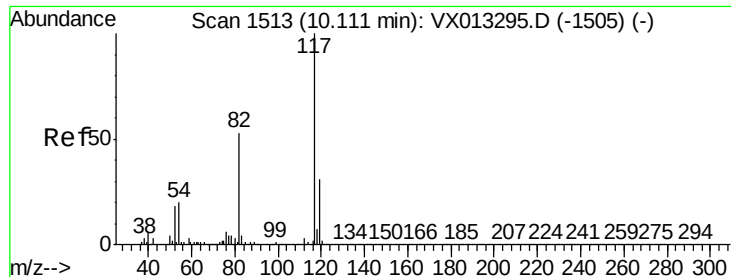

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1512
Delta R.T. -0.01 min
Lab File: VX013469.D
Acq: 20 Nov 2019 10:35

Instrument :
MSVOA_X
ClientSampleId :
VX1120WBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	55.2	42.6	64.0
119	31.9	24.8	37.2

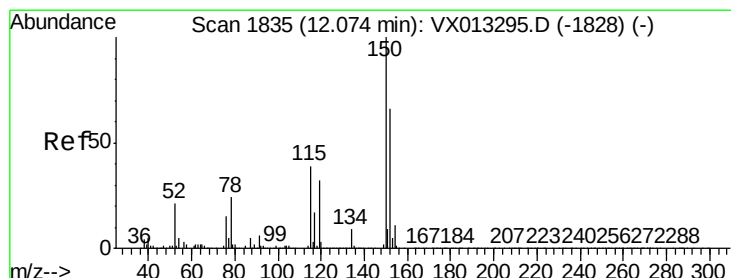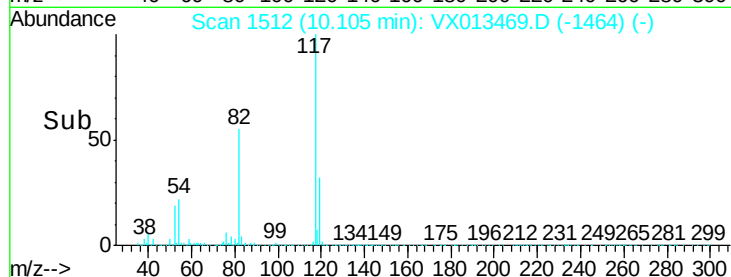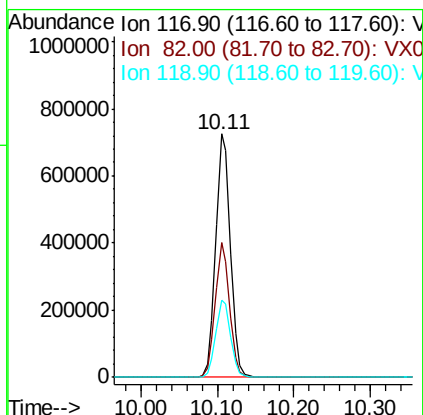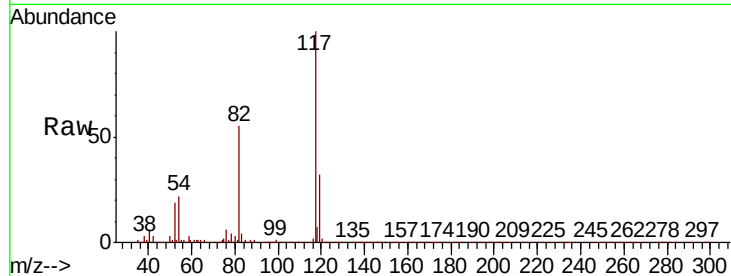

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX013469.D
Acq: 20 Nov 2019 10:35

Tgt Ion	Ratio	Lower	Upper
152	100		
115	54.9	39.5	118.3
150	152.7	0.0	344.4

