


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX112019\
Data File : VX013467.D
Acq On : 20 Nov 2019 09:19
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Title : SW846 8260
Last Update : Sat Nov 02 07:06:38 2019

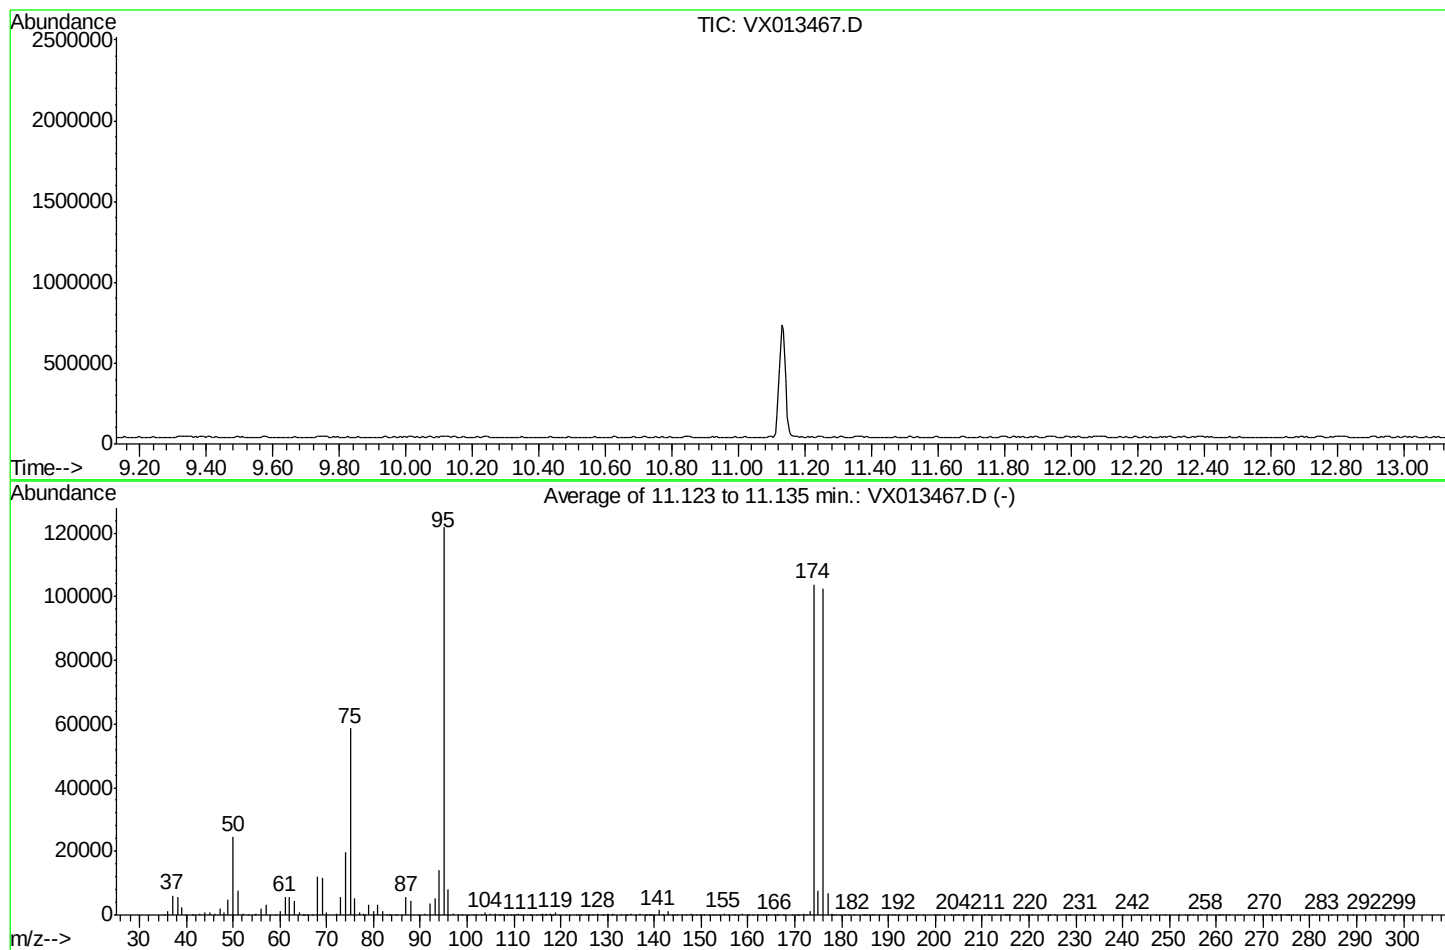

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1668

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	24728	PASS
75	95	30	60	48.2	58692	PASS
95	95	100	100	100.0	121768	PASS
96	95	5	9	6.7	8100	PASS
173	174	0.00	2	1.1	1124	PASS
174	95	50	100	85.3	103840	PASS
175	174	5	9	7.5	7837	PASS
176	174	95	101	98.6	102390	PASS
177	176	5	9	6.7	6824	PASS