

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112020\
 Data File : VX019485.D
 Acq On : 19 Nov 2020 22:47
 Operator : JC/MD
 Sample : L4834-02 10X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DSN-002-SEWER-OUTLET-002

Integration Parameters: RTEINT3.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X112020W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.587	74	82	83	rBV5	8026	16965	1.19%	0.344%
2	2.422	211	219	235	rBV	141100	235182	16.47%	4.765%
3	2.599	235	248	268	rBV	715864	1428102	100.00%	28.937%
4	4.672	573	588	598	rBV2	11822	41351	2.90%	0.838%
5	4.977	626	638	655	rBV2	105848	315761	22.11%	6.398%
6	5.172	662	670	679	rVB2	6739	20013	1.40%	0.406%
7	6.025	799	810	828	rBV	109965	290728	20.36%	5.891%
8	6.830	931	942	957	rBV	240894	584860	40.95%	11.851%
9	8.696	1241	1248	1261	rBV	508143	804236	56.32%	16.296%
10	10.092	1471	1477	1494	rBV	496012	701240	49.10%	14.209%
11	11.122	1640	1646	1659	rBV	388863	496821	34.79%	10.067%




Sum of corrected areas: 4935259

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112020\
Data File : VX019485.D
Acq On : 19 Nov 2020 22:47
Operator : JC/MD
Sample : L4834-02 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-002-SEWER-OUTLET-002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X112020W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

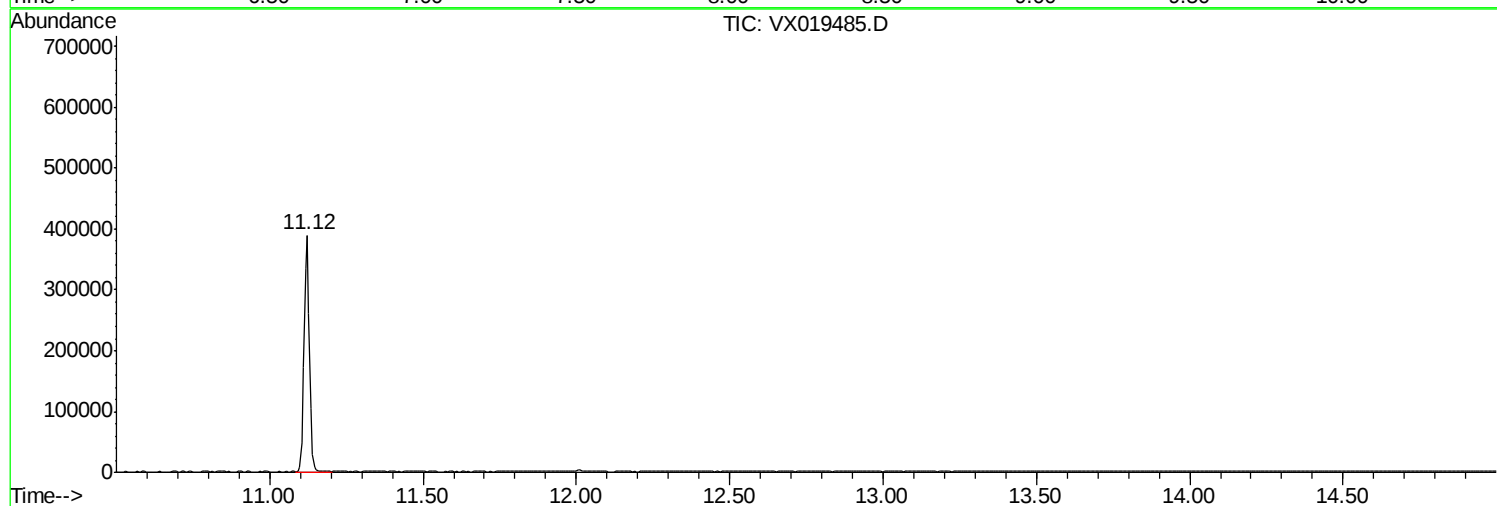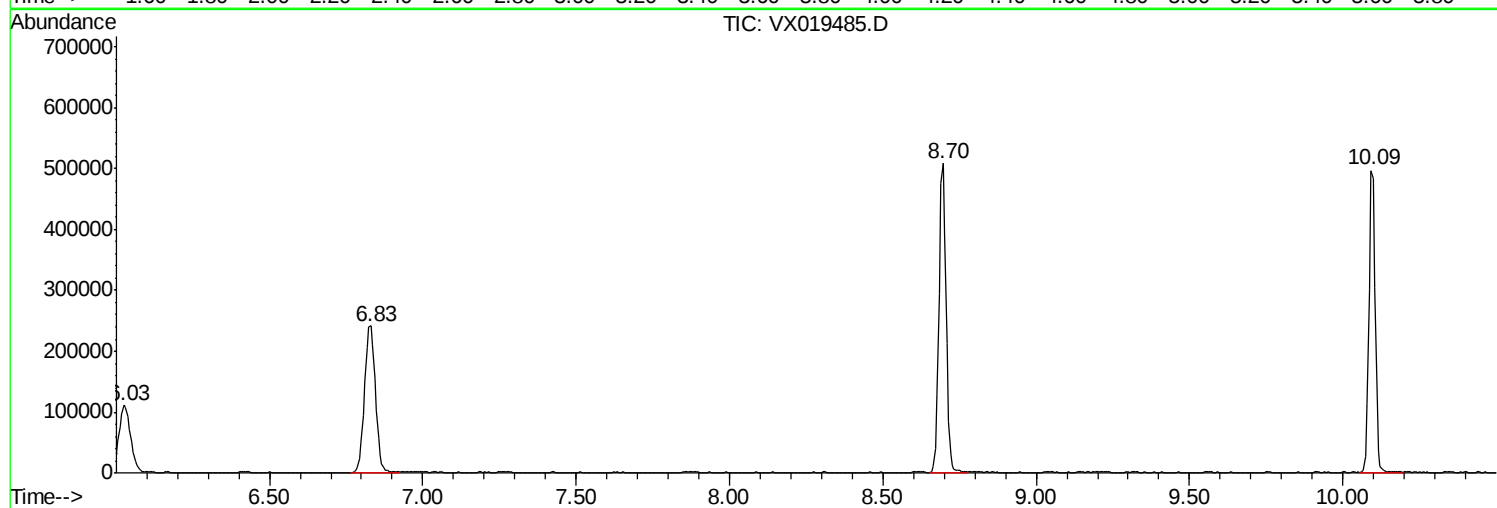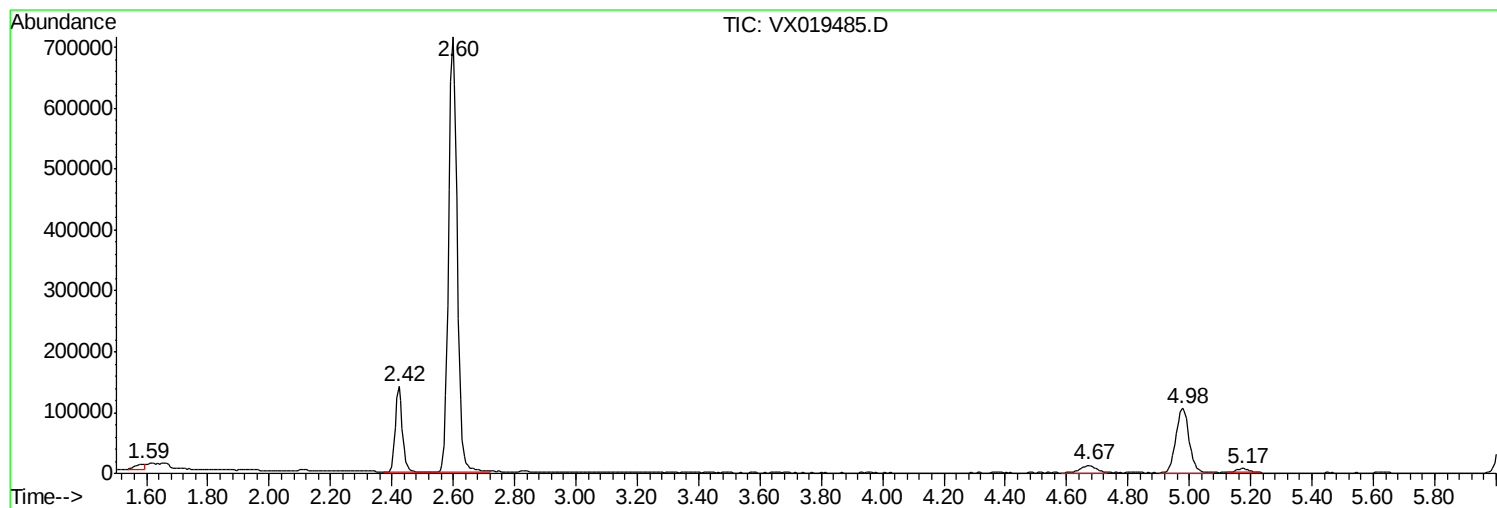

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112020\
Data File : VX019485.D
Acq On : 19 Nov 2020 22:47
Operator : JC/MD
Sample : L4834-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-002-SEWER-OUTLET-002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\624X112020W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX112020\
Data File : VX019485.D
Acq On : 19 Nov 2020 22:47
Operator : JC/MD
Sample : L4834-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-002-SEWER-OUTLET-002

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X112020W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
