


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX112020\
 Data File : VX019467.D
 Acq On : 19 Nov 2020 15:26
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X112020W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Nov 20 01:06:02 2020

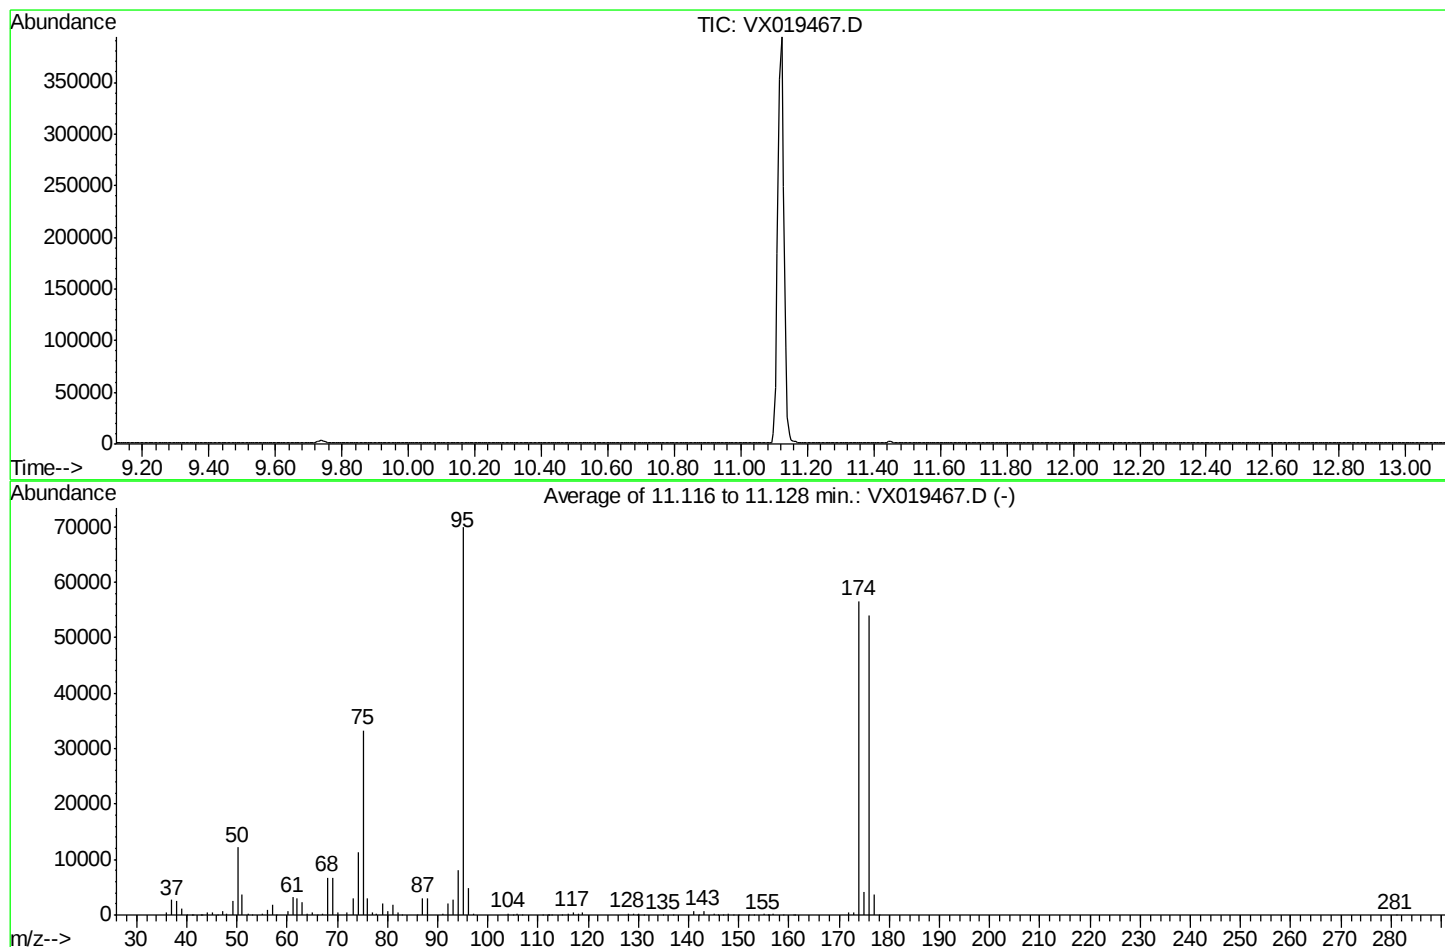

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	12235	PASS
75	95	30	60	47.7	33360	PASS
95	95	100	100	100.0	69925	PASS
96	95	5	9	7.0	4890	PASS
173	174	0.00	2	0.8	467	PASS
174	95	50	100	80.9	56581	PASS
175	174	5	9	7.5	4255	PASS
176	174	95	101	95.6	54093	PASS
177	176	5	9	6.8	3673	PASS