

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
 Data File : VX038947.D
 Acq On : 20 Nov 2023 10:34
 Operator : JC/MD
 Sample : VX1120MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1120MBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX038947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.538	69	74	83	rBV10	4370	9400	1.16%	0.205%
2	2.520	229	235	242	rVB2	5622	10759	1.33%	0.235%
3	2.788	272	279	288	rVB3	3676	8265	1.02%	0.181%
4	4.544	560	567	581	rVB2	3858	13351	1.65%	0.292%
5	5.379	693	704	719	rBV	88630	259661	32.03%	5.673%
6	5.544	719	731	749	rVB	131656	381242	47.02%	8.329%
7	5.952	788	798	812	rBV	93511	258467	31.88%	5.647%
8	6.757	921	930	944	rBV	236752	574121	70.81%	12.543%
9	8.647	1232	1240	1249	rBV	513540	810785	100.00%	17.713%
10	9.269	1336	1342	1350	rVB	19767	32863	4.05%	0.718%
11	10.049	1465	1470	1484	rBV	541770	771344	95.14%	16.851%
12	11.079	1633	1639	1651	rBV	487821	614483	75.79%	13.424%
13	11.311	1672	1677	1682	rVB2	19238	25519	3.15%	0.558%
14	12.018	1788	1793	1802	rBV	618995	807139	99.55%	17.633%




Sum of corrected areas: 4577399

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038947.D
Acq On : 20 Nov 2023 10:34
Operator : JC/MD
Sample : VX1120MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

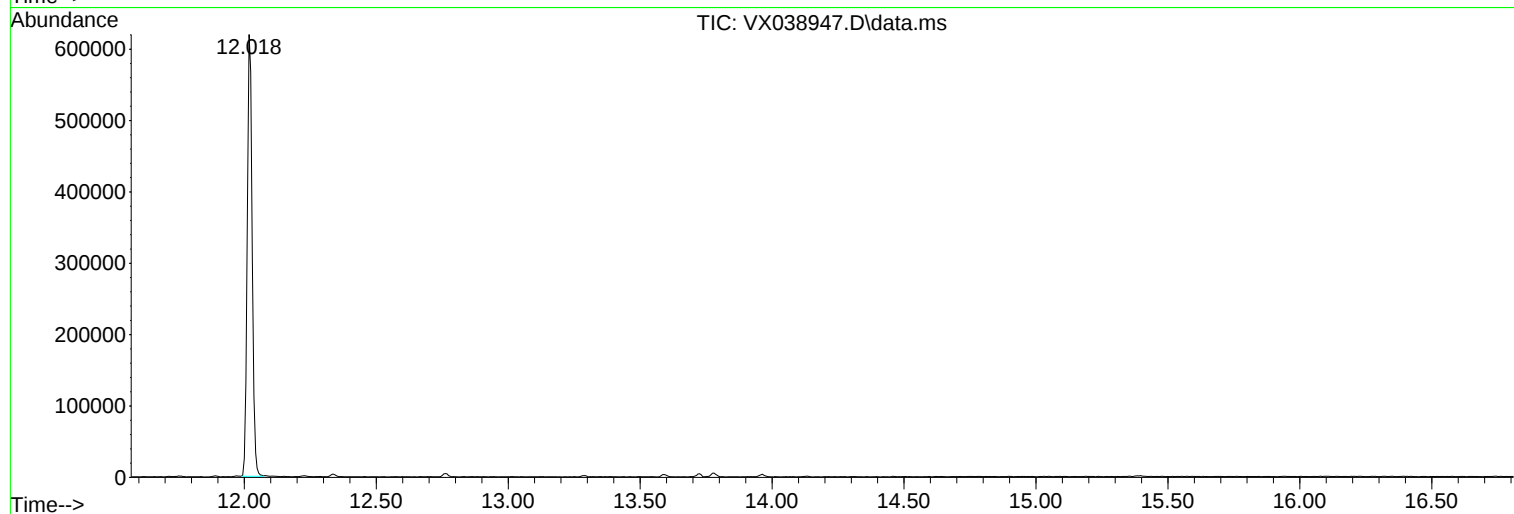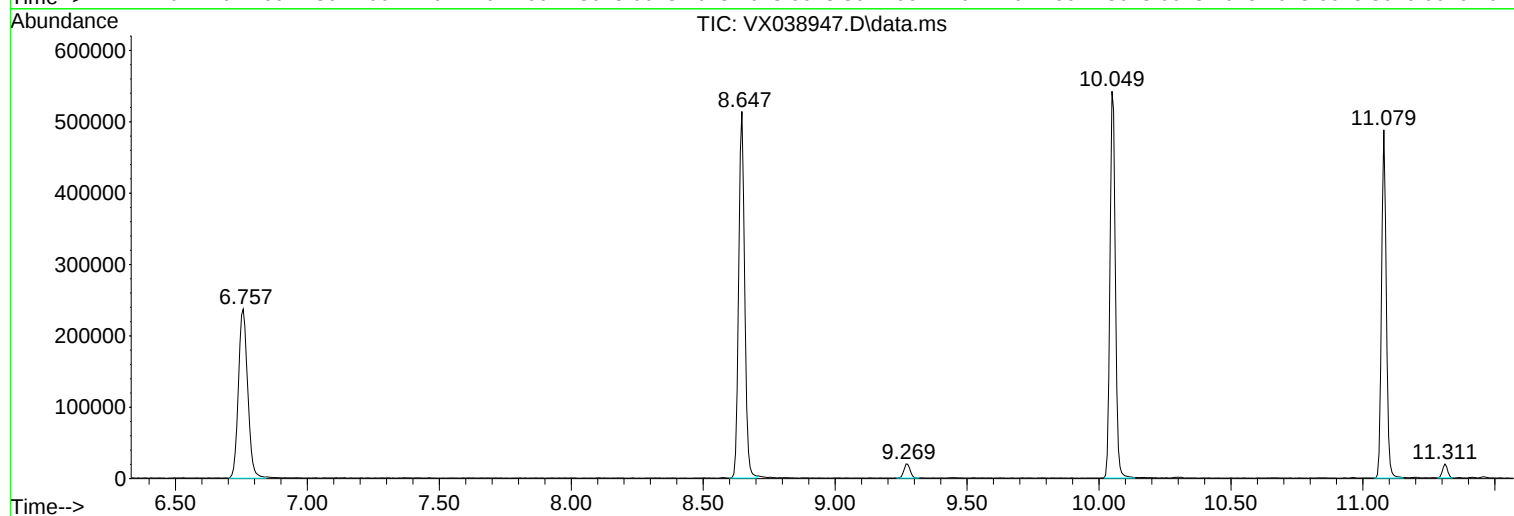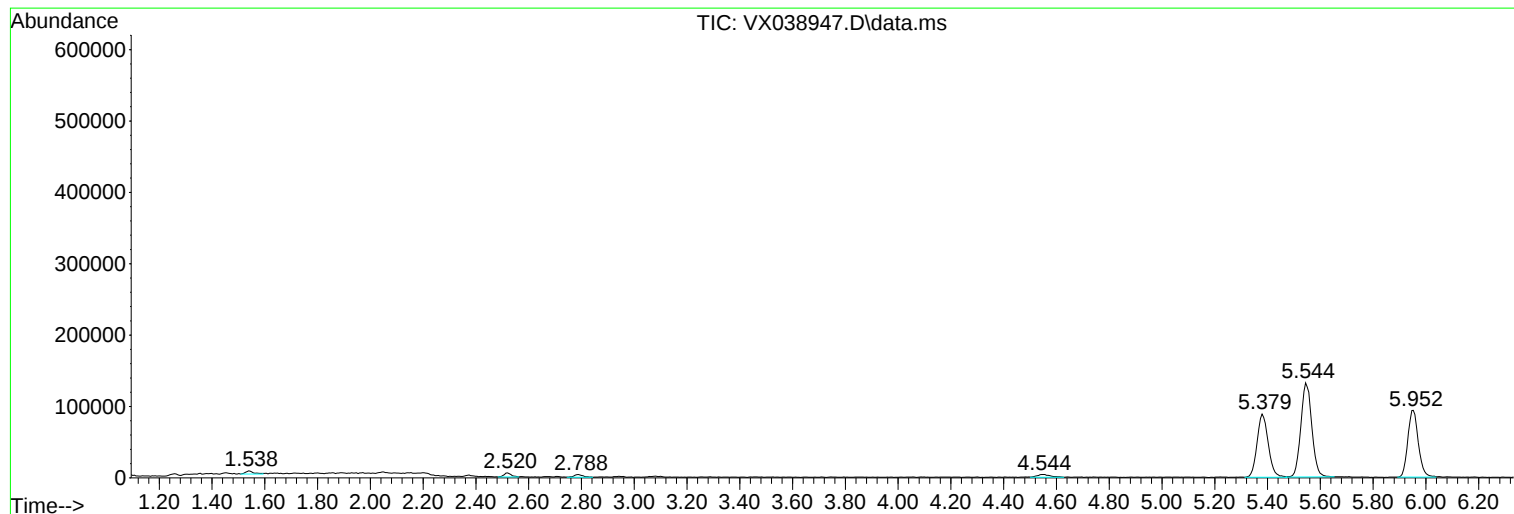

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038947.D
Acq On : 20 Nov 2023 10:34
Operator : JC/MD
Sample : VX1120MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038947.D
Acq On : 20 Nov 2023 10:34
Operator : JC/MD
Sample : VX1120MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120MBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc