

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038948.D
Acq On : 20 Nov 2023 10:57
Operator : JC/MD
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX038948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.538	69	74	79	rBV9	5040	10850	1.33%	0.241%
2	5.385	693	705	720	rBV2	84235	256525	31.47%	5.692%
3	5.550	720	732	745	rVV	131212	370765	45.49%	8.227%
4	5.952	786	798	820	rBV	97429	263570	32.34%	5.848%
5	6.757	921	930	949	rBV	230040	565975	69.44%	12.558%
6	8.647	1233	1240	1249	rBV	512666	807448	99.07%	17.916%
7	9.275	1337	1343	1348	rVB2	5034	8219	1.01%	0.182%
8	10.049	1465	1470	1487	rBV	550773	780002	95.70%	17.307%
9	11.079	1634	1639	1650	rBV	488233	619750	76.04%	13.751%
10	11.311	1673	1677	1684	rBV2	6040	8800	1.08%	0.195%
11	12.018	1788	1793	1806	rBV	630234	815047	100.00%	18.084%




Sum of corrected areas: 4506951

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038948.D
Acq On : 20 Nov 2023 10:57
Operator : JC/MD
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

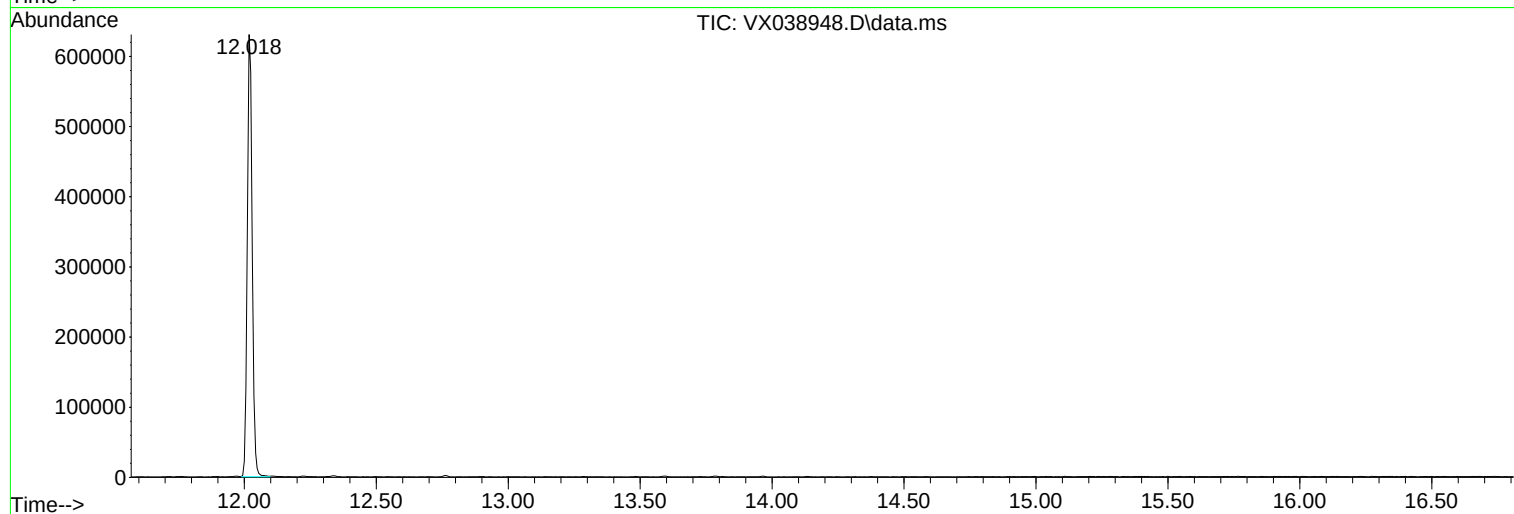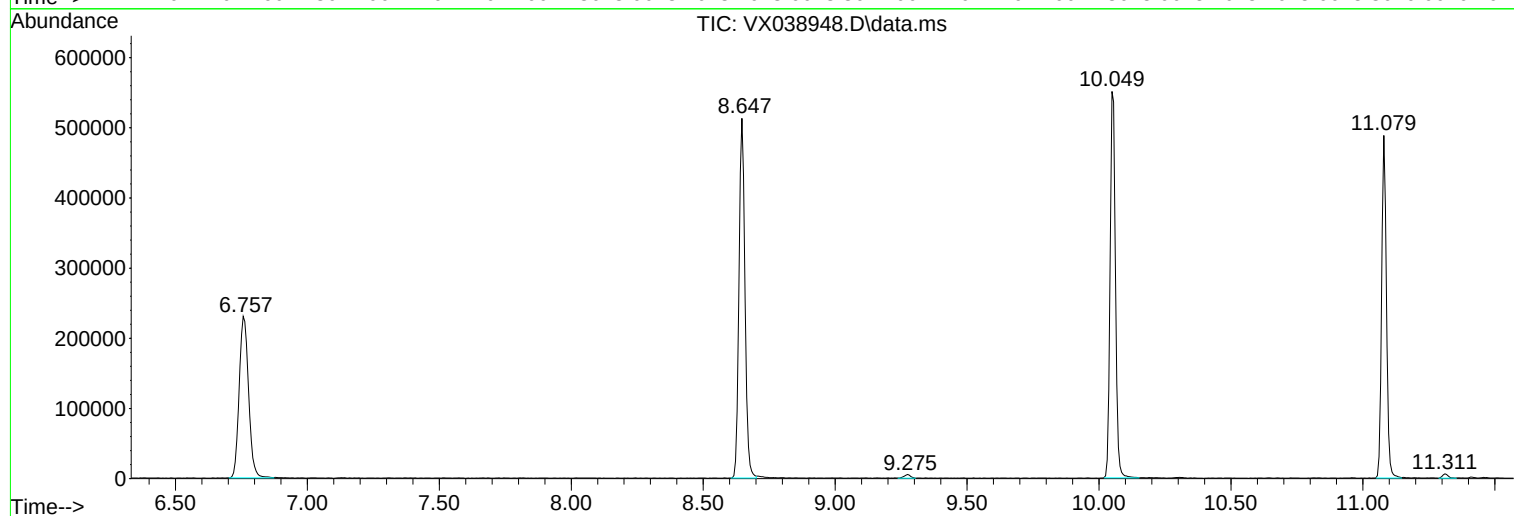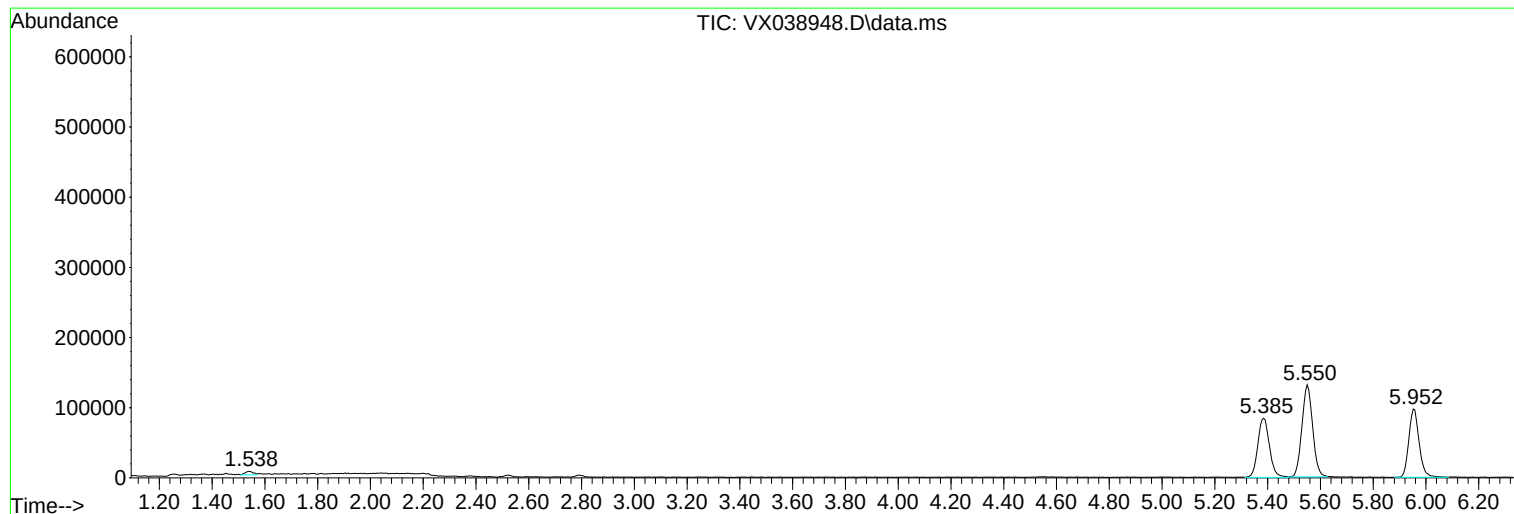

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038948.D
Acq On : 20 Nov 2023 10:57
Operator : JC/MD
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038948.D
Acq On : 20 Nov 2023 10:57
Operator : JC/MD
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1120WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------