

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
 Data File : VX038956.D
 Acq On : 20 Nov 2023 14:19
 Operator : JC/MD
 Sample : 05404-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP06-20231109

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX038956.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.325	197	203	210	rBV5	4502	9510	1.24%	0.208%
2	5.385	694	705	720	rBV2	81036	236197	30.86%	5.170%
3	5.550	722	732	747	rVV2	122102	351032	45.87%	7.684%
4	5.952	787	798	812	rBV	89707	246649	32.23%	5.399%
5	6.757	921	930	947	rBV	218127	535314	69.94%	11.717%
6	7.123	982	990	1003	rBV	150007	333392	43.56%	7.298%
7	8.647	1232	1240	1255	rBV	480335	765344	100.00%	16.752%
8	9.275	1336	1343	1349	rBV2	13097	20617	2.69%	0.451%
9	10.055	1465	1471	1486	rBV	521382	733168	95.80%	16.048%
10	11.079	1634	1639	1653	rVB	438533	572085	74.75%	12.522%
11	12.018	1788	1793	1807	rBV	585919	765244	99.99%	16.750%




Sum of corrected areas: 4568552

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038956.D
Acq On : 20 Nov 2023 14:19
Operator : JC/MD
Sample : 05404-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20231109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

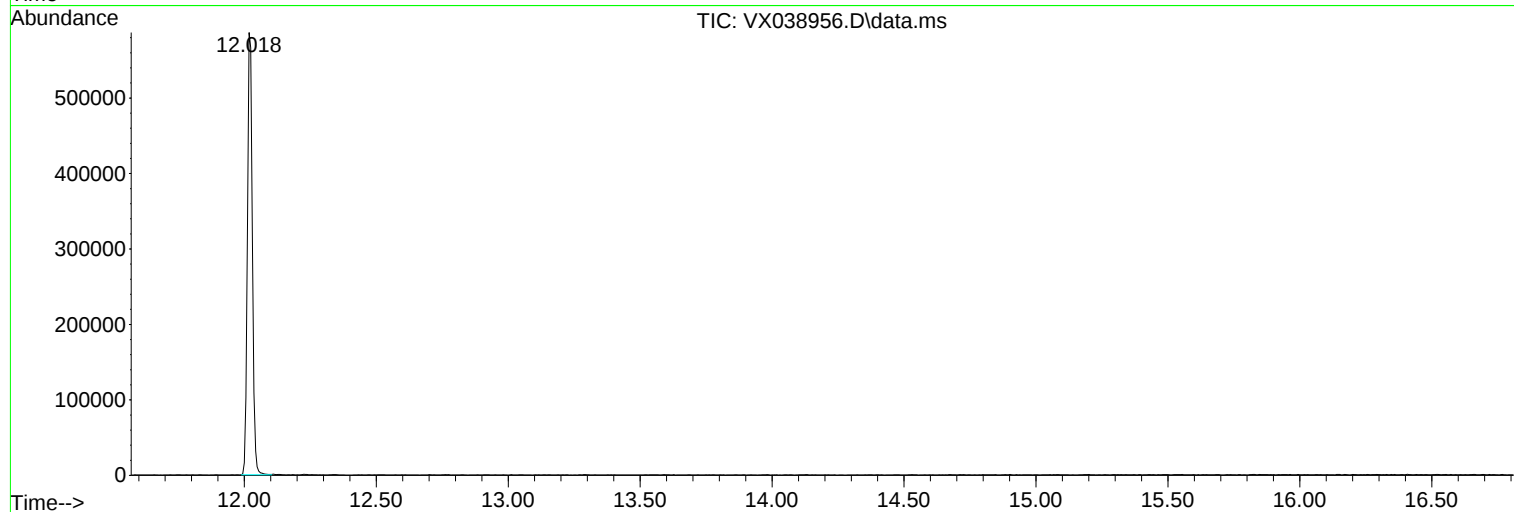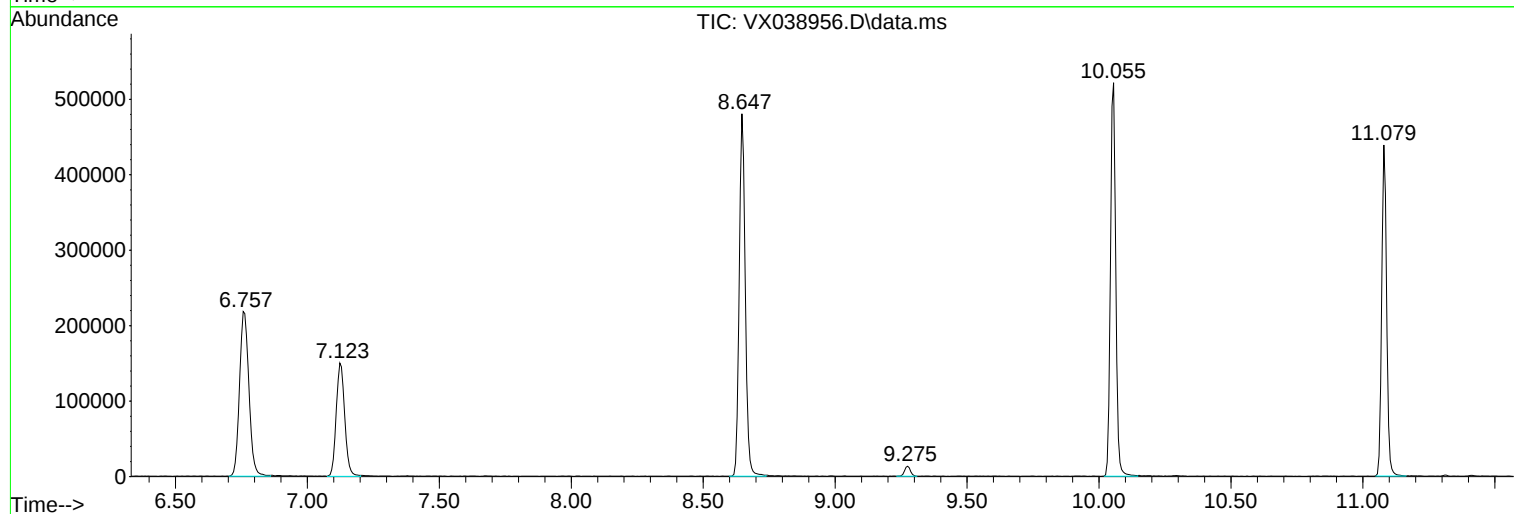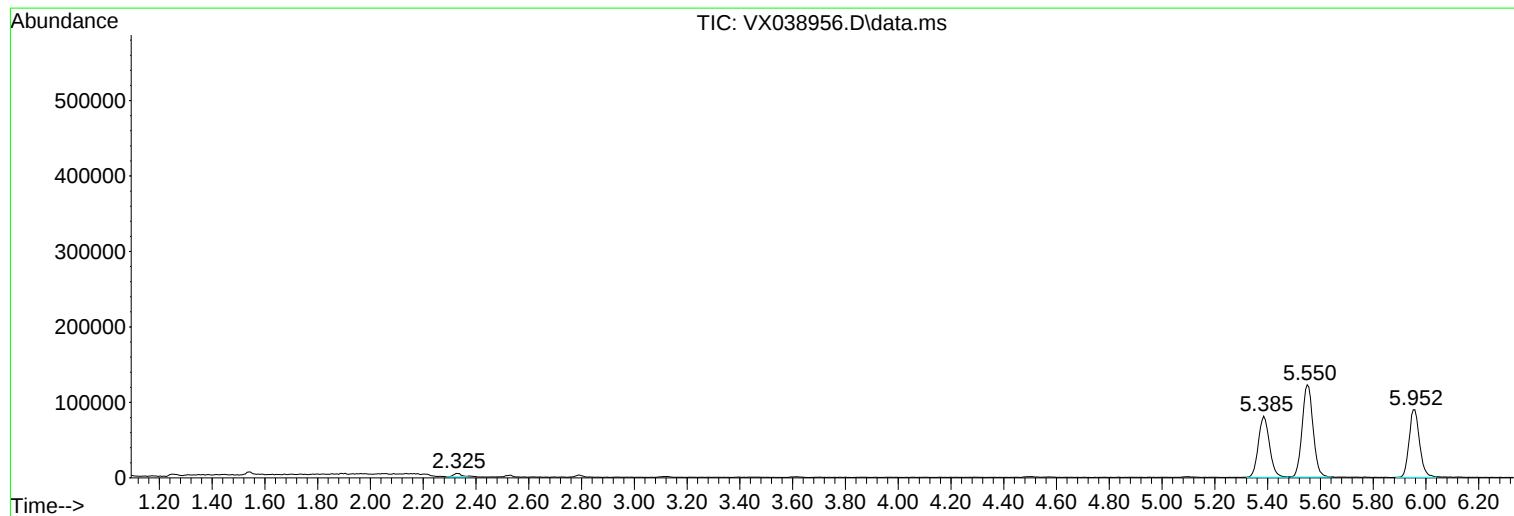

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038956.D
Acq On : 20 Nov 2023 14:19
Operator : JC/MD
Sample : 05404-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20231109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038956.D
Acq On : 20 Nov 2023 14:19
Operator : JC/MD
Sample : 05404-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP06-20231109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------