

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
 Data File : VX038968.D
 Acq On : 20 Nov 2023 18:54
 Operator : JC/MD
 Sample : 05431-12 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 91BR-20231113

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX038968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	55	rVB	18625	19849	2.55%	0.424%
2	4.489	547	558	579	rBV	109664	316487	40.60%	6.763%
3	5.385	694	705	721	rBV	80771	239006	30.66%	5.107%
4	5.550	721	732	747	rVV	124586	354475	45.48%	7.575%
5	5.952	789	798	813	rBV	92424	250963	32.20%	5.363%
6	6.757	920	930	946	rBV	221958	541014	69.41%	11.561%
7	7.129	982	991	1004	rBV2	41038	95024	12.19%	2.031%
8	8.647	1234	1240	1258	rBV	490510	769303	98.70%	16.439%
9	10.055	1465	1471	1488	rBV	516560	734996	94.30%	15.706%
10	11.079	1634	1639	1654	rBV	454532	579163	74.30%	12.376%
11	12.018	1788	1793	1804	rBV	600670	779441	100.00%	16.656%




Sum of corrected areas: 4679721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038968.D
Acq On : 20 Nov 2023 18:54
Operator : JC/MD
Sample : 05431-12 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
91BR-20231113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

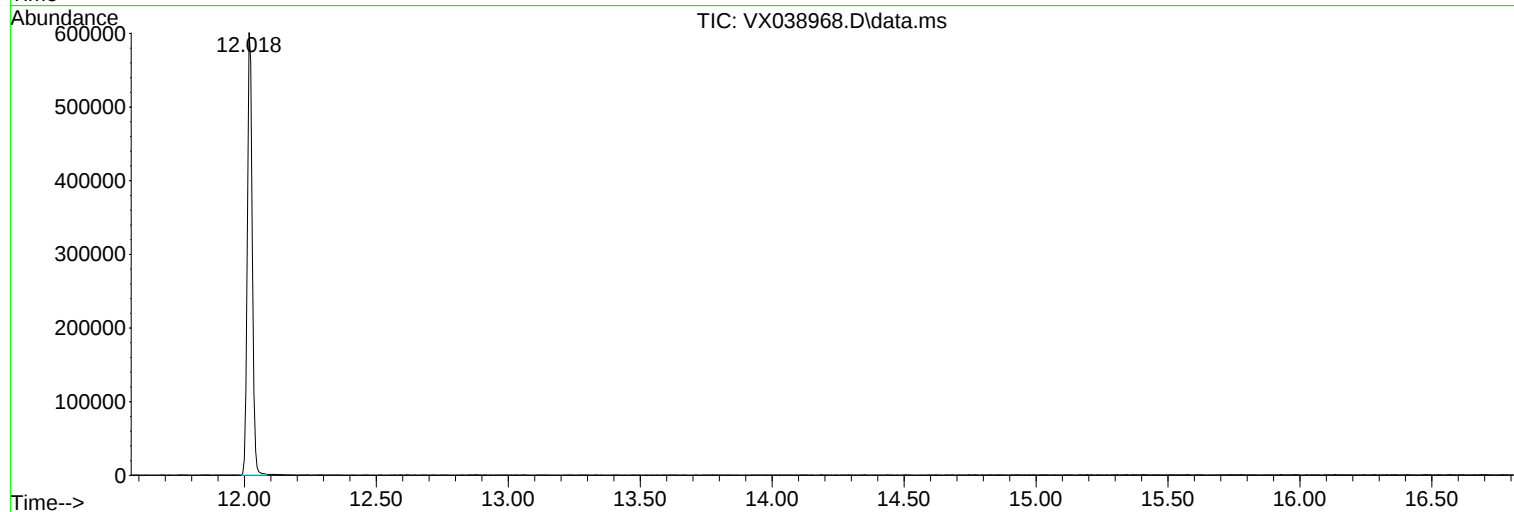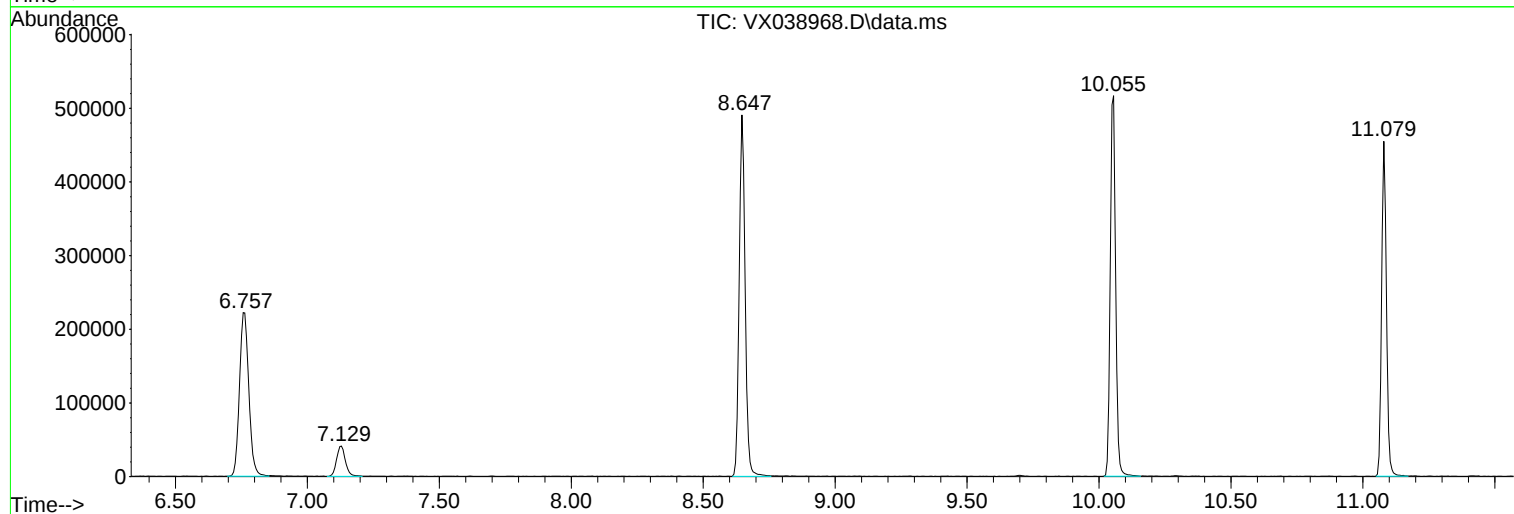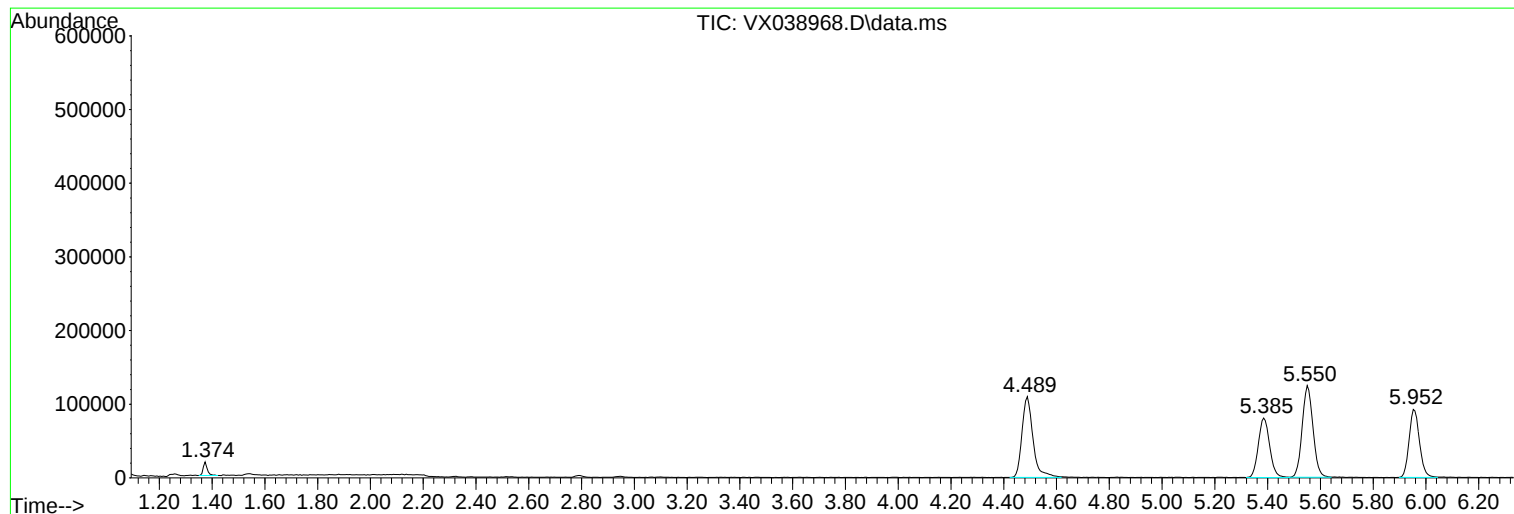

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038968.D
Acq On : 20 Nov 2023 18:54
Operator : JC/MD
Sample : 05431-12 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
91BR-20231113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038968.D
Acq On : 20 Nov 2023 18:54
Operator : JC/MD
Sample : 05431-12 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
91BR-20231113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------