

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
 Data File : VX038970.D
 Acq On : 20 Nov 2023 19:40
 Operator : JC/MD
 Sample : 05431-14 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP-01-20231113

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX038970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.788	273	279	287	rBV	6011	12378	1.70%	0.271%
2	4.489	547	558	580	rBV	71235	213575	29.42%	4.681%
3	5.385	693	705	720	rBV	77181	225348	31.04%	4.939%
4	5.550	722	732	747	rVB	113277	329349	45.36%	7.219%
5	5.958	787	799	816	rBV	86953	237892	32.77%	5.214%
6	6.763	921	931	948	rBV	207886	508474	70.03%	11.145%
7	7.123	981	990	1002	rBV2	158388	355051	48.90%	7.782%
8	8.647	1233	1240	1259	rBV	458692	722336	99.49%	15.833%
9	10.055	1465	1471	1482	rBV	498763	690890	95.16%	15.144%
10	11.079	1634	1639	1656	rBV	422549	540920	74.50%	11.856%
11	12.018	1788	1793	1809	rBV	551161	726055	100.00%	15.914%




Sum of corrected areas: 4562268

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038970.D
Acq On : 20 Nov 2023 19:40
Operator : JC/MD
Sample : 05431-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-20231113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

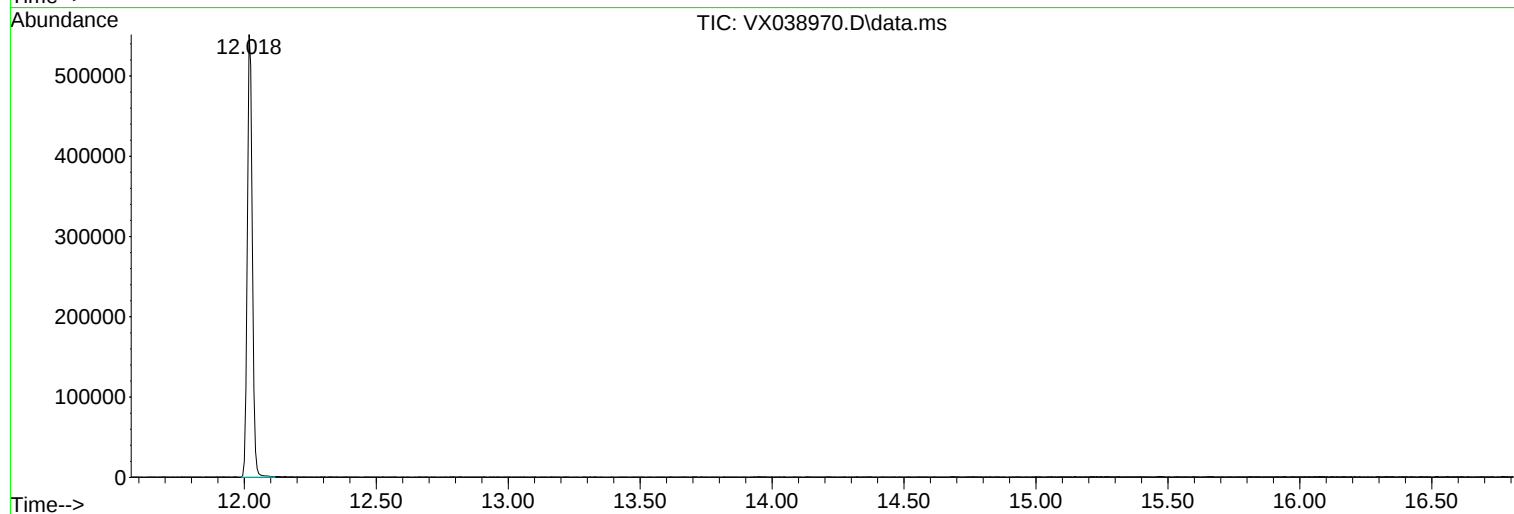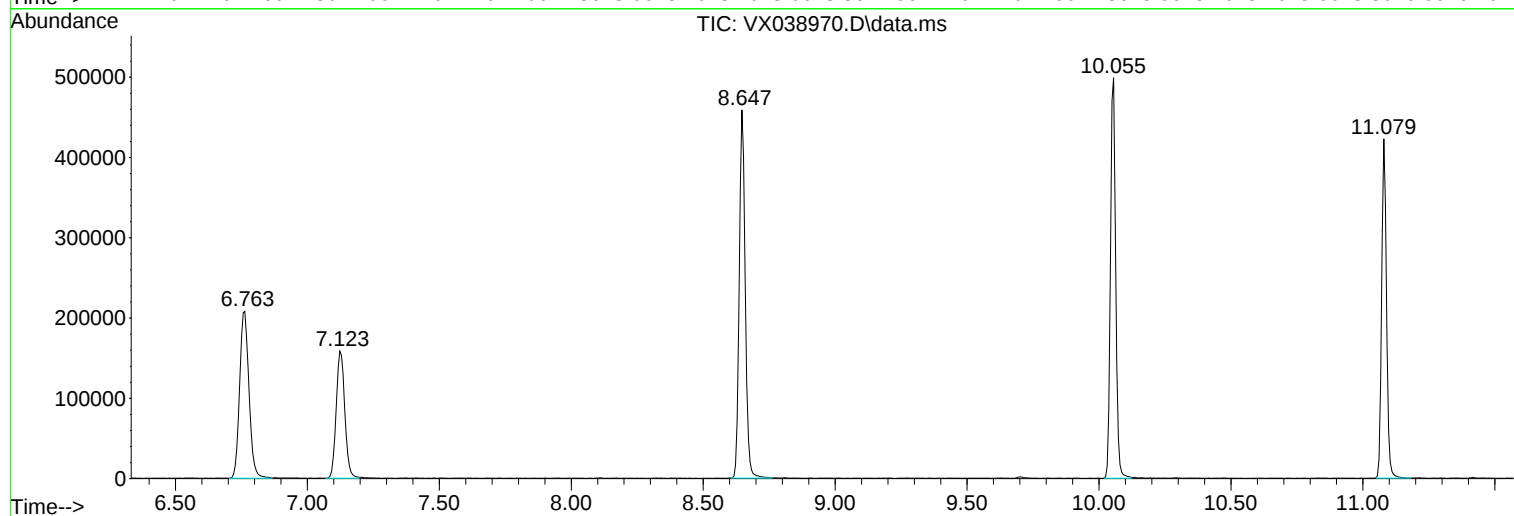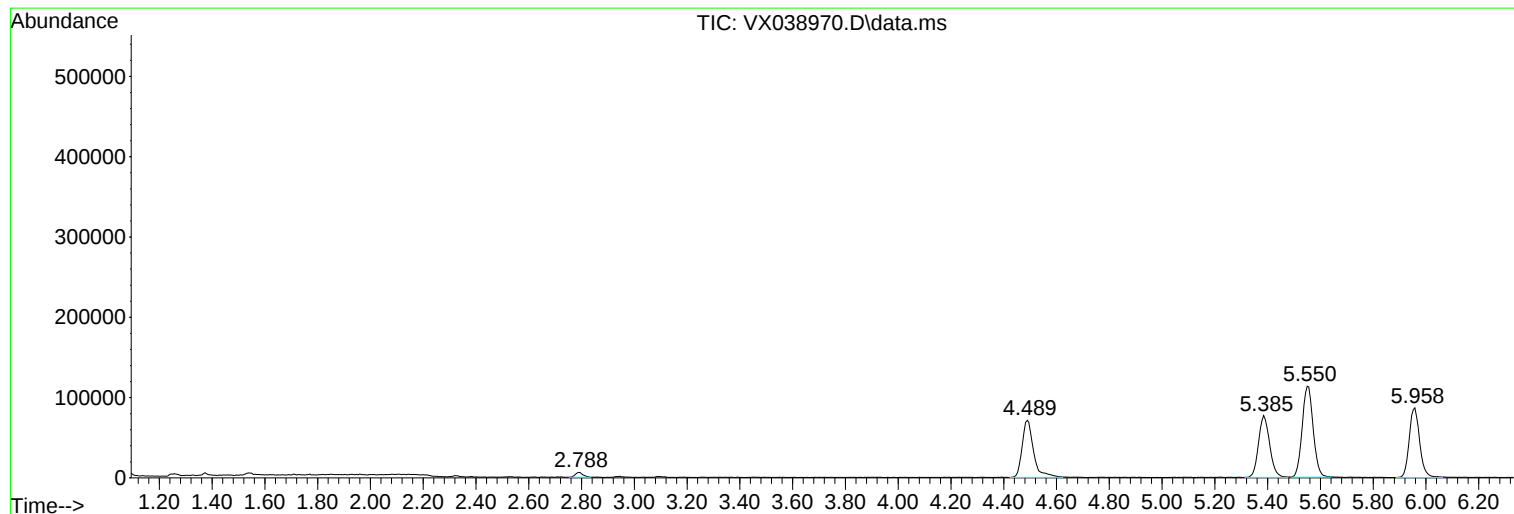

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038970.D
Acq On : 20 Nov 2023 19:40
Operator : JC/MD
Sample : 05431-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-20231113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038970.D
Acq On : 20 Nov 2023 19:40
Operator : JC/MD
Sample : 05431-14 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-01-20231113

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------