
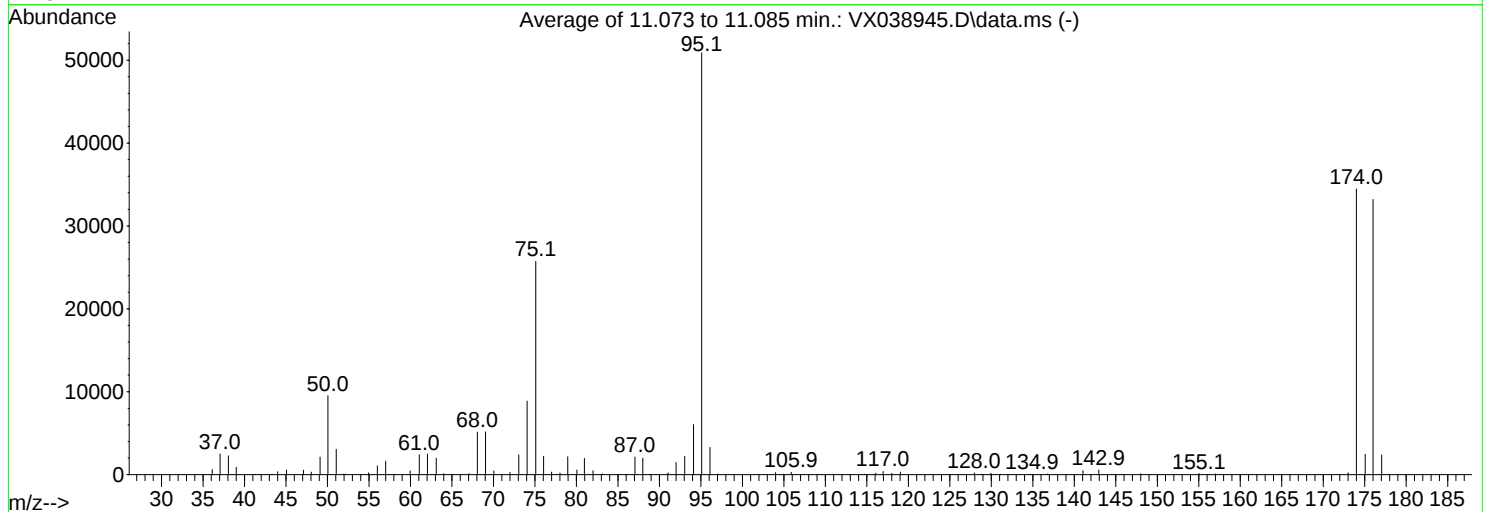


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112023\
Data File : VX038945.D
Acq On : 20 Nov 2023 09:08
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Title : SW846 8260
Last Update : Thu Nov 16 22:59:22 2023

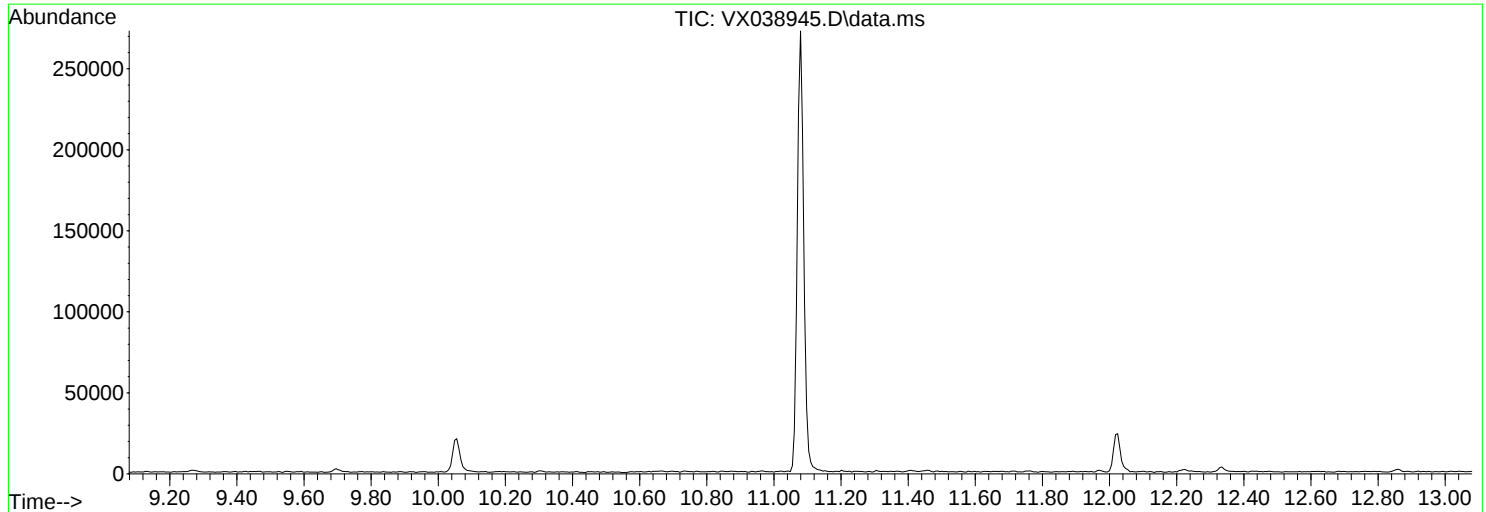

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1630

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	9532	PASS
75	95	30	60	50.6	25739	PASS
95	95	100	100	100.0	50883	PASS
96	95	5	9	6.5	3287	PASS
173	174	0.00	2	0.7	233	PASS
174	95	50	100	67.7	34464	PASS
175	174	5	9	7.1	2454	PASS
176	174	95	101	96.3	33192	PASS
177	176	5	9	7.2	2378	PASS