

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
 Data File : VX043908.D
 Acq On : 20 Nov 2024 10:42
 Operator : JC/MD
 Sample : VX1120MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 21 00:39:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 21 00:38:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	239712	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.049	117	230003	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	91805	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	91553	47.872	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	95.740%		
7) Chloroethane-d5	1.648	69	36528	45.293	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	90.580%		
11) 1,1-Dichloroethene-d2	2.288	65	42442	55.218	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	110.440%		
21) 2-Butanone-d5	4.465	46	140604	122.345	ug/L	0.01
Spiked Amount	100.000	Range 40 - 130	Recovery =	122.340%		
24) Chloroform-d	5.044	84	190188	53.669	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	107.340%		
26) 1,2-Dichloroethane-d4	5.946	65	126514	53.778	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	107.560%		
32) Benzene-d6	5.964	84	380810	50.206	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	100.420%		
36) 1,2-Dichloropropane-d6	7.305	67	108902	47.506	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	95.020%		
41) Toluene-d8	8.647	98	336496	50.573	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	101.140%		
43) trans-1,3-Dichloroprop...	8.945	79	49473	47.690	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	95.380%		
47) 2-Hexanone-d5	9.384	63	97785	114.250	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	114.250%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	162786	56.319	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	112.640%		
66) 1,2-Dichlorobenzene-d4	12.317	152	111431	57.182	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	114.360%		
Target Compounds						
48) 2-Hexanone	9.384	43	12032	5.835	ug/L #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
 Data File : VX043908.D
 Acq On : 20 Nov 2024 10:42
 Operator : JC/MD
 Sample : VX1120MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :


Quant Time: Nov 21 00:39:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 21 00:38:46 2024
 Response via : Initial Calibration

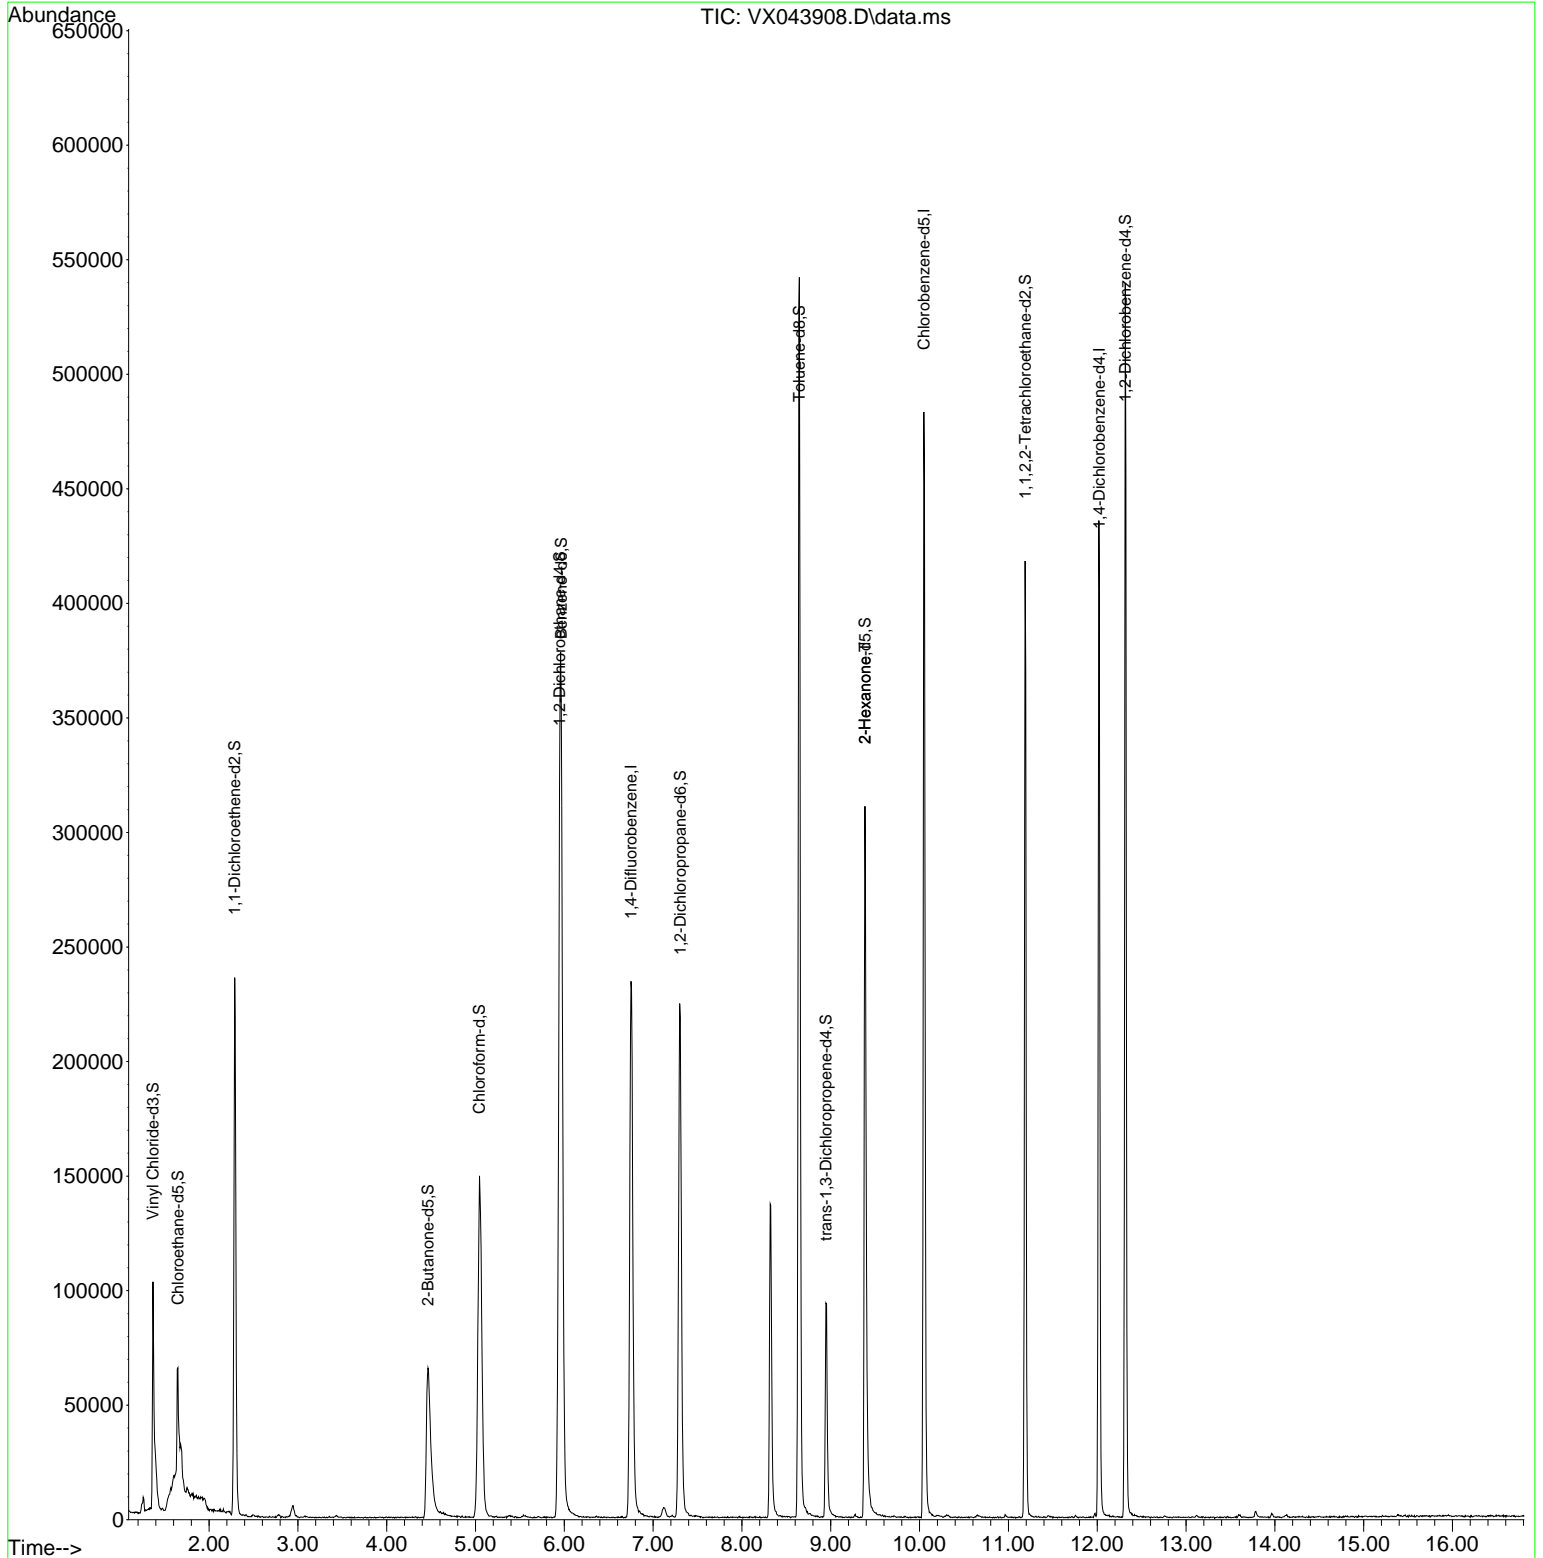

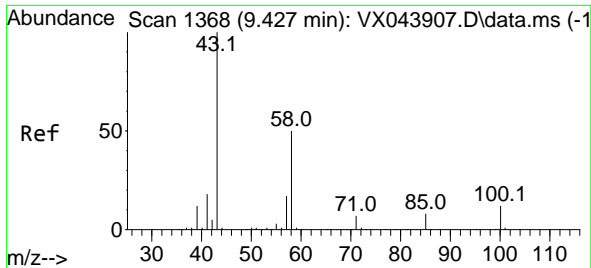

#48
 2-Hexanone
 Concen: 5.835 ug/L
 RT: 9.384 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VX043908.D
 Acq: 20 Nov 2024 10:42

Instrument :
 MSVOA_X
 ClientSampleId :

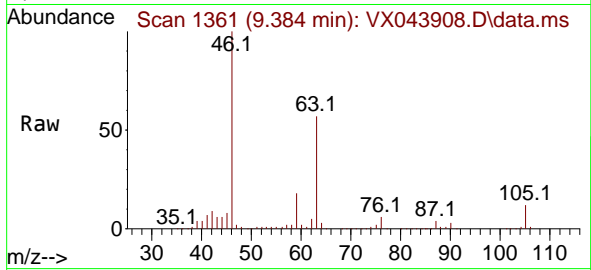

Tgt Ion: 43 Resp: 12032

Ion	Ratio	Lower	Upper
43	100		
58	30.6	45.4	68.2#
57	23.4	15.4	23.0#
100	0.7	10.6	15.8#

