

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
 Data File : VX043908.D
 Acq On : 20 Nov 2024 10:42
 Operator : JC/MD
 Sample : VX1120WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK731

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111924WMA.M
 Title : VOC Analysis

Signal : TIC: VX043908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	61	rVB	99582	150699	13.38%	1.923%
2	1.648	89	92	96	rBV	44623	60783	5.40%	0.776%
3	2.288	191	197	210	rVB	234668	362806	32.21%	4.630%
4	2.678	259	261	262	rBV2	541	353	0.03%	0.005%
5	2.745	270	272	273	rVB2	539	310	0.03%	0.004%
6	2.782	273	278	282	rVB4	1455	2897	0.26%	0.037%
7	2.818	282	284	287	rBV2	681	718	0.06%	0.009%
8	2.946	299	305	310	rBV2	4557	9067	0.80%	0.116%
9	3.203	345	347	348	rBV	331	235	0.02%	0.003%
10	3.300	361	363	364	rVB2	372	217	0.02%	0.003%
11	3.355	368	372	374	rBV3	581	546	0.05%	0.007%
12	3.520	397	399	402	rBV2	373	491	0.04%	0.006%
13	3.556	402	405	406	rBV	375	373	0.03%	0.005%
14	3.635	417	418	420	rBV	446	210	0.02%	0.003%
15	3.745	435	436	437	rBV	346	233	0.02%	0.003%
16	3.861	453	455	457	rVB2	281	220	0.02%	0.003%
17	3.977	472	474	475	rBV	293	222	0.02%	0.003%
18	4.019	479	481	482	rVV	330	210	0.02%	0.003%
19	4.074	489	490	492	rVB2	440	274	0.02%	0.003%
20	4.099	492	494	495	rBV	460	323	0.03%	0.004%
21	4.123	495	498	499	rBV2	293	271	0.02%	0.003%
22	4.227	513	515	516	rBV	373	291	0.03%	0.004%
23	4.355	534	536	539	rBV2	473	557	0.05%	0.007%
24	4.465	546	554	575	rBV2	65441	239319	21.25%	3.054%
25	4.849	615	617	620	rVB2	633	372	0.03%	0.005%
26	4.885	621	623	624	rVB2	491	241	0.02%	0.003%
27	5.044	638	649	667	rBV	149154	459976	40.84%	5.870%
28	5.355	699	700	701	rBV	756	450	0.04%	0.006%
29	5.519	725	727	728	rBV	413	339	0.03%	0.004%
30	5.537	728	730	732	rVV2	817	632	0.06%	0.008%
31	5.708	754	758	764	rVB3	518	911	0.08%	0.012%
32	5.958	788	799	824	rBV2	377735	1126385	100.00%	14.375%
33	6.446	877	879	880	rBV	452	313	0.03%	0.004%
34	6.751	920	929	943	rBV	233956	584161	51.86%	7.455%
35	7.299	1010	1019	1038	rBV	224203	507955	45.10%	6.483%
36	7.568	1062	1063	1066	rBV	303	397	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
 Data File : VX043908.D
 Acq On : 20 Nov 2024 10:42
 Operator : JC/MD
 Sample : VX1120WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK731

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

37	7.836	1105	1107	1110	rVB2	482	357	0.03%	0.005%
38	7.964	1126	1128	1129	rBV2	558	472	0.04%	0.006%
39	8.031	1137	1139	1141	rBV	278	231	0.02%	0.003%
40	8.080	1145	1147	1148	rBV2	465	204	0.02%	0.003%
41	8.147	1154	1158	1159	rVB2	586	523	0.05%	0.007%
42	8.202	1165	1167	1169	rVB2	570	354	0.03%	0.005%
43	8.263	1175	1177	1180	rVB2	400	241	0.02%	0.003%
44	8.317	1181	1186	1202	rVV	136755	242257	21.51%	3.092%
45	8.647	1233	1240	1257	rBV	541193	881265	78.24%	11.247%
46	8.891	1278	1280	1281	rBV	324	323	0.03%	0.004%
47	8.945	1284	1289	1301	rBV	93405	151329	13.43%	1.931%
48	9.201	1329	1331	1334	rVB2	437	451	0.04%	0.006%
49	9.232	1334	1336	1337	rBV2	416	306	0.03%	0.004%
50	9.275	1340	1343	1345	rBV3	1401	1320	0.12%	0.017%
51	9.384	1356	1361	1381	rBV	310196	513735	45.61%	6.556%
52	9.896	1442	1445	1446	rVB2	418	381	0.03%	0.005%
53	9.915	1446	1448	1449	rBV2	302	264	0.02%	0.003%
54	9.982	1455	1459	1460	rBV2	444	573	0.05%	0.007%
55	10.049	1465	1470	1480	rBV	482675	690561	61.31%	8.813%
56	10.305	1505	1512	1514	rBV4	1177	2013	0.18%	0.026%
57	10.470	1538	1539	1542	rBV2	347	249	0.02%	0.003%
58	10.628	1562	1565	1566	rBV	486	469	0.04%	0.006%
59	10.829	1597	1598	1600	rBV2	359	255	0.02%	0.003%
60	10.854	1600	1602	1603	rBV	363	244	0.02%	0.003%
61	10.878	1604	1606	1608	rVB2	559	481	0.04%	0.006%
62	10.908	1608	1611	1613	rVB2	519	525	0.05%	0.007%
63	10.963	1618	1620	1627	rVB3	1267	1483	0.13%	0.019%
64	11.122	1644	1646	1649	rVB3	513	517	0.05%	0.007%
65	11.189	1652	1657	1664	rBV	417267	546030	48.48%	6.968%
66	11.451	1696	1700	1703	rBV5	812	1288	0.11%	0.016%
67	11.683	1736	1738	1740	rBV2	368	401	0.04%	0.005%
68	11.756	1746	1750	1755	rVB3	1185	1680	0.15%	0.021%
69	11.799	1755	1757	1758	rBV	348	317	0.03%	0.004%
70	11.975	1783	1786	1788	rBV4	1864	1997	0.18%	0.025%
71	12.018	1788	1793	1804	rVV	434825	571070	50.70%	7.288%
72	12.317	1837	1842	1851	rBV	538623	687188	61.01%	8.770%
73	12.609	1888	1890	1892	rBV3	521	560	0.05%	0.007%
74	12.713	1904	1907	1911	rBV2	361	523	0.05%	0.007%
75	12.762	1911	1915	1918	rBV2	791	1192	0.11%	0.015%
76	12.859	1928	1931	1933	rBV2	363	377	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
 Data File : VX043908.D
 Acq On : 20 Nov 2024 10:42
 Operator : JC/MD
 Sample : VX1120WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK731

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
 Title : VOC Analysis

77	13.067	1963	1965	1969	rBV	408	519	0.05%	0.007%
78	13.121	1971	1974	1977	rVV4	988	1374	0.12%	0.018%
79	13.176	1981	1983	1984	rVB2	456	255	0.02%	0.003%
80	13.195	1984	1986	1989	rVB2	525	542	0.05%	0.007%
81	13.219	1989	1990	1991	rBV	450	232	0.02%	0.003%
82	13.329	2007	2008	2009	rBV	445	317	0.03%	0.004%
83	13.384	2015	2017	2018	rVB	477	239	0.02%	0.003%
84	13.463	2028	2030	2032	rBV2	730	697	0.06%	0.009%
85	13.567	2046	2047	2048	rVB	609	223	0.02%	0.003%
86	13.591	2048	2051	2053	rBV3	1365	1654	0.15%	0.021%
87	13.786	2079	2083	2090	rVB3	2560	4287	0.38%	0.055%
88	13.963	2109	2112	2116	rBV4	1921	2897	0.26%	0.037%
89	14.274	2161	2163	2165	rBV	433	264	0.02%	0.003%
90	14.353	2175	2176	2179	rVB2	373	346	0.03%	0.004%
91	14.383	2179	2181	2183	rBV	699	352	0.03%	0.004%
92	14.408	2183	2185	2186	rBV	398	238	0.02%	0.003%
93	14.633	2221	2222	2224	rBV3	507	326	0.03%	0.004%
94	14.658	2224	2226	2229	rVB3	485	513	0.05%	0.007%
95	14.725	2235	2237	2238	rBV	639	388	0.03%	0.005%
96	14.743	2238	2240	2242	rVB	421	356	0.03%	0.005%
97	14.914	2265	2268	2270	rBV2	523	440	0.04%	0.006%
98	14.944	2272	2273	2275	rBV2	638	345	0.03%	0.004%
99	15.213	2315	2317	2319	rBV2	696	567	0.05%	0.007%
100	15.511	2365	2366	2368	rBV2	880	640	0.06%	0.008%

Sum of corrected areas: 7835774




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
Data File : VX043908.D
Acq On : 20 Nov 2024 10:42
Operator : JC/MD
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK731

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

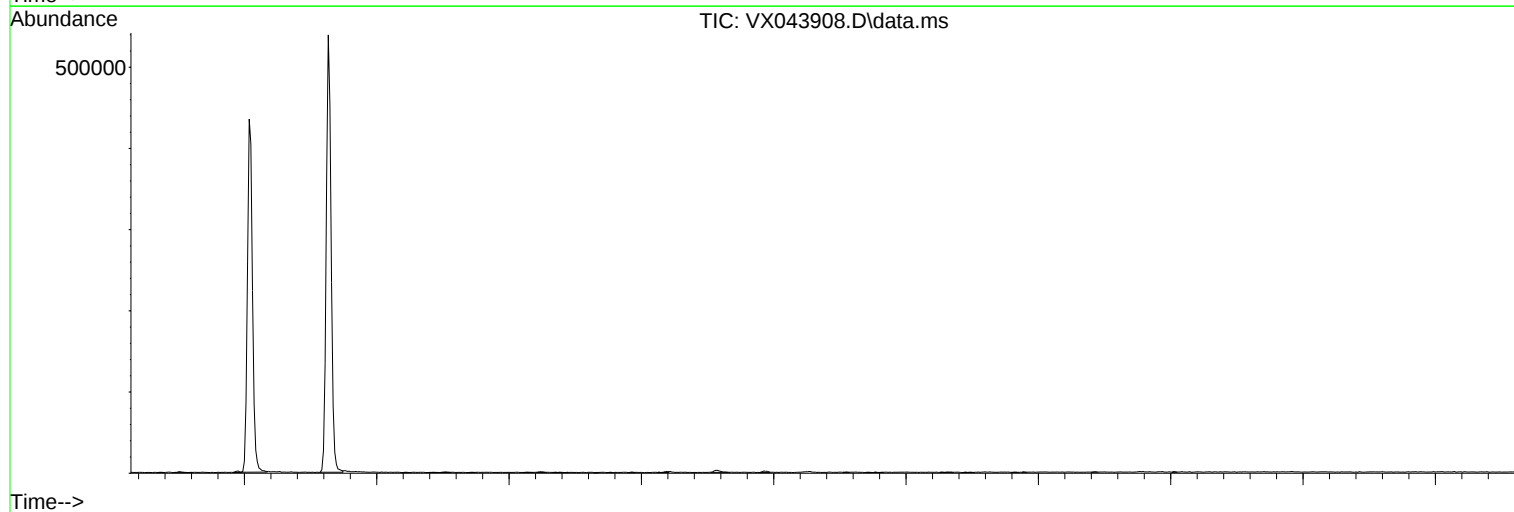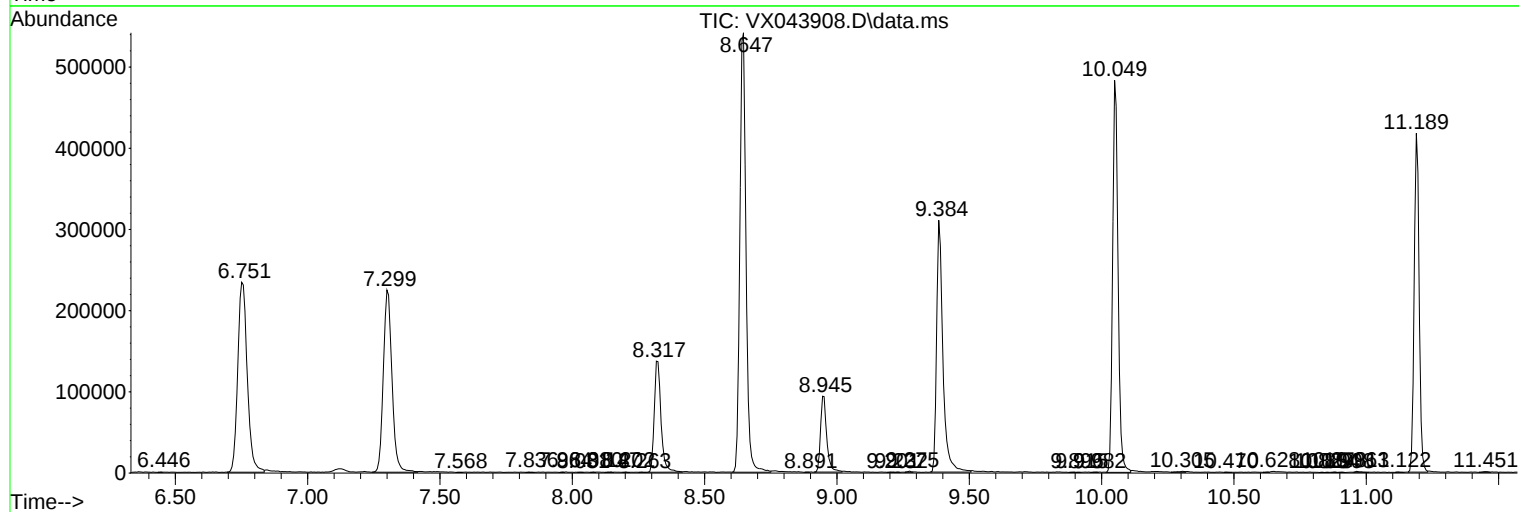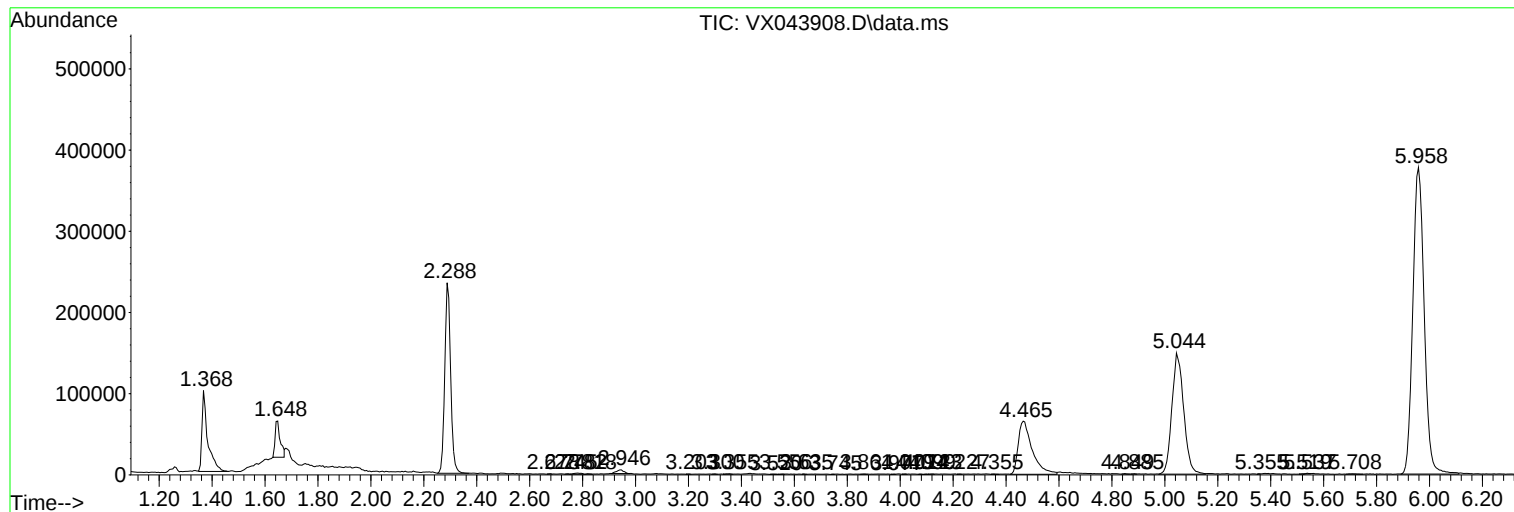

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
Data File : VX043908.D
Acq On : 20 Nov 2024 10:42
Operator : JC/MD
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK731

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
Data File : VX043908.D
Acq On : 20 Nov 2024 10:42
Operator : JC/MD
Sample : VX1120WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK731

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc