
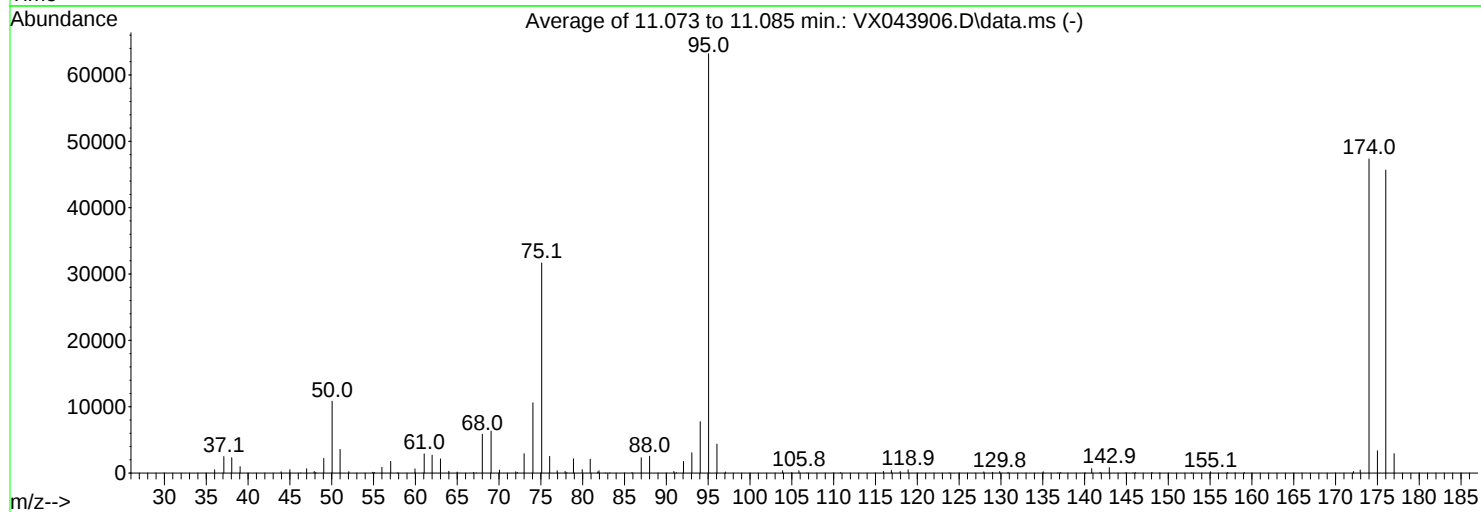


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112024\
Data File : VX043906.D
Acq On : 20 Nov 2024 09:41
Operator : JC/MD
Sample : BFB702
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB702

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111924WMA.M
Title : VOC Analysis
Last Update : Thu Nov 21 00:38:46 2024

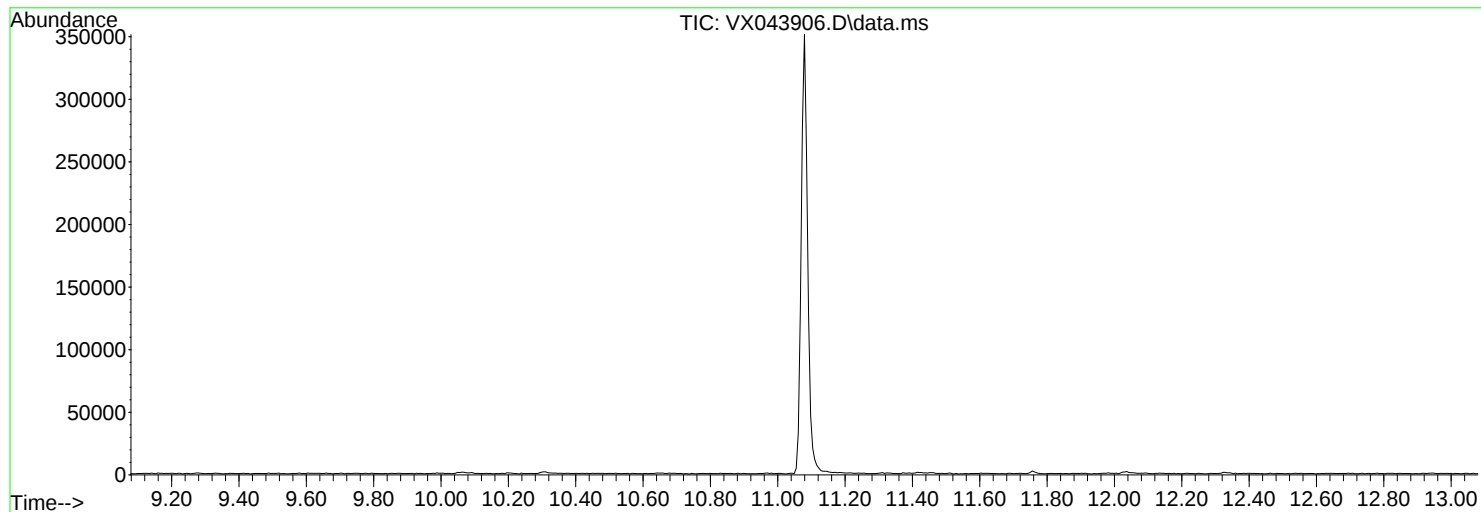

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	10840	PASS
75	95	30	80	50.1	31672	PASS
95	95	100	100	100.0	63200	PASS
96	95	5	9	6.9	4372	PASS
173	174	0.00	2	1.0	460	PASS
174	95	50	120	74.9	47347	PASS
175	174	5	9	7.1	3366	PASS
176	174	95	101	96.5	45667	PASS
177	176	5	9	6.4	2937	PASS

Scan 1632 (11.037 min): VX043906.D\data.ms
BFB702

m/z	Abundance
37.80	53.0
39.10	167.0
40.00	726.0
43.90	382.0

Instrument :
MSVOA_X
ClientSampleId :
BFB702

m/z	Abundance
36.00	392.0
37.10	2625.0
38.10	2512.0
39.00	1245.0
40.00	618.0
44.00	525.0
45.00	650.0
46.30	80.0
46.90	553.0
47.90	430.0
49.00	2252.0
50.10	10936.0
51.00	3759.0
52.10	257.0
54.90	216.0
56.00	783.0
57.00	1855.0
59.90	476.0
61.00	2999.0
62.00	2948.0
63.00	2417.0
64.00	304.0
65.10	205.0
67.30	71.0
68.00	6233.0
69.10	6374.0
70.00	514.0
72.00	243.0
73.00	2835.0
74.00	10505.0
75.10	30840.0
76.10	2772.0
76.90	455.0
78.00	467.0
78.90	2007.0
79.90	451.0
80.90	2150.0
81.80	549.0
82.70	76.0
87.00	2406.0
88.00	2494.0
91.00	269.0
92.10	1629.0
93.10	2800.0
94.00	7389.0
95.00	60232.0
96.00	4624.0
97.10	135.0
103.90	388.0
105.00	69.0
106.00	366.0
110.80	102.0
116.00	271.0
116.90	280.0
118.00	289.0
119.00	417.0
128.00	132.0
129.00	179.0
129.90	206.0
130.90	197.0
135.00	173.0
137.10	98.0
140.10	61.0
140.80	595.0
141.80	109.0
143.00	586.0
144.90	63.0
146.20	115.0
148.10	90.0
155.10	173.0
157.20	59.0
159.10	82.0
172.10	176.0
173.00	416.0
174.00	40720.0
175.00	3018.0
176.00	37784.0
177.00	2313.0

Instrument :
MSVOA_X
ClientSampleId :
BFB702

m/z	Abundance
36.00	595.0
37.10	2835.0
38.00	2580.0
39.10	1299.0
40.00	619.0
44.10	743.0
44.90	443.0
47.00	748.0
48.10	350.0
49.10	2688.0
50.10	13059.0
51.00	4388.0
52.10	191.0
54.90	182.0
56.00	1226.0
57.00	2058.0
57.80	55.0
60.00	829.0
61.10	3429.0
62.00	3028.0
63.00	2374.0
64.10	302.0
64.90	194.0
67.00	205.0
68.00	6801.0
69.00	7207.0
70.10	530.0
72.00	367.0
73.00	3478.0
74.10	12600.0
75.10	37760.0
76.00	2979.0
76.90	194.0
77.80	336.0
78.90	2886.0
80.00	638.0
80.90	2366.0
82.00	498.0
83.20	63.0
85.90	167.0
87.00	2641.0
88.00	2770.0
90.80	299.0
91.20	195.0
91.90	2211.0
93.00	3929.0
94.10	9701.0
95.10	76200.0
96.10	5305.0
97.10	204.0
103.90	431.0
105.00	100.0
105.80	375.0
106.80	63.0
110.00	80.0
110.80	62.0
116.00	250.0
116.90	635.0
117.90	293.0
118.90	569.0
123.80	64.0
128.00	269.0
129.00	134.0
129.80	283.0
130.80	110.0
135.10	249.0
136.80	63.0
137.20	91.0
140.90	933.0
141.90	97.0
142.90	1174.0
144.90	93.0
146.00	102.0
148.10	116.0
152.80	87.0
155.00	338.0
157.10	131.0
158.00	76.0
159.10	130.0
172.20	230.0
173.00	599.0
174.00	55744.0
175.00	3656.0
176.00	53560.0
177.00	3766.0

Instrument :
MSVOA_X
ClientSampleId :
BFB702

m/z	Abundance
36.00	504.0
37.10	2008.0
38.00	1876.0
39.10	861.0
40.00	828.0
44.00	495.0
45.10	469.0
47.10	647.0
47.90	302.0
49.00	1681.0
50.00	8525.0
51.00	2565.0
51.90	214.0
55.10	263.0
56.00	608.0
57.10	1382.0
57.90	54.0
60.00	578.0
61.00	2262.0
62.00	2123.0
63.00	1634.0
63.90	233.0
65.00	90.0
66.90	124.0
68.00	4553.0
69.00	5421.0
70.00	328.0
72.20	266.0
73.00	2466.0
74.00	8683.0
75.10	26416.0
76.10	1836.0
77.00	412.0
78.10	231.0
79.00	1584.0
79.90	476.0
80.90	1747.0
81.90	571.0
83.30	66.0
85.90	83.0
87.00	1898.0
88.00	2336.0
90.90	167.0
92.10	1424.0
93.00	2461.0
94.10	6175.0
95.00	53168.0
96.10	3188.0
97.00	160.0
103.90	217.0
105.80	300.0
110.80	66.0
115.90	244.0
116.90	361.0
117.90	162.0
118.80	547.0
127.90	192.0
129.00	56.0
129.90	217.0
130.90	65.0
135.10	177.0
136.80	82.0
137.10	71.0
140.90	522.0
141.90	163.0
142.90	695.0
145.00	71.0
145.80	96.0
148.00	118.0
149.00	60.0
155.00	95.0
157.00	131.0
172.10	312.0
172.80	364.0
174.00	45576.0
175.00	3423.0
176.00	45656.0
177.00	2732.0

Instrument :
MSVOA_X
ClientSampleId :
BFB702