

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112118\
 Data File : VX006141.D
 Acq On : 22 Nov 2018 00:05
 Operator : JC/MD
 Sample : J6047-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EP2-TB-02

Quant Time: Nov 22 04:09:58 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 21 08:15:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	331781	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	486452	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	470548	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	228895	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	202392	52.64	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.28%	
35) Dibromofluoromethane	5.50	113	163363	52.32	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.64%	
50) Toluene-d8	8.71	98	587803	49.35	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.70%	
62) 4-Bromofluorobenzene	11.14	95	208534	46.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.32%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112118\
Data File : VX006141.D
Acq On : 22 Nov 2018 00:05
Operator : JC/MD
Sample : J6047-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EP2-TB-02

Quant Time: Nov 22 04:09:58 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 21 08:15:54 2018
Response via : Initial Calibration

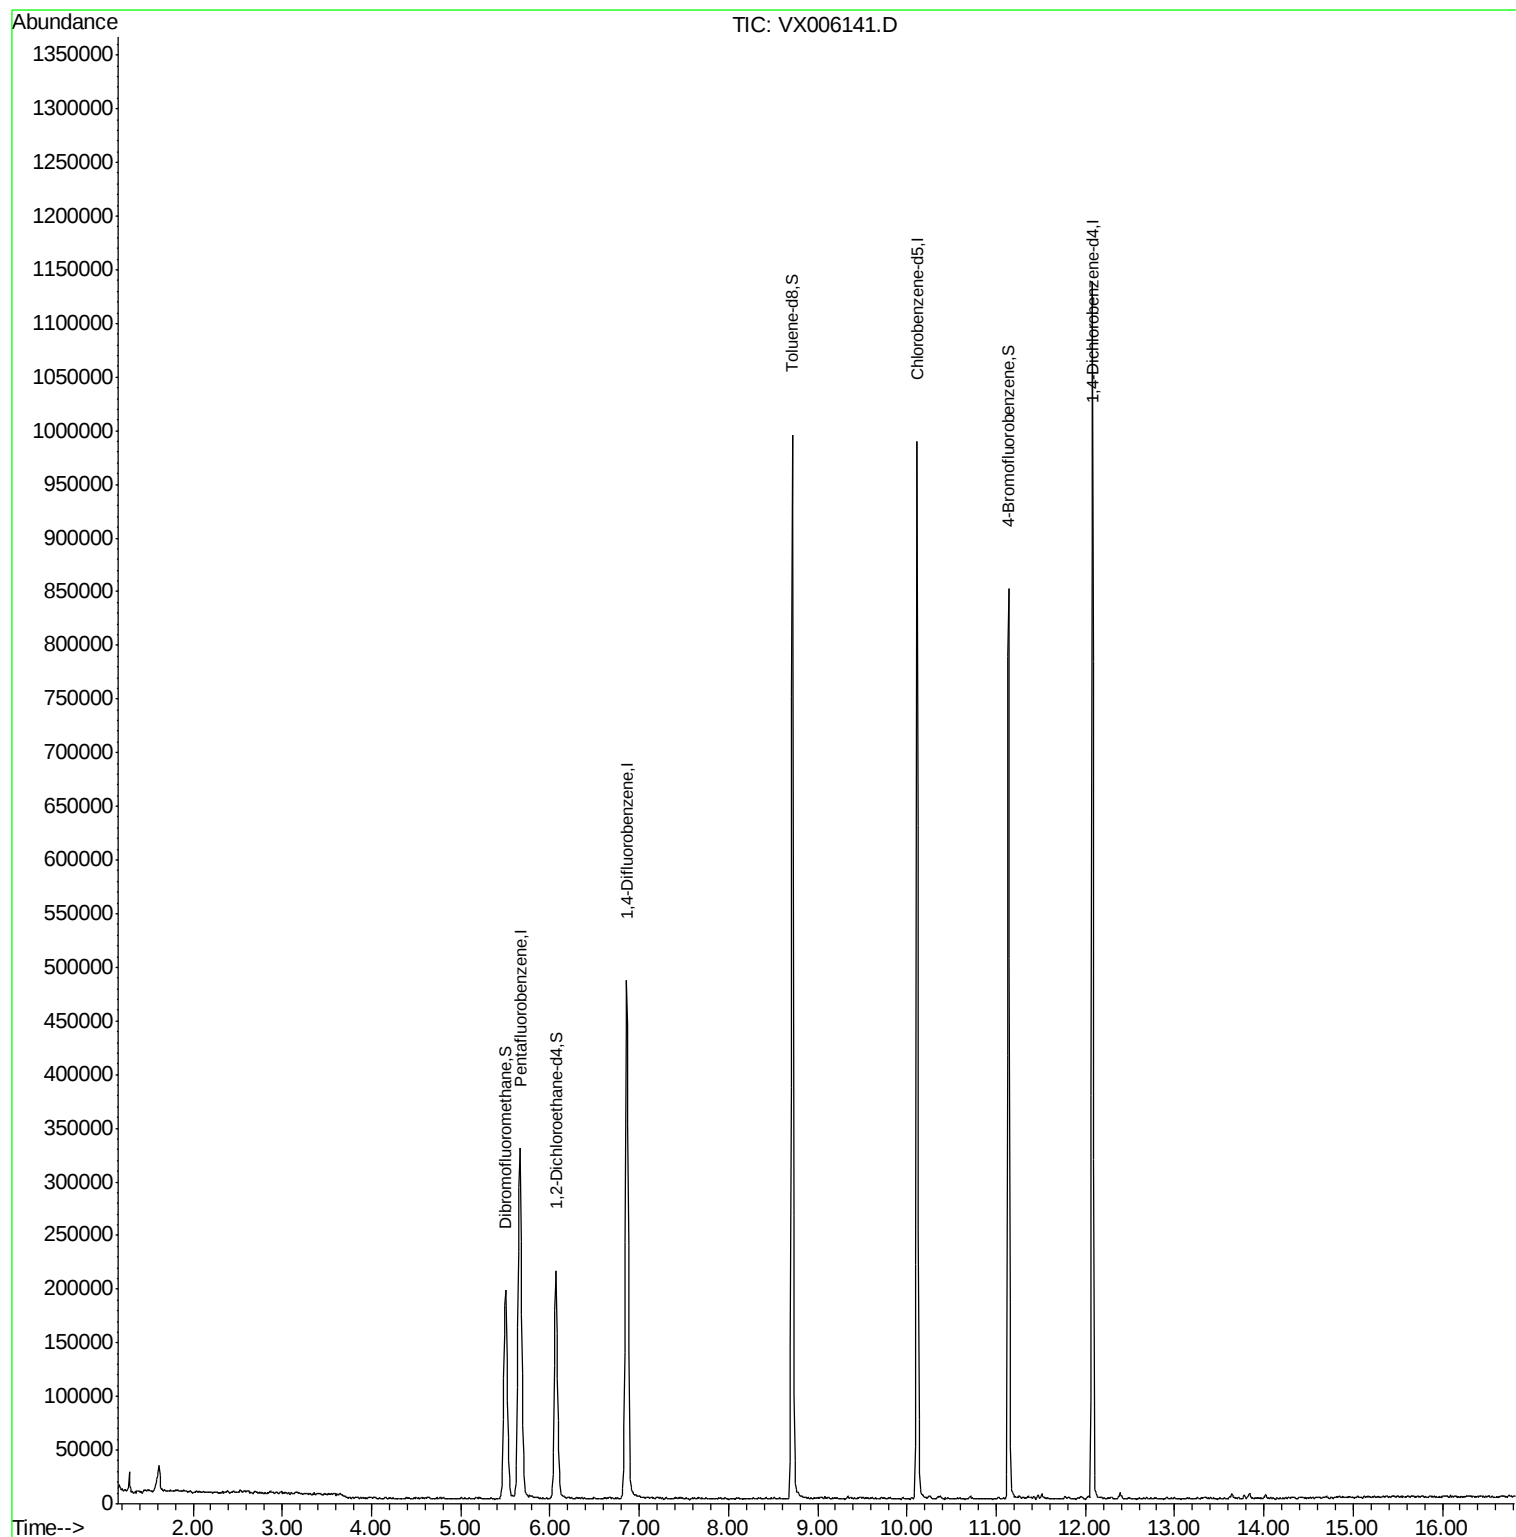

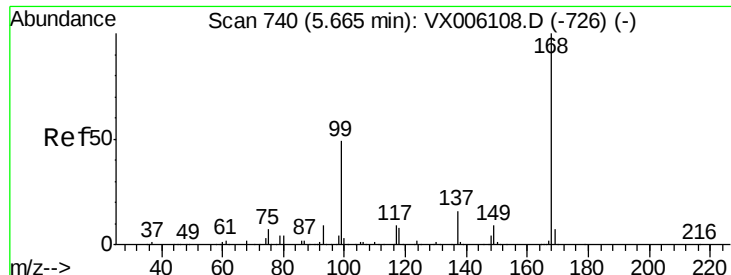

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006141.D

Acq: 22 Nov 2018 00:05

Instrument :

MSVOA_X

ClientSampleId :


EP2-TB-02

Tot Ion:168 Resp: 331781

Ion Ratio Lower Upper

168 100

99 47.4 39.2 58.8

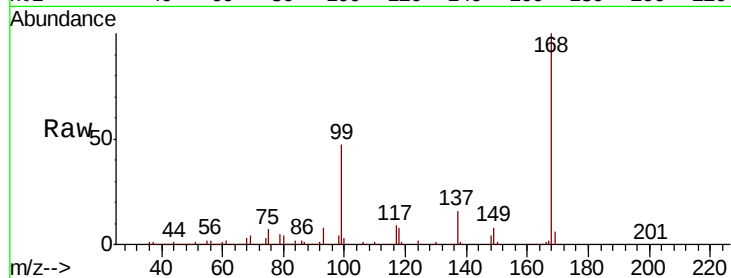

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0



5.67

100000

50000

0

Time--> 5.50 5.60 5.70 5.80

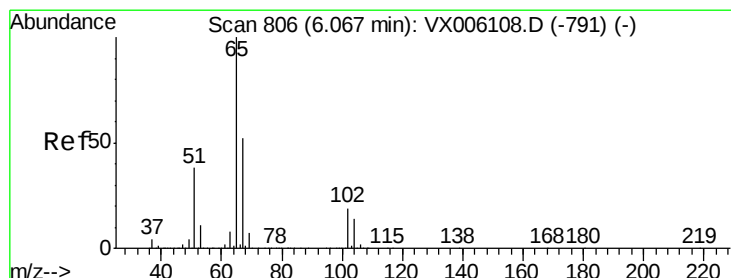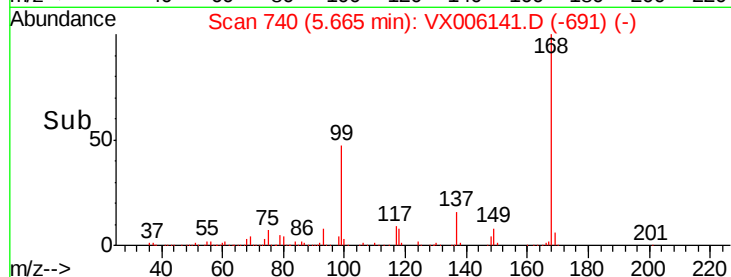

#33

1,2-Dichloroethane-d4

Concen: 52.645 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX006141.D


Acq: 22 Nov 2018 00:05

Tgt Ion: 65 Resp: 202392

Ion Ratio Lower Upper

65 100

67 52.9 0.0 105.8

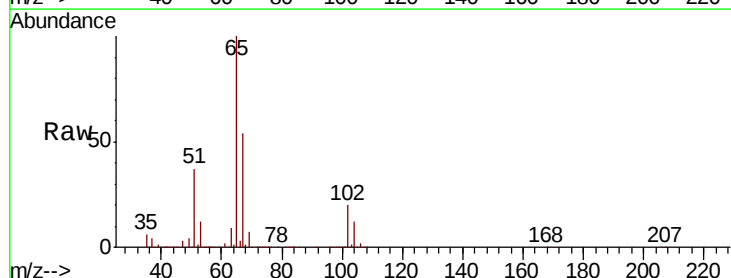

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

80000


60000


40000

20000

0

Time--> 5.90 6.00 6.10 6.20 6.30

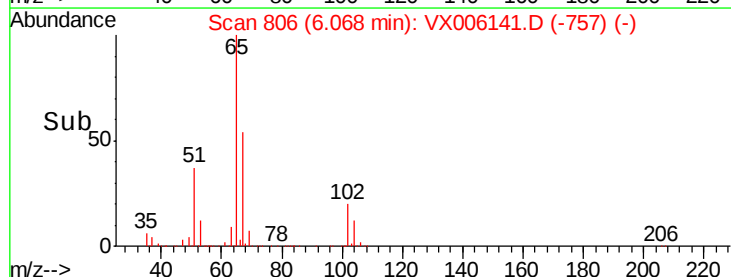

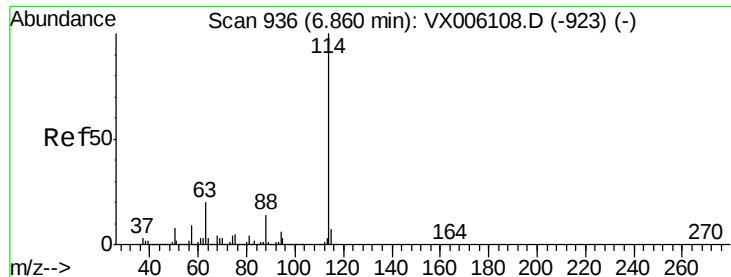

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006141.D

Acq: 22 Nov 2018 00:05

Instrument :

MSVOA_X

ClientSampled :

EP2-TB-02


Tot Ion:114 Resp: 486452

Ion Ratio Lower Upper

114 100

63 21.1 0.0 39.2




88 15.4 0.0 28.6

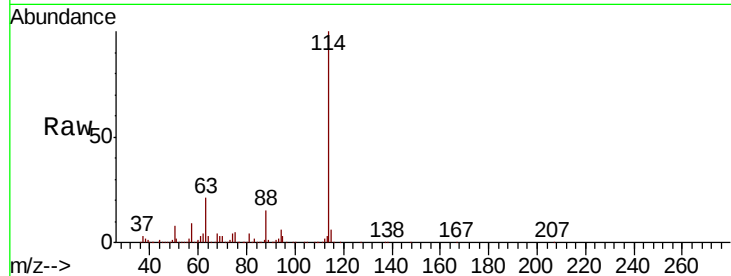

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

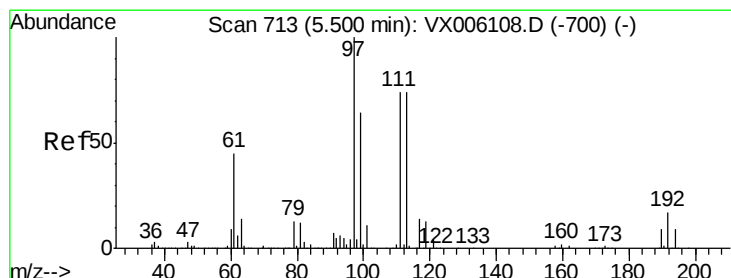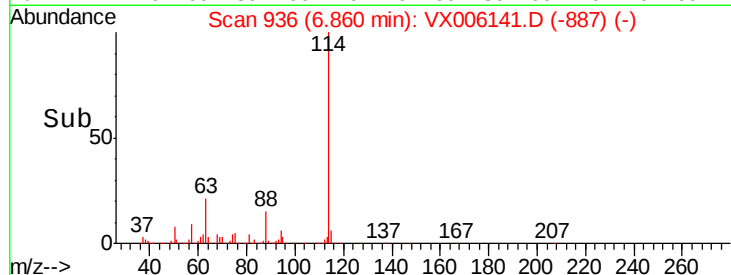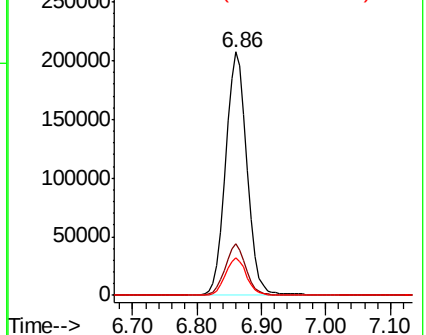

#35

Dibromofluoromethane

Concen: 52.316 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX006141.D

Acq: 22 Nov 2018 00:05


Tgt Ion:113 Resp: 163363

Ion Ratio Lower Upper

113 100

111 103.1 81.5 122.3



192 23.3 18.6 28.0

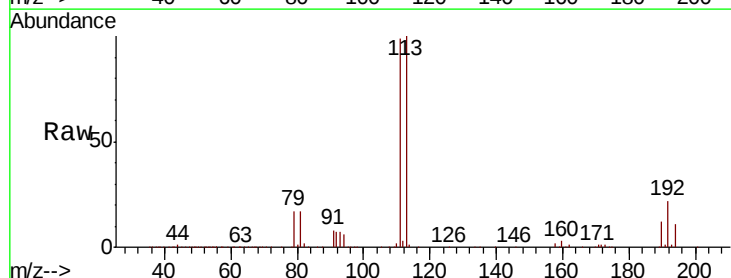


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

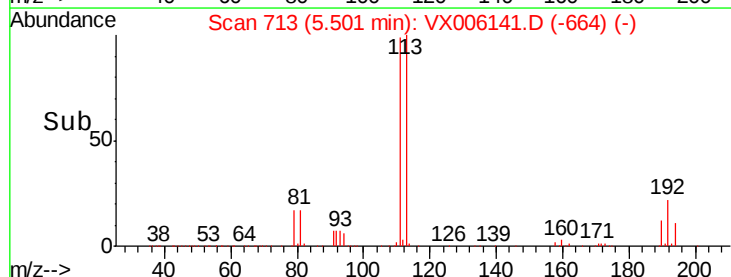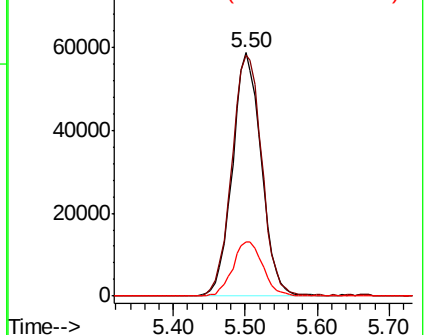

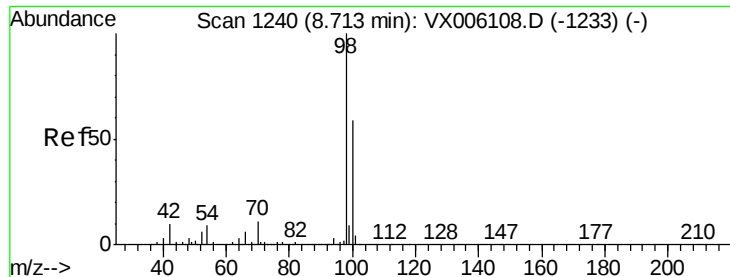

#50

Toluene-d8

Concen: 49.353 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006141.D

Acq: 22 Nov 2018 00:05

Instrument :

MSVOA_X

ClientSampleId :


EP2-TB-02

Tot Ion: 98 Resp: 587803

Ion Ratio Lower Upper




98 100

100 62.4 51.0 76.4

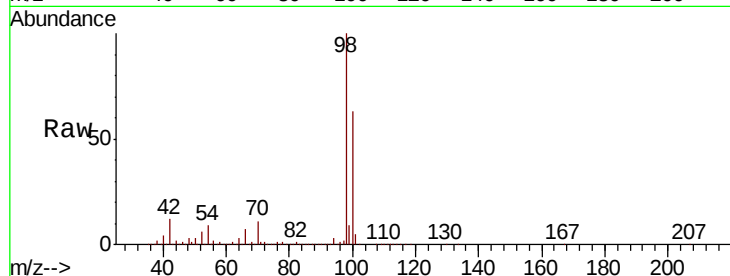

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

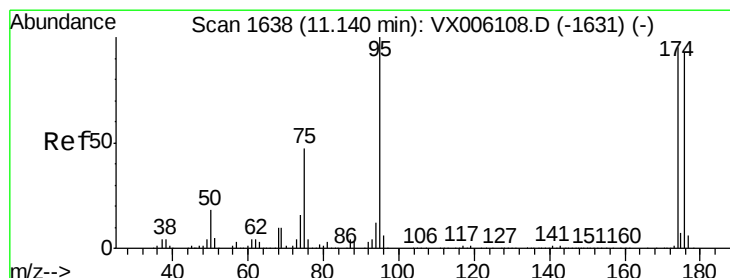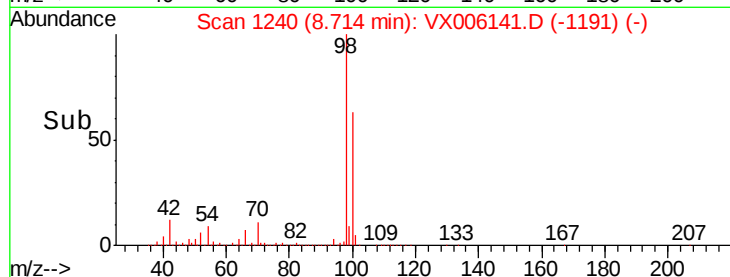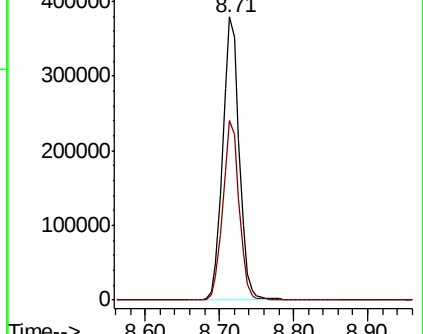

#62

4-Bromofluorobenzene

Concen: 46.665 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. 0.00 min

Lab File: VX006141.D

Acq: 22 Nov 2018 00:05


Tgt Ion: 95 Resp: 208534

Ion Ratio Lower Upper

95 100

174 94.3 0.0 184.4



176 91.1 0.0 179.0

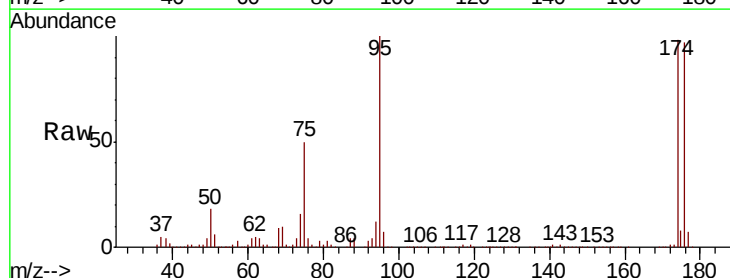


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



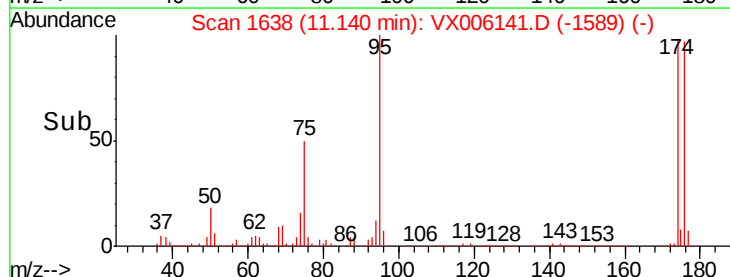
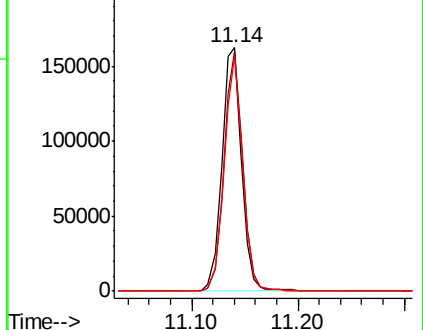


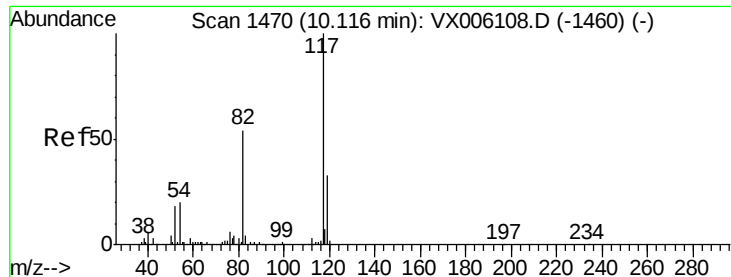

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.00 min
Lab File: VX006141.D
Acq: 22 Nov 2018 00:05

Instrument :
MSVOA_X
ClientSampleId :
EP2-TB-02

Tot Ion:117 Resp: 470548
Ion Ratio Lower Upper
117 100
82 53.6 43.0 64.4
119 32.8 26.1 39.1

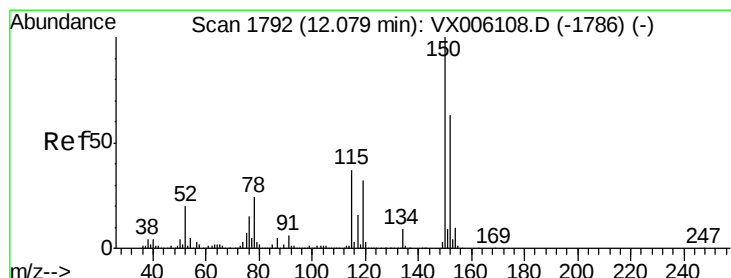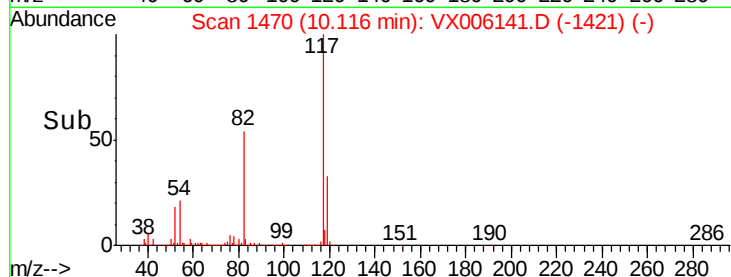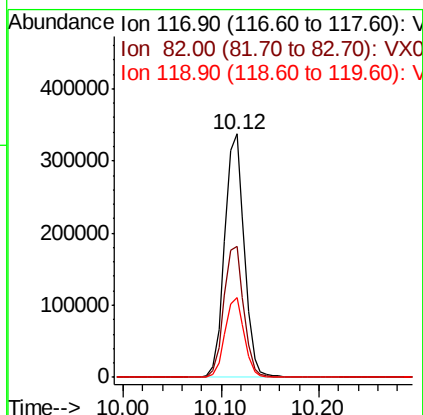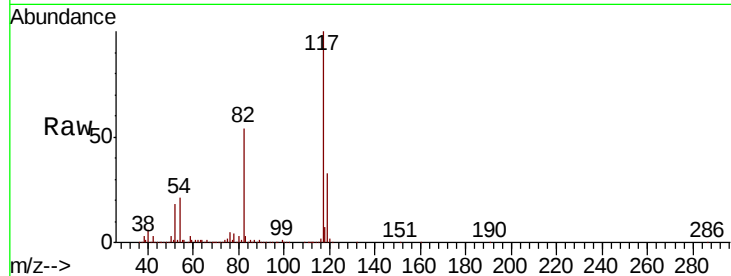

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX006141.D
Acq: 22 Nov 2018 00:05

Tgt Ion:152 Resp: 228895
Ion Ratio Lower Upper
152 100
115 55.4 39.0 116.9
150 156.7 0.0 346.6

