

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112118\
 Data File : VX006146.D
 Acq On : 22 Nov 2018 02:18
 Operator : JC/MD
 Sample : J6047-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EP2-FD-02

Quant Time: Nov 22 04:22:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 21 08:15:54 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	331075	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	496094	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	454733	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	218063	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	204136	53.21	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.42%	
35) Dibromofluoromethane	5.50	113	164836	51.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.52%	
50) Toluene-d8	8.71	98	598183	49.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.50%	
62) 4-Bromofluorobenzene	11.14	95	198095	43.47	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.94%	
Target Compounds						
64) Tetrachloroethene	9.34	164	2961	0.791	ug/l	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112118\
 Data File : VX006146.D
 Acq On : 22 Nov 2018 02:18
 Operator : JC/MD
 Sample : J6047-05
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 EP2-FD-02

Quant Time: Nov 22 04:22:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112018W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 21 08:15:54 2018
 Response via : Initial Calibration




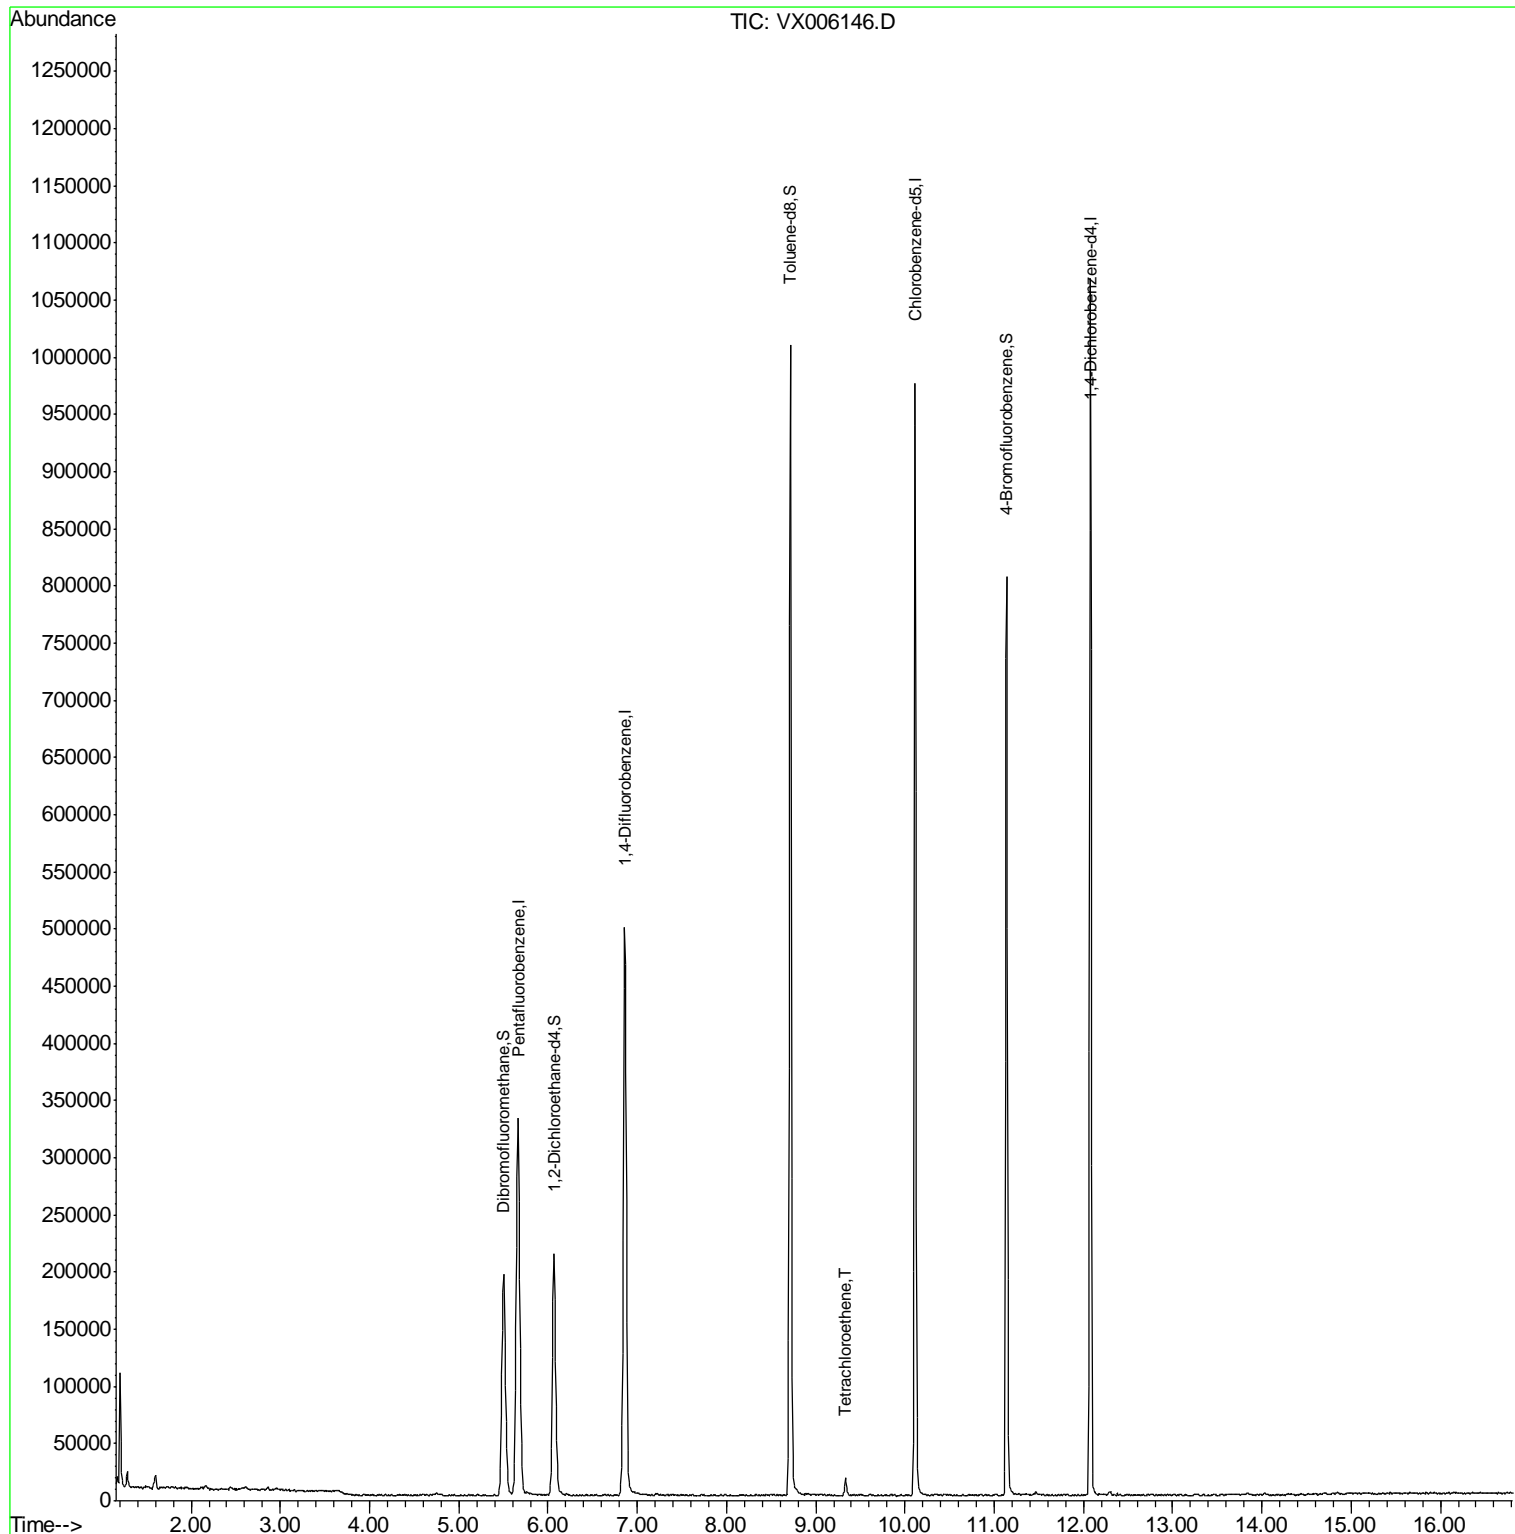


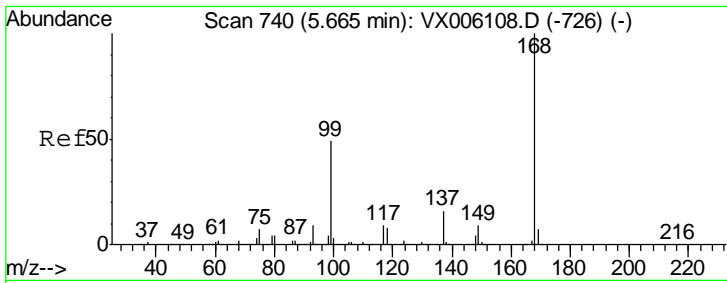

#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.67 min Scan# 740
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18




Instrument :
 MSVOA_X
 ClientSampled :
 EP2-FD-02


Tgt Ion	Resp	Lower	Upper
168	331075		
99	50.6	39.2	58.8

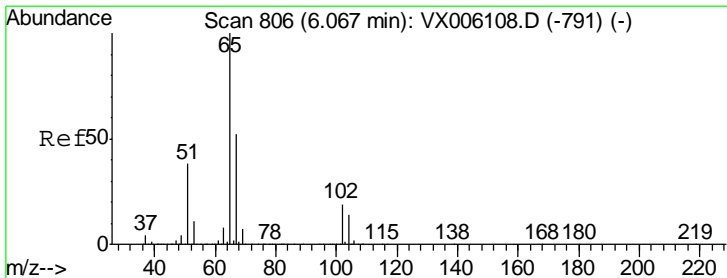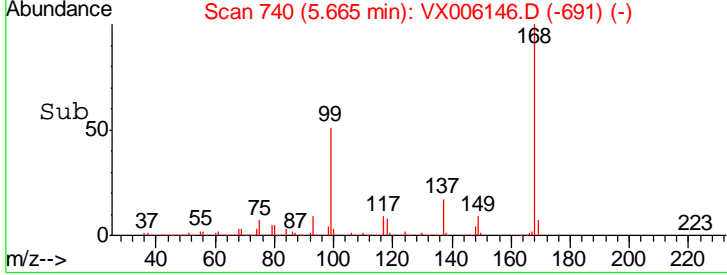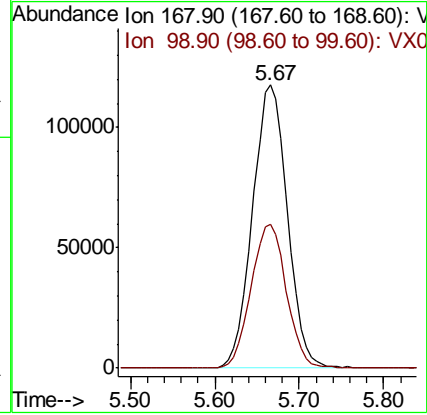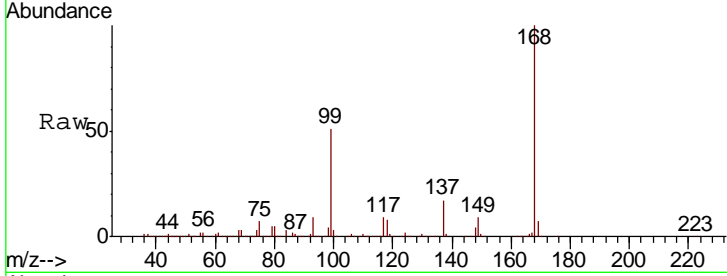

#33
 1,2-Dichloroethane-d4
 Concen: 53.211 ug/l
 RT: 6.07 min Scan# 806
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18

Tgt Ion	Resp	Lower	Upper
65	204136		
67	52.5	0.0	105.8


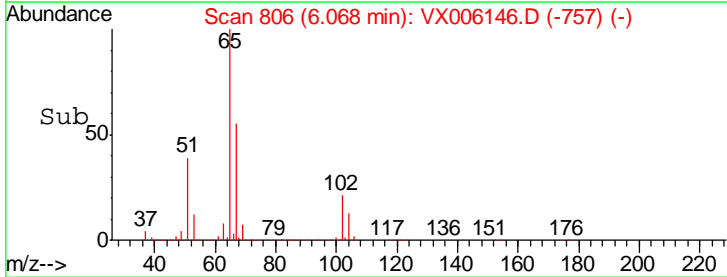
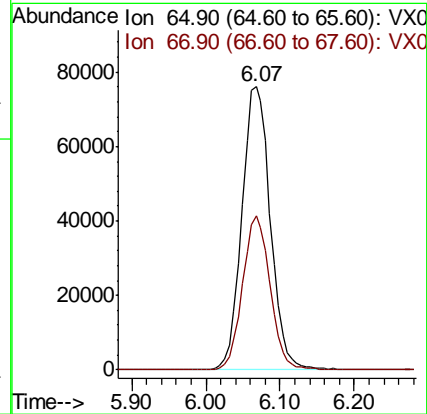
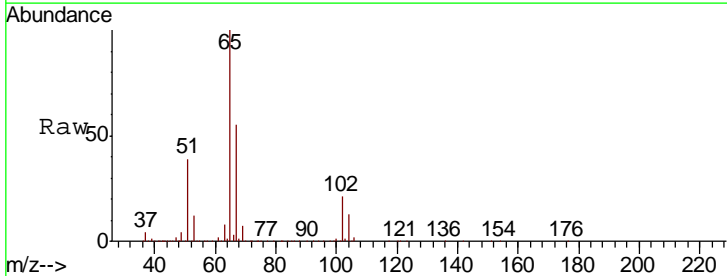


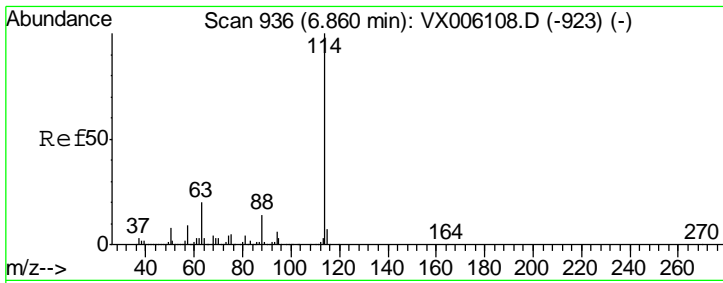

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18




Instrument :
 MSVOA_X
 ClientSampled :
 EP2-FD-02


Tgt Ion	Resp	Lower	Upper
114	496094		
63	20.5	0.0	39.2
88	15.8	0.0	28.6

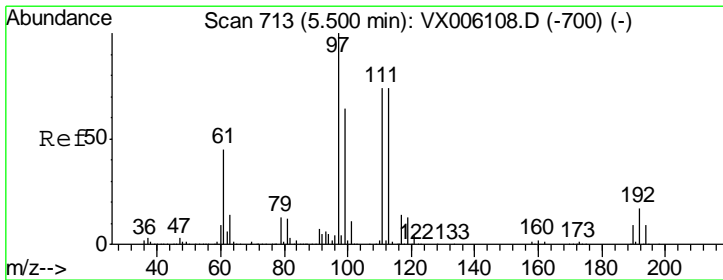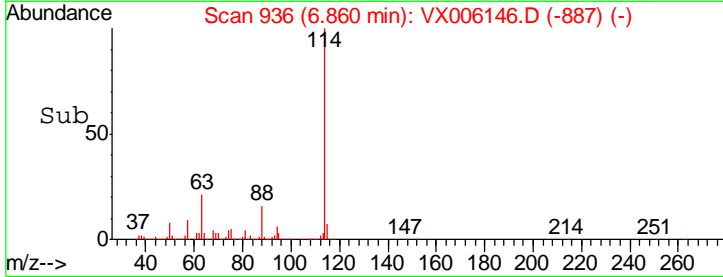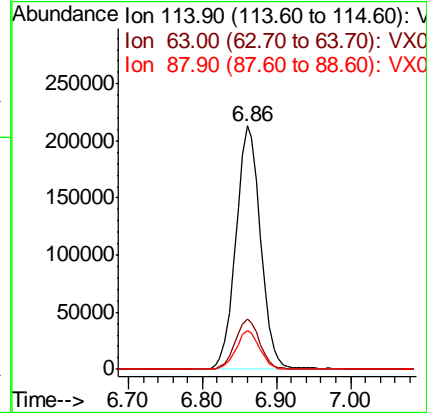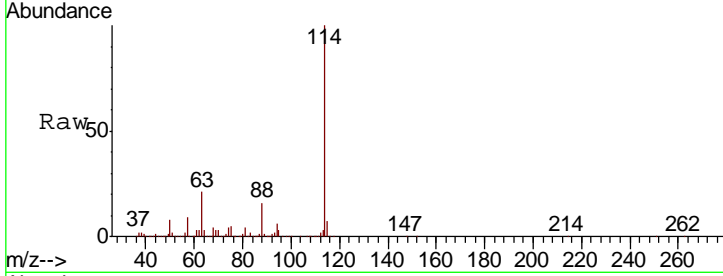

#35
 Dibromofluoromethane
 Concen: 51.762 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18

Tgt Ion	Resp	Lower	Upper
113	164836		
111	102.2	81.5	122.3
192	23.3	18.6	28.0


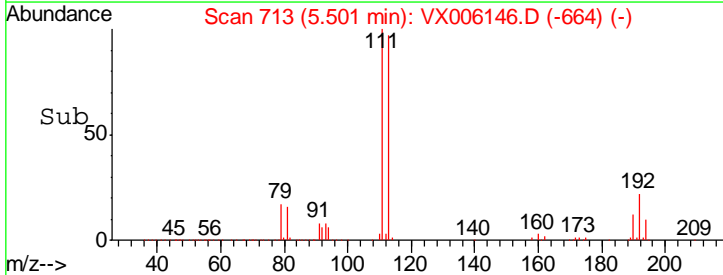
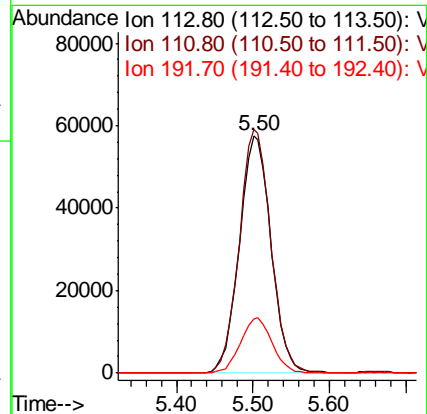
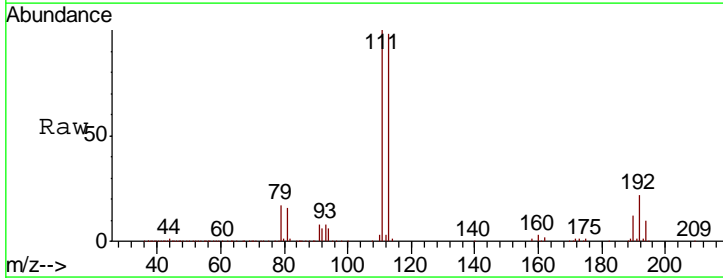


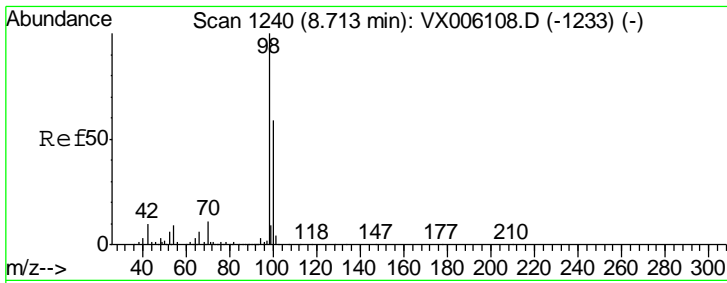

#50
 Toluene-d8
 Concen: 49.248 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18




Instrument :
 MSVOA_X
ClientSampled :
 EP2-FD-02


Tgt Ion	Resp	Lower	Upper
98	598183		
100	63.3	51.0	76.4

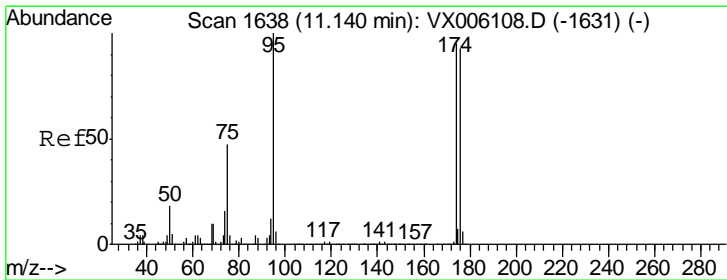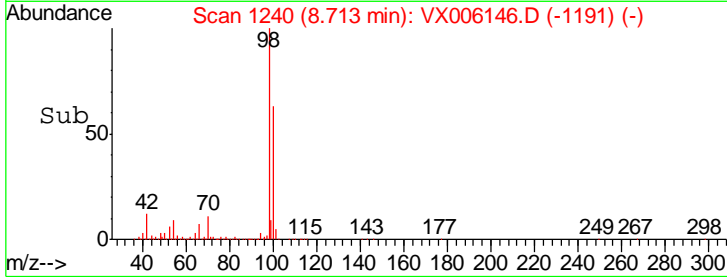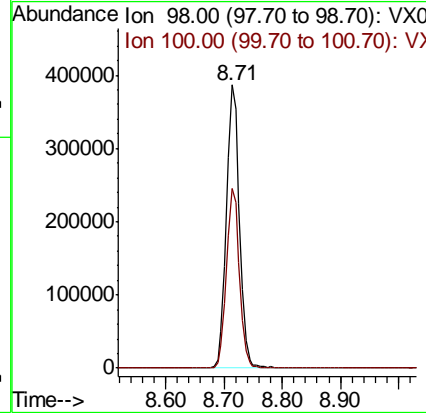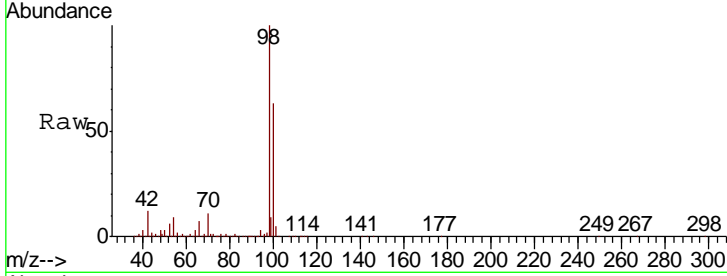

#62
 4-Bromofluorobenzene
 Concen: 43.467 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18

Tgt Ion	Resp	Lower	Upper
95	198095		
174	95.0	0.0	184.4
176	91.1	0.0	179.0


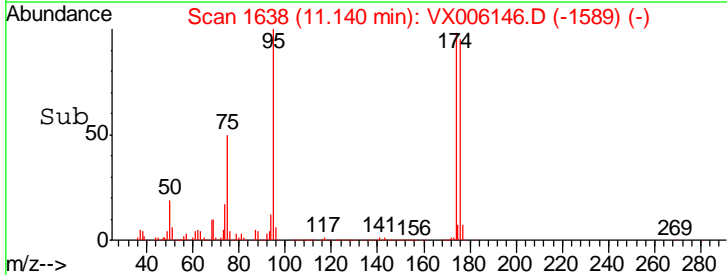
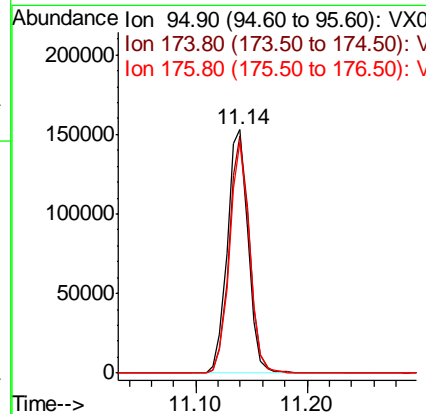
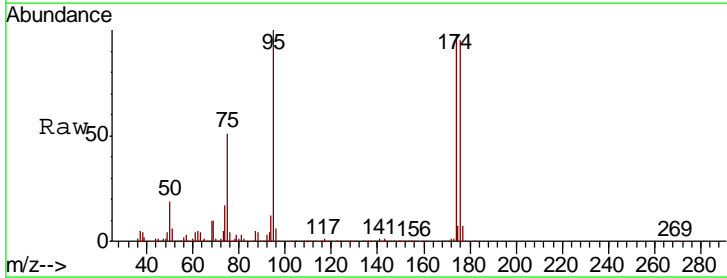


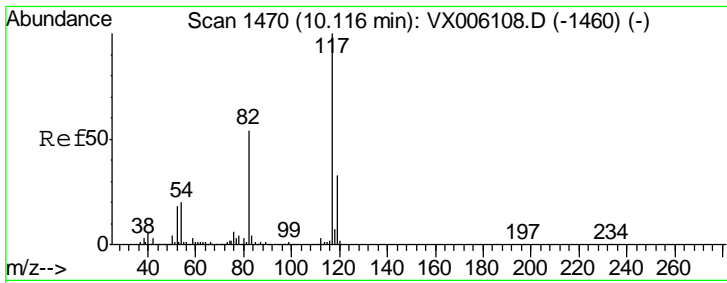

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.12 min Scan# 1470
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18




Instrument : MSVOA_X
 ClientSampled : EP2-FD-02


Tgt Ion	Resp	Lower	Upper
117	454733		
82	53.4	43.0	64.4
119	32.0	26.1	39.1

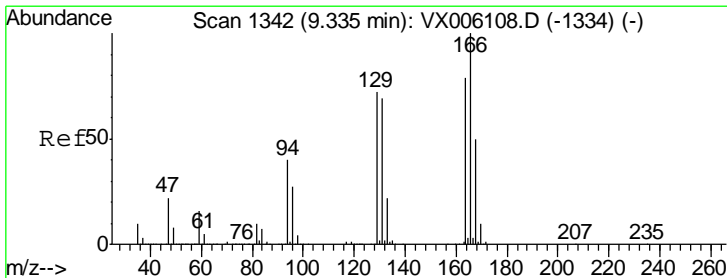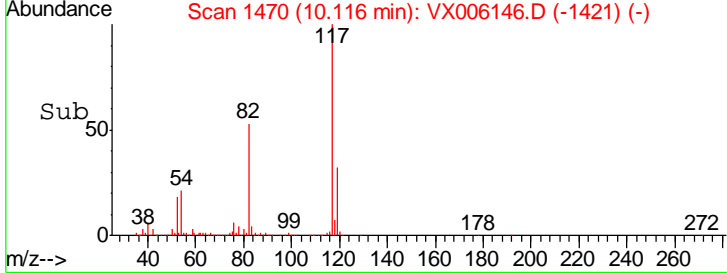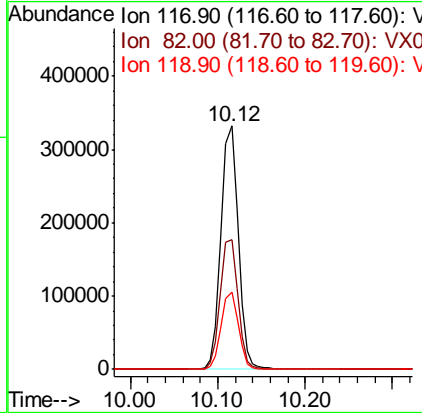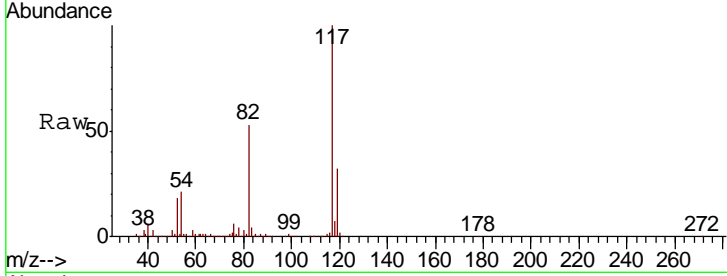

#64
 Tetrachloroethene
 Concen: 0.791 ug/l
 RT: 9.34 min Scan# 1342
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18

Tgt Ion	Resp	Lower	Upper
164	2961		
166	148.1	101.5	152.3
129	95.9	73.4	110.0
131	90.2	70.2	105.4

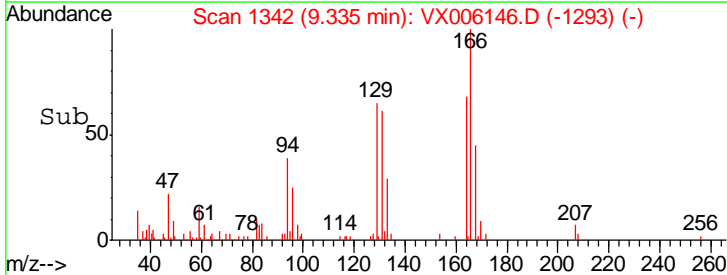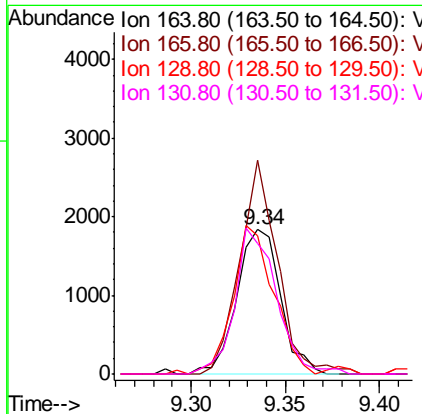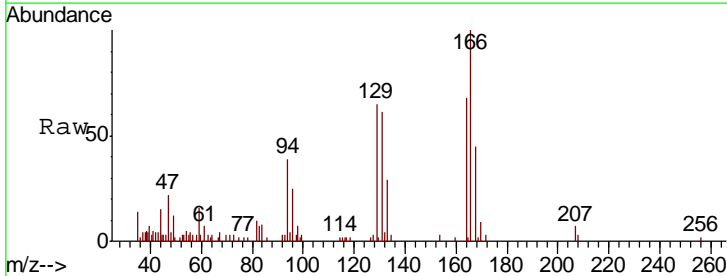

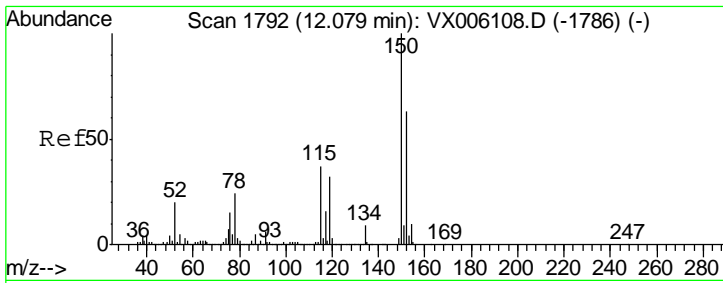

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. 0.00 min
 Lab File: VX006146.D
 Acq: 22 Nov 2018 02:18

Instrument :
 MSVOA_X
 ClientSampleId :
 EP2-FD-02

Tot Ion	Resp	Lower	Upper
152	100		
115	55.7	39.0	116.9
150	156.5	0.0	346.6

