


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX112119\
Data File : VX013491.D
Acq On : 21 Nov 2019 09:25
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X103119W.M
Title : SW846 8260
Last Update : Sat Nov 02 07:06:38 2019

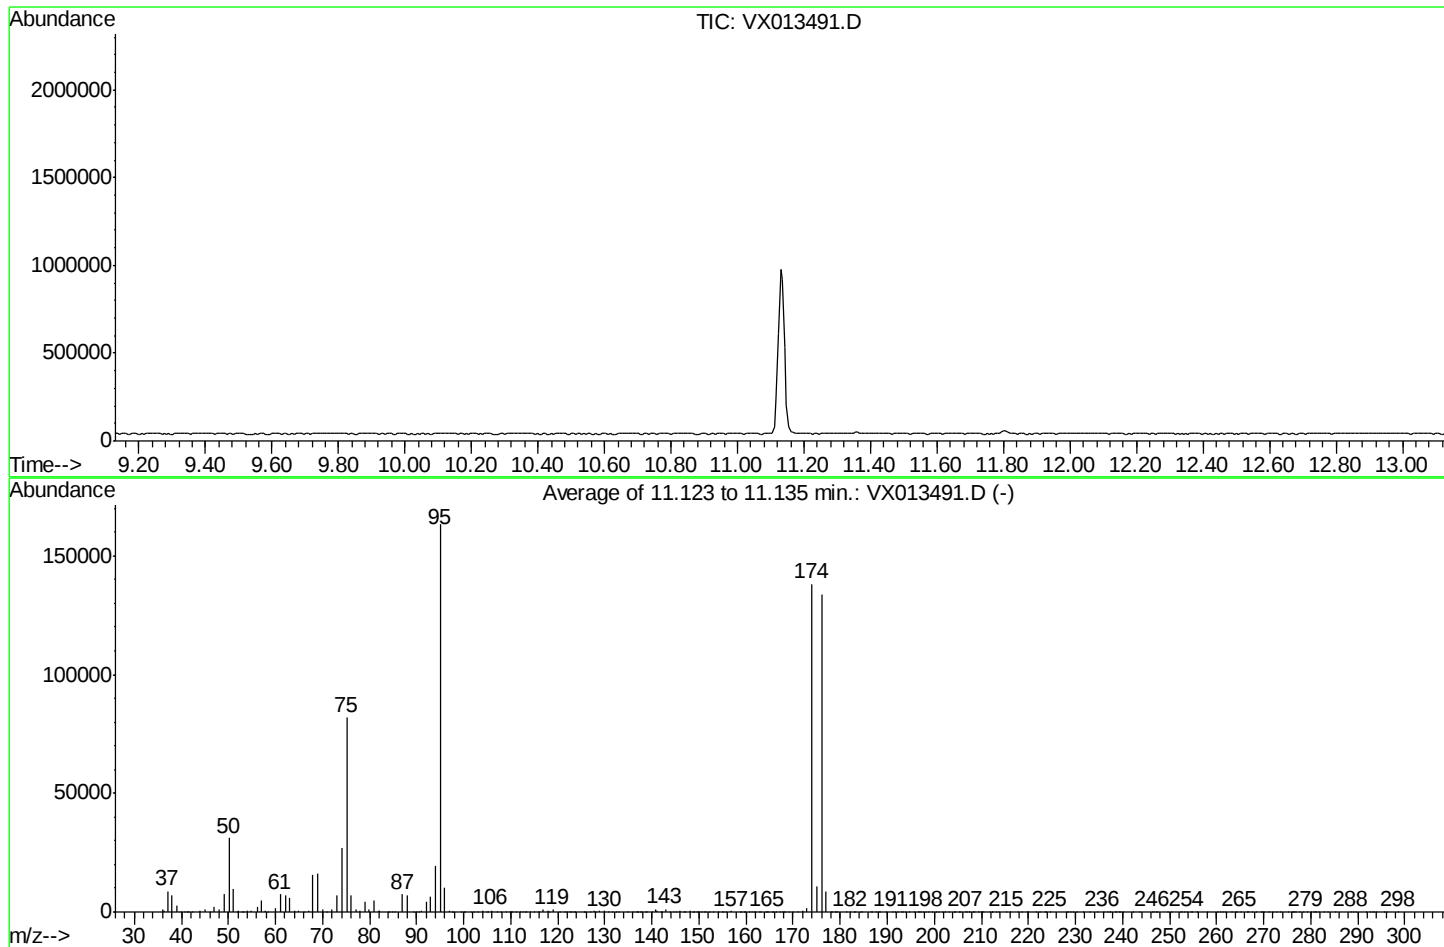

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	31112	PASS
75	95	30	60	50.1	81723	PASS
95	95	100	100	100.0	163270	PASS
96	95	5	9	6.4	10495	PASS
173	174	0.00	2	1.1	1536	PASS
174	95	50	100	84.7	138277	PASS
175	174	5	9	7.8	10782	PASS
176	174	95	101	96.7	133654	PASS
177	176	5	9	6.6	8861	PASS