

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112120\
 Data File : VX019530.D
 Acq On : 21 Nov 2020 06:17
 Operator : JC/MD
 Sample : L4778-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 358

Quant Time: Nov 21 07:47:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 21 01:57:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	327400	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	529964	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	454062	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	209262	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.03	65	195173	45.98	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	91.96%
35) Dibromofluoromethane	5.46	113	158733	47.72	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.44%
50) Toluene-d8	8.70	98	618598	47.85	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	95.70%
62) 4-Bromofluorobenzene	11.12	95	219283	47.15	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	94.30%

Target Compounds


					Qvalue	
3) Chloromethane	1.26	50	5830	1.596	ug/l #	41
5) Bromomethane	1.62	94	330	0.222	ug/l #	57
6) Chloroethane	1.65	64	847	Below Cal	#	48
11) Tert butyl alcohol	3.04	59	1486	1.850	ug/l #	83
13) Acrolein	2.29	56	364	0.674	ug/l #	15
16) Acetone	2.43	43	32067	19.534	ug/l	97
17) Carbon Disulfide	2.54	76	1899	0.217	ug/l #	88
18) Methyl Acetate	2.75	43	3391	1.466	ug/l	99
20) Methylene Chloride	2.83	84	18882	4.602	ug/l	96
25) 2-Butanone	4.65	43	5160	2.092	ug/l	98
29) Tetrahydrofuran	5.10	42	1951	1.240	ug/l #	89
31) Cyclohexane	5.62	56	6342	1.149	ug/l #	1
36) 1,1-Dichloropropene	5.62	75	24513	4.934	ug/l #	49
38) Carbon Tetrachloride	5.62	117	32153	6.686	ug/l #	16
43) Isopropyl Acetate	6.42	43	28727	3.664	ug/l	100
48) Methyl methacrylate	7.65	41	7607	2.072	ug/l #	9
49) 1,4-Dioxane	7.73	88	65	0.780	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	94339	20.633	ug/l #	47
54) cis-1,3-Dichloropropene	8.60	75	50856	8.502	ug/l #	57
57) 1,3-Dichloropropane	9.52	76	15535	2.440	ug/l #	44
59) 2-Hexanone	9.52	43	180849	52.153	ug/l #	47
60) Dibromochloromethane	9.32	129	1280	0.344	ug/l #	10
64) Tetrachloroethene	9.32	164	1247	0.349	ug/l	91
70) Styrene	10.70	104	218	1.665	ug/l #	39
76) 1,2,3-Trichloropropane	11.12	75	107555	23.551	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	107555	62.458	ug/l #	12
95) Naphthalene	13.82	128	1239	2.255	ug/l #	75

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112120\
Data File : VX019530.D
Acq On : 21 Nov 2020 06:17
Operator : JC/MD
Sample : L4778-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
358

Quant Time: Nov 21 07:47:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 21 01:57:45 2020
Response via : Initial Calibration

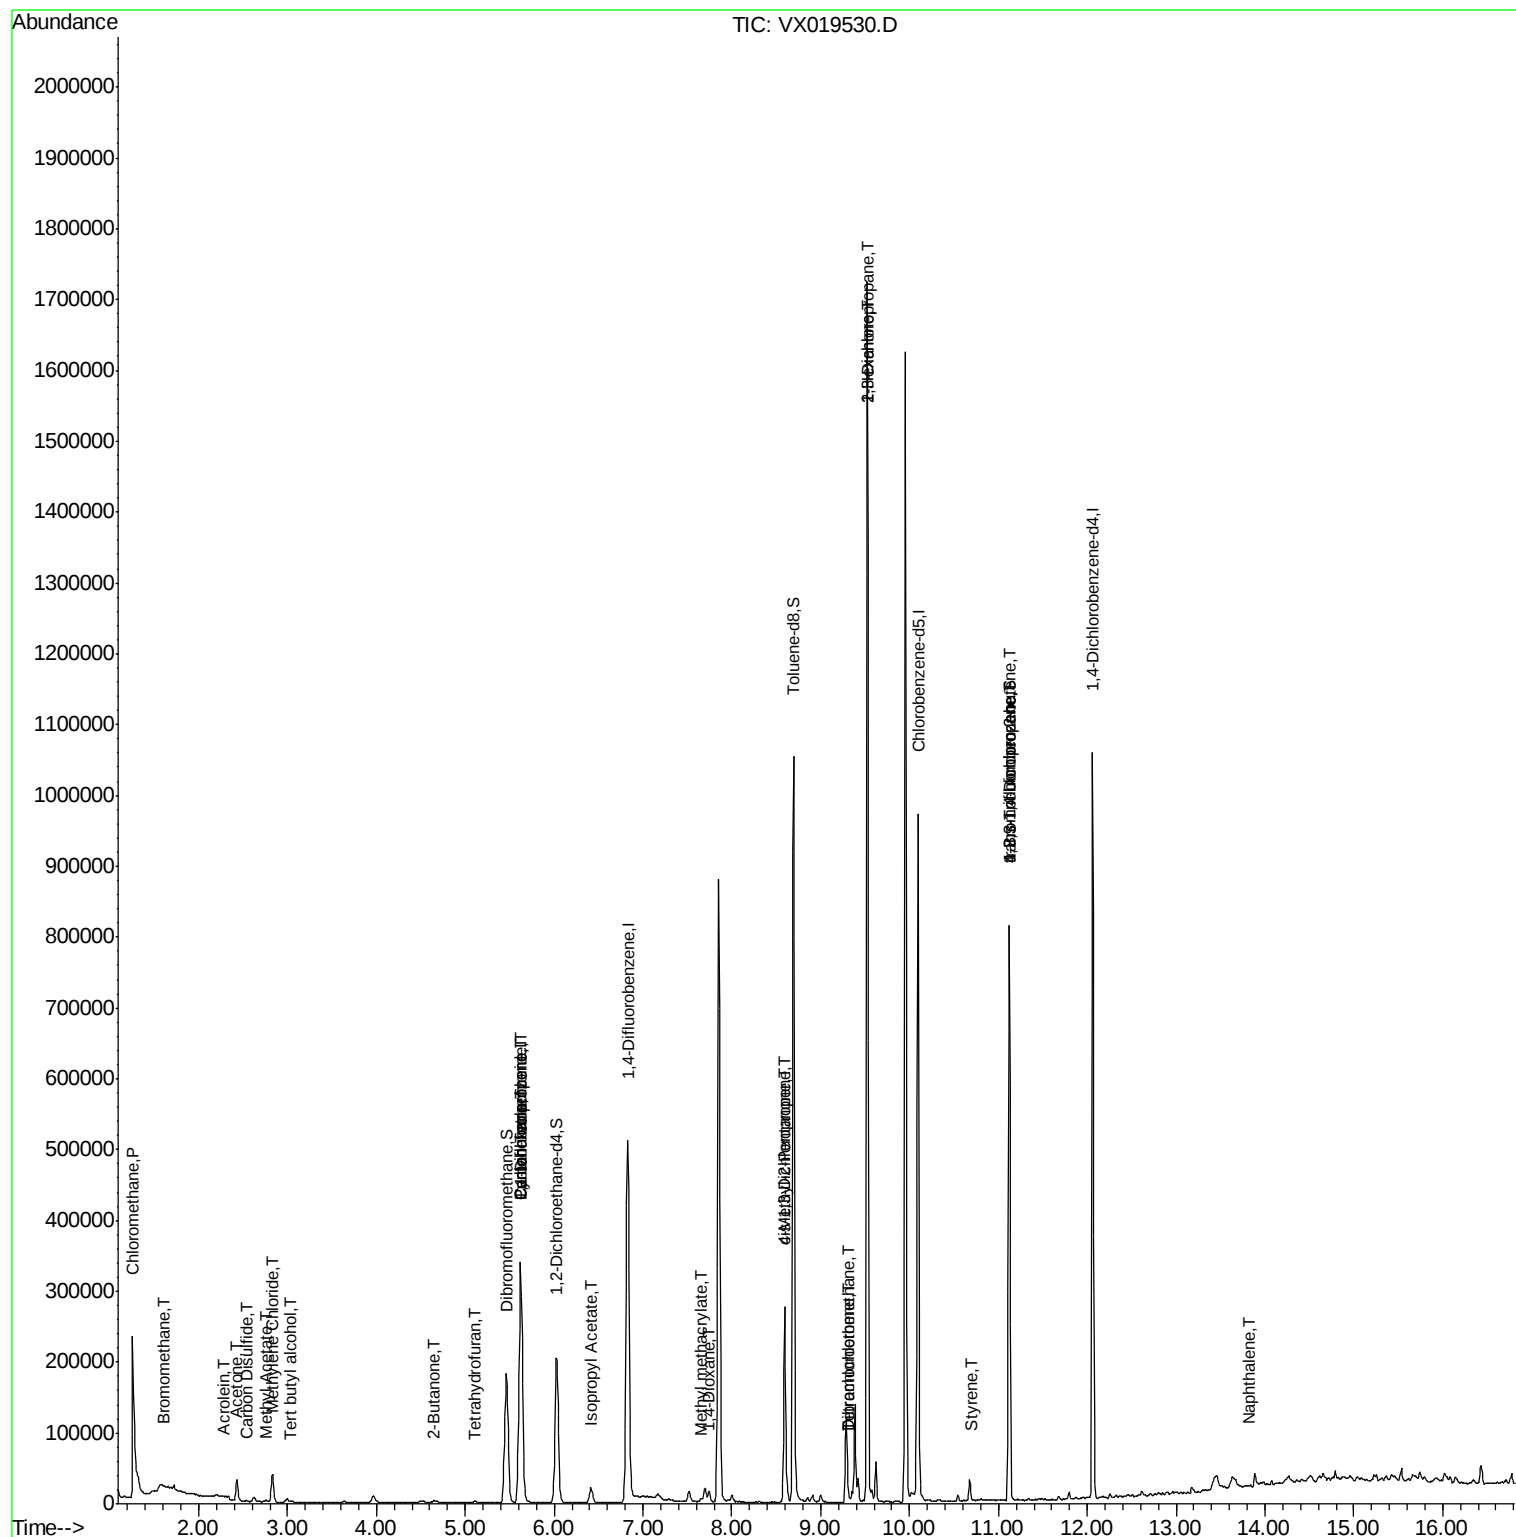



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampled :


358

Tot Ion:168 Resp: 327400

Ion Ratio Lower Upper




168 100

99 56.4 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

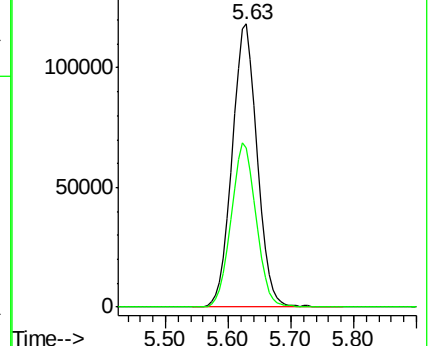

#3

Chloromethane

Concen: 1.596 ug/l

RT: 1.26 min Scan# 28

Delta R.T. -0.06 min

Lab File: VX019530.D


Acq: 21 Nov 2020 06:17

Tgt Ion: 50 Resp: 5830

Ion Ratio Lower Upper



50 100


52 0.0 27.0 40.6#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

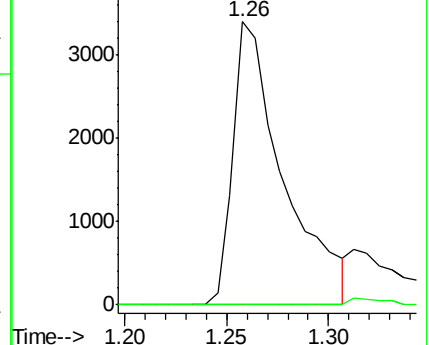



#5

Bromomethane

Concen: 0.222 ug/l

RT: 1.62 min Scan# 87

Delta R.T. -0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :


358

Tot Ion: 94 Resp: 330

Ion Ratio Lower Upper




94 100

96 53.3 75.6 113.4#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

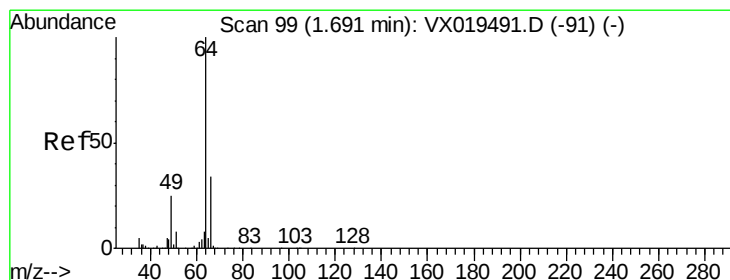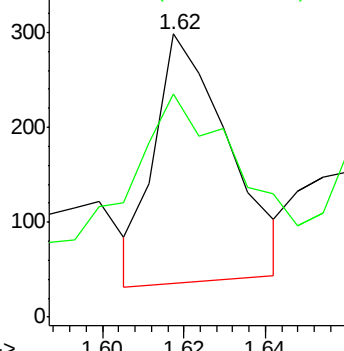

#6

Chloroethane

Concen: Below Cal

RT: 1.65 min Scan# 93

Delta R.T. -0.04 min

Lab File: VX019530.D


Acq: 21 Nov 2020 06:17

Tgt Ion: 64 Resp: 847

Ion Ratio Lower Upper



64 100


66 4.1 27.1 40.7#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

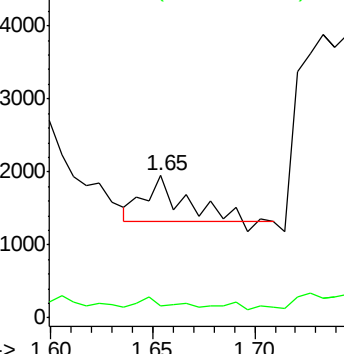




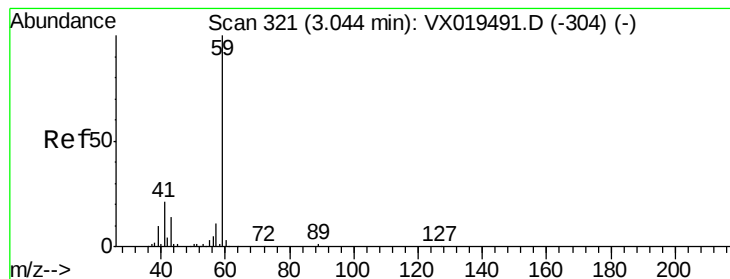


#11

Tert butyl alcohol
 Concen: 1.850 ug/l
 RT: 3.04 min Scan# 321
 Delta R.T. -0.00 min
 Lab File: VX019530.D
 Acq: 21 Nov 2020 06:17

Instrument :
 MSVOA_X
 ClientSampled :
 358




Tot Ion: 59 Resp: 1486
 Ion Ratio Lower Upper
 59 100
 57 16.1 7.9 11.9#

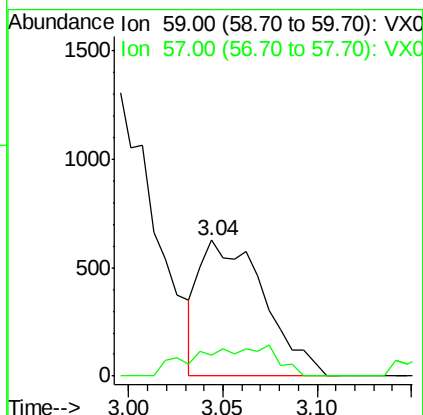


#13

Acrolein
 Concen: 0.674 ug/l
 RT: 2.29 min Scan# 197
 Delta R.T. 0.01 min
 Lab File: VX019530.D
 Acq: 21 Nov 2020 06:17

Tgt Ion: 56 Resp: 364
 Ion Ratio Lower Upper
 56 100
 55 0.0 55.5 83.3#

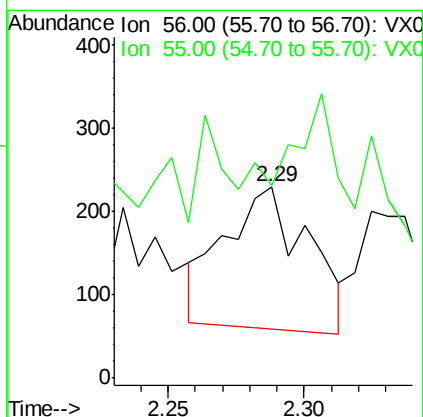

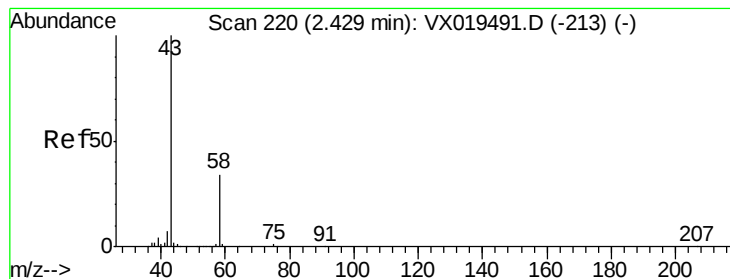

#16

Acetone

Concen: 19.534 ug/l

RT: 2.43 min Scan# 220

Delta R.T. -0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampled :





358

Tot Ion: 43 Resp: 32067

Ion Ratio Lower Upper

43 100

58 35.8 27.4 41.2

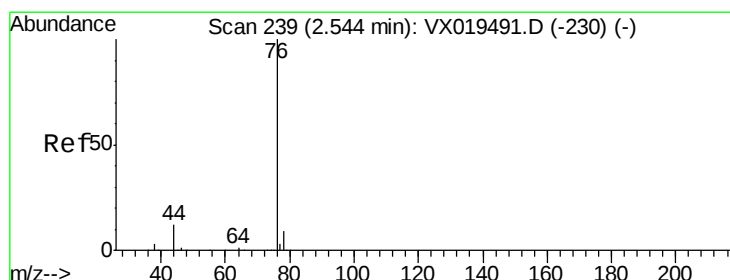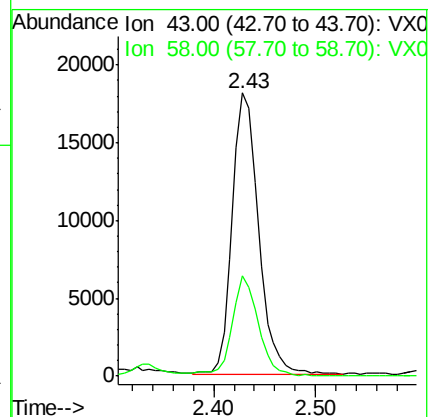

#17

Carbon Disulfide

Concen: 0.217 ug/l

RT: 2.54 min Scan# 238

Delta R.T. -0.01 min

Lab File: VX019530.D




Acq: 21 Nov 2020 06:17


Tgt Ion: 76 Resp: 1899

Ion Ratio Lower Upper

76 100

78 13.4 7.2 10.8#



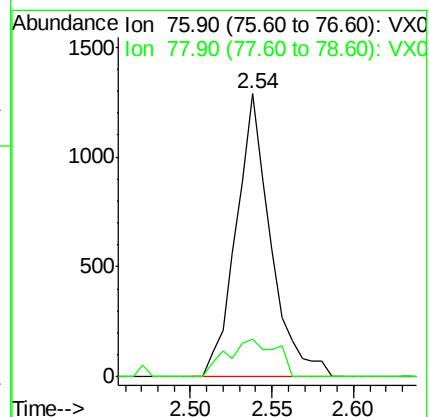





#18
Methvl Acetate
Concen: 1.466 ug/l
RT: 2.75 min Scan# 273
Delta R.T. 0.00 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17




Instrument :
MSVOA_X
ClientSampleId :
358


Tot Ion: 43 Resp: 3391
Ion Ratio Lower Upper
43 100
74 27.3 22.2 33.4

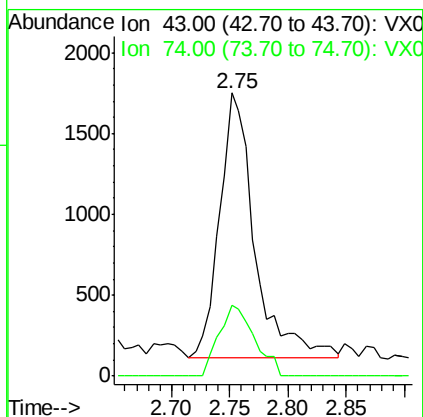

#20
Methylene Chloride
Concen: 4.602 ug/l
RT: 2.83 min Scan# 286
Delta R.T. -0.00 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17

Tgt Ion: 84 Resp: 18882
Ion Ratio Lower Upper
84 100
49 104.6 88.5 132.7
51 34.3 28.0 42.0
86 67.6 53.0 79.4

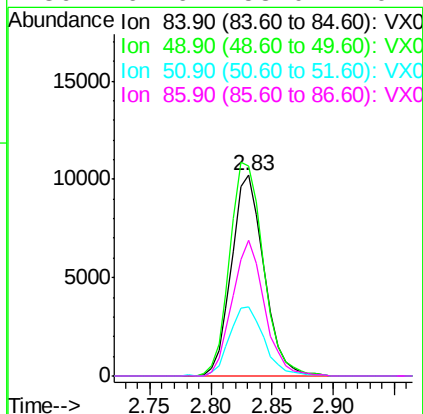



#25

2-Butanone

Concen: 2.092 ug/l

RT: 4.65 min Scan# 584

Delta R.T. 0.01 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :





358

Tot Ion: 43 Resp: 5160

Ion Ratio Lower Upper

43 100

72 30.8 24.0 36.0

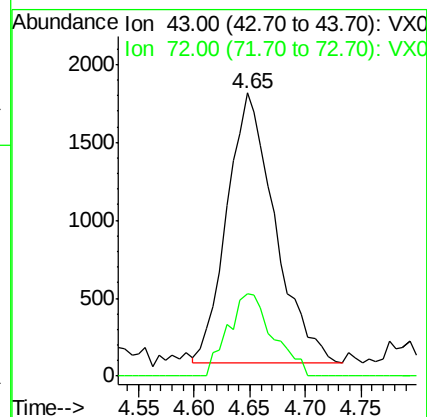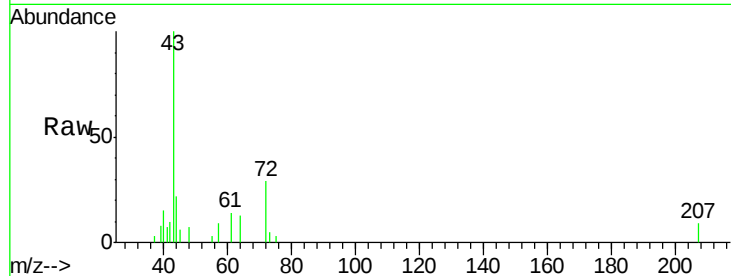

#29

Tetrahydrofuran

Concen: 1.240 ug/l

RT: 5.10 min Scan# 658

Delta R.T. 0.01 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17




Tgt Ion: 42 Resp: 1951


Ion Ratio Lower Upper

42 100

72 40.9 42.6 63.8#

71 45.4 39.0 58.6

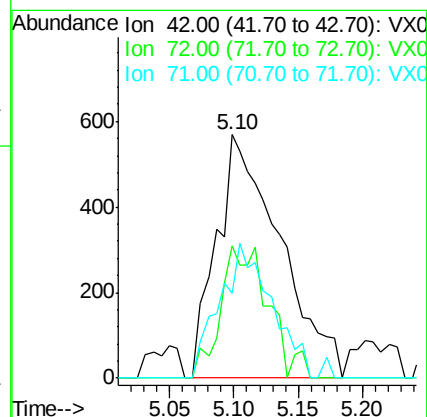







#31
Cyclohexane
Concen: 1.149 ug/l
RT: 5.62 min Scan# 744
Delta R.T. 0.09 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17

Instrument :
MSVOA_X
ClientSampled :
358

Tot Ion: 56 Resp: 6342
Ion Ratio Lower Upper
56 100
69 172.6 25.5 38.3#
84 136.9 71.1 106.7#

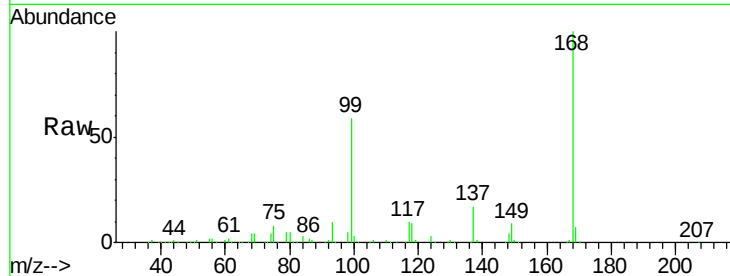


Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0


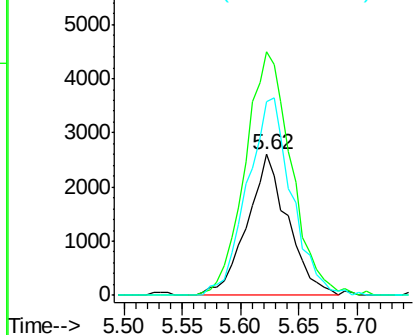



#33
1,2-Dichloroethane-d4
Concen: 45.977 ug/l
RT: 6.03 min Scan# 810
Delta R.T. -0.01 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17

Tgt Ion: 65 Resp: 195173
Ion Ratio Lower Upper
65 100
67 53.0 0.0 105.0

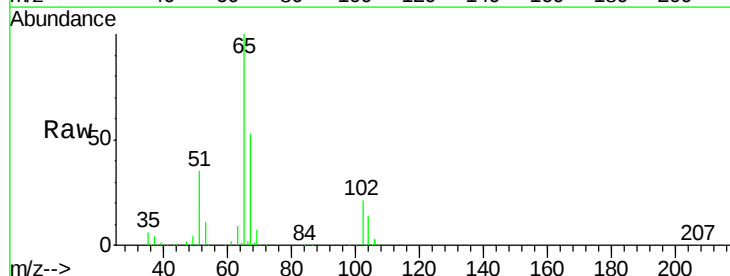

Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0

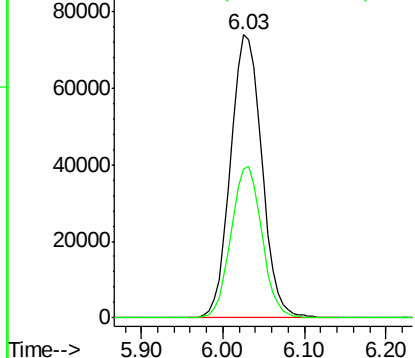



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :

358


Tot Ion:114 Resp: 529964

Ion Ratio Lower Upper

114 100

63 19.3 0.0 38.8




88 16.2 0.0 31.6



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

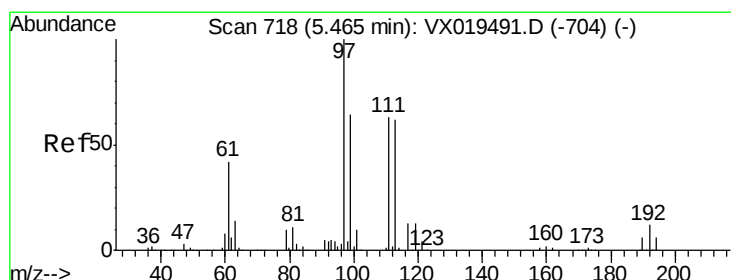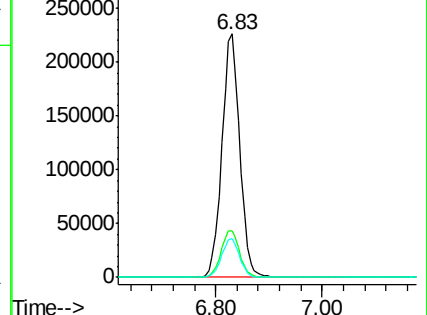

#35

Dibromofluoromethane

Concen: 47.717 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17


Tgt Ion:113 Resp: 158733

Ion Ratio Lower Upper

113 100

111 103.0 81.5 122.3



192 20.0 16.2 24.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

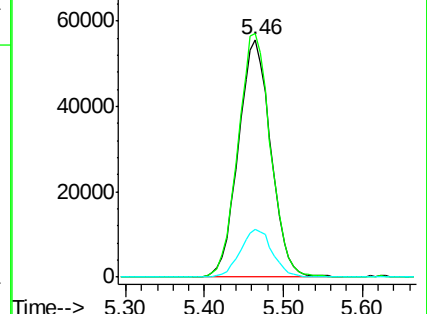



#36

1,1-Dichloropropene

Concen: 4.934 ug/l

RT: 5.62 min Scan# 744





Delta R.T. -0.14 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :
MSVOA_X
ClientSampled :
358

Tot Ion:	75	Resp:	24513
Ion	Ratio	Lower	Upper
75	100		
110	8.9	18.1	54.3#
77	0.0	24.2	36.4#

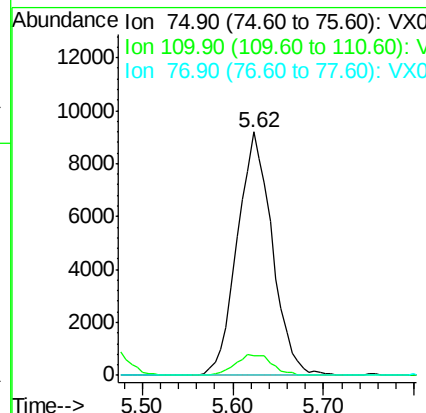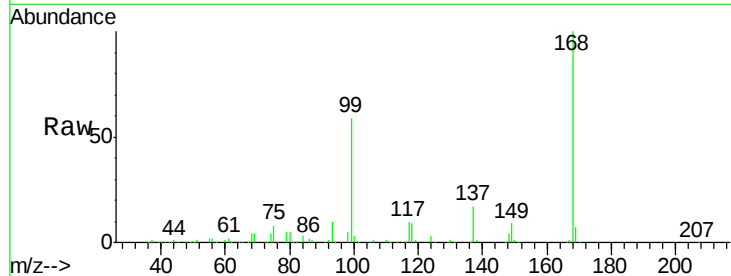

#38

Carbon Tetrachloride

Concen: 6.686 ug/l




RT: 5.62 min Scan# 744


Delta R.T. -0.13 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Tgt Ion:	117	Resp:	32153
Ion	Ratio	Lower	Upper
117	100		
119	5.2	75.9	113.9#
121	0.0	24.0	36.0#

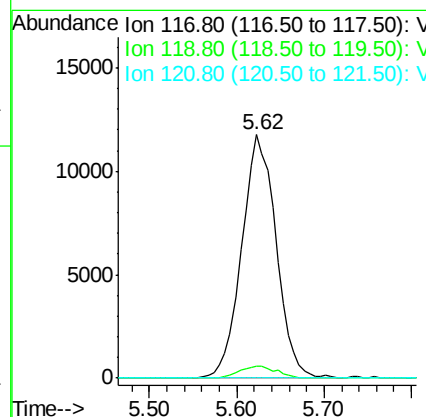



#43

Isopropyl Acetate

Concen: 3.664 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampled :

358


Tot Ion: 43 Resp: 28727

Ion Ratio Lower Upper

43 100

61 22.5 18.2 27.2




87 15.5 12.6 18.8

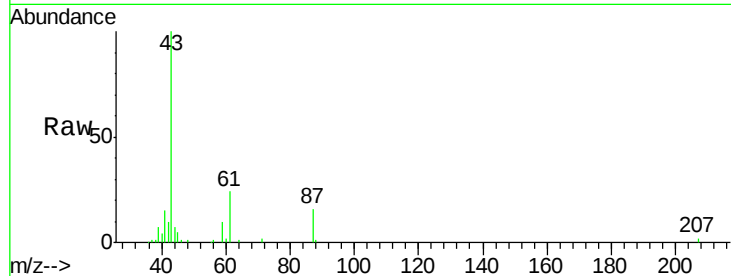

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

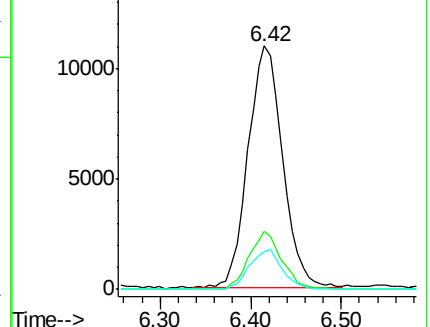

#48

Methyl methacrylate

Concen: 2.072 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.09 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17


Tgt Ion: 41 Resp: 7607

Ion Ratio Lower Upper

41 100

69 0.0 77.0 115.6#



39 0.0 45.6 68.4#




Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

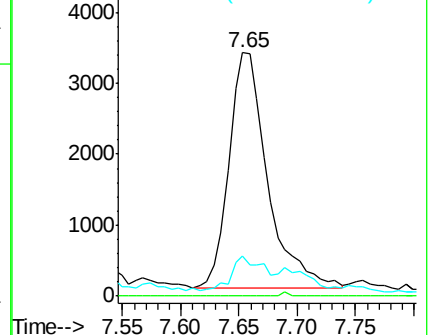



#49

1,4-Dioxane

Concen: 0.780 ug/l

RT: 7.73 min Scan# 1090

Delta R.T. 0.01 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :

358


Tot Ion: 88 Resp: 65

Ion Ratio Lower Upper

88 100

43 0.0 23.8 35.6#




58 689.2 54.2 81.2#

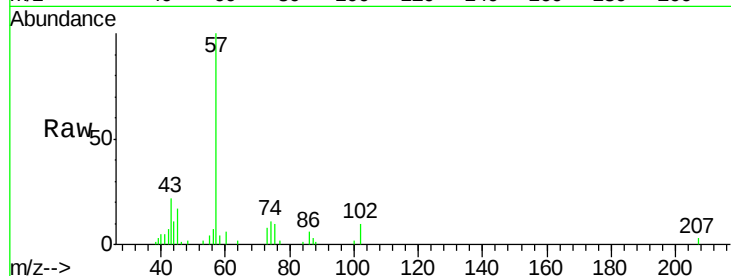

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

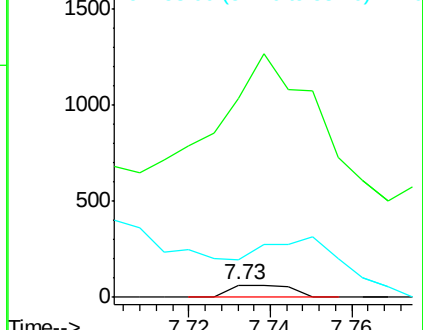

#50

Toluene-d8

Concen: 47.854 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX019530.D


Acq: 21 Nov 2020 06:17

Tgt Ion: 98 Resp: 618598

Ion Ratio Lower Upper



98 100


100 66.3 52.4 78.6



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

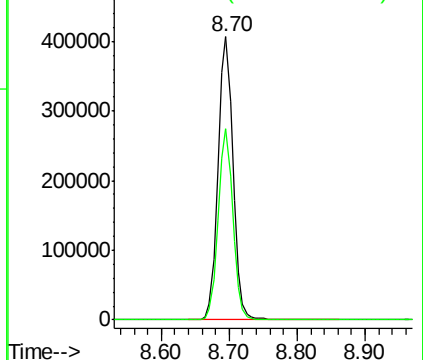



#51

4-Methyl-2-Pentanone

Concen: 20.633 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :





358

Tot Ion: 43 Resp: 94339

Ion Ratio Lower Upper

43 100

58 9.9 35.1 52.7#

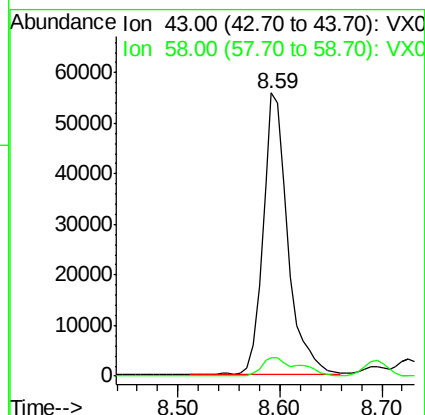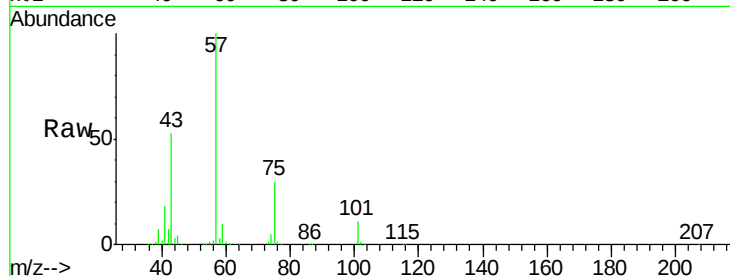

#54

cis-1,3-Dichloropropene

Concen: 8.502 ug/l

RT: 8.60 min Scan# 1232

Delta R.T. 0.18 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17




Tgt Ion: 75 Resp: 50856


Ion Ratio Lower Upper

75 100

77 0.7 25.8 38.6#

39 22.4 34.6 51.8#

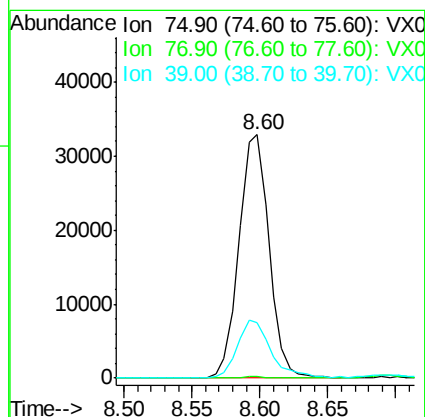



#57

1,3-Dichloropropane

Concen: 2.440 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :





358

Tot Ion: 76 Resp: 15535

Ion Ratio Lower Upper

76 100

78 0.7 25.7 38.5#

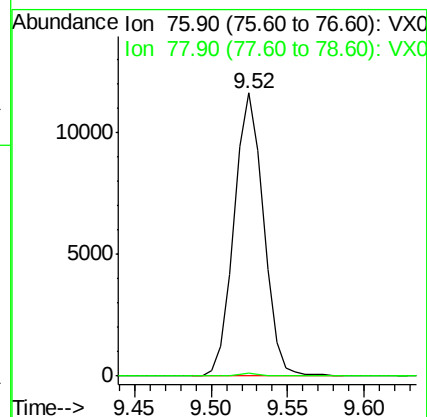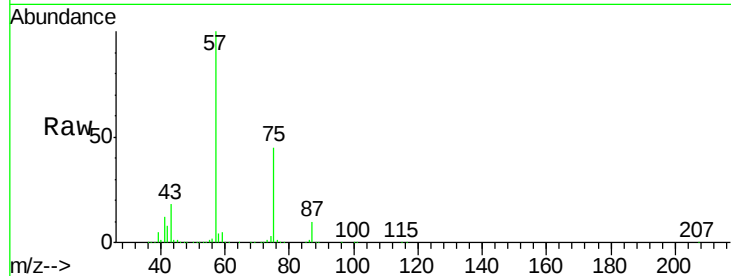

#59

2-Hexanone

Concen: 52.153 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.05 min

Lab File: VX019530.D




Acq: 21 Nov 2020 06:17


Tgt Ion: 43 Resp: 180849

Ion Ratio Lower Upper

43 100

58 20.8 30.6 91.6#

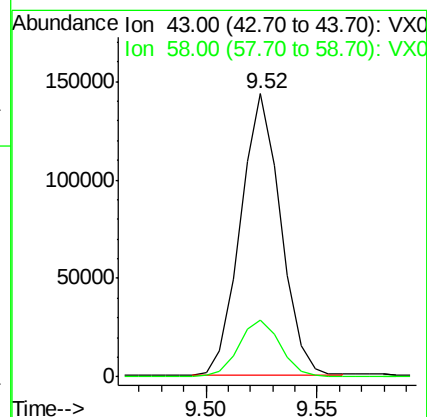



#60

Dibromochloromethane

Concen: 0.344 ug/l

RT: 9.32 min Scan# 1350

Delta R.T. -0.25 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :


358

Tot Ion:129 Resp: 1280

Ion Ratio Lower Upper

129 100

127 0.0 39.0 116.9#

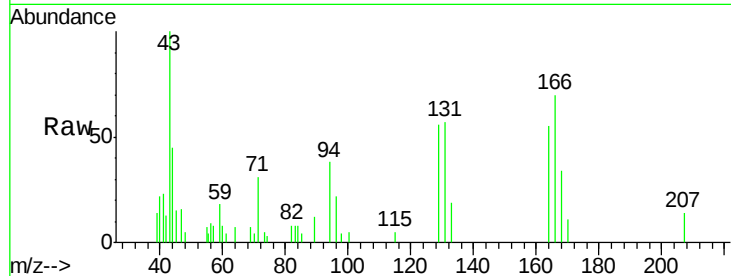

Abundance Ion 128.80 (128.50 to 129.50): V

Ion 126.80 (126.50 to 127.50): V

9.32

800

600



400

200

0

9.30 9.35

Time-->



#62

4-Bromofluorobenzene

Concen: 47.149 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17


Tgt Ion: 95 Resp: 219283

Ion Ratio Lower Upper

95 100

174 77.9 0.0 156.2

176 75.1 0.0 151.4



Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

200000

150000


100000


50000

0

11.00 11.10 11.20

Time-->




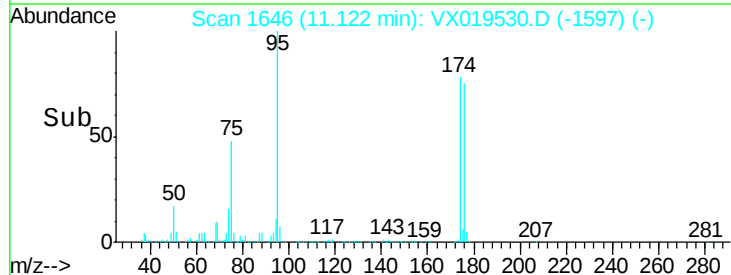




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17




Instrument :
MSVOA_X
ClientSampled :
358


Tot Ion:117 Resp: 454062
Ion Ratio Lower Upper
117 100
82 54.4 43.0 64.4
119 30.7 25.6 38.4

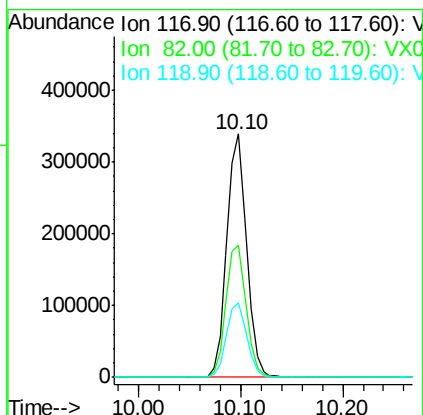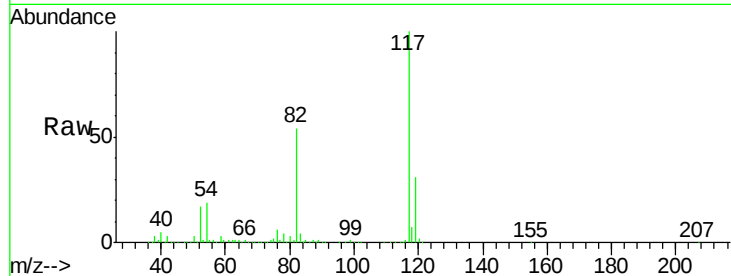

#64
Tetrachloroethene
Concen: 0.349 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.00 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17

Tgt Ion:164 Resp: 1247
Ion Ratio Lower Upper
164 100
166 125.8 107.4 161.0
129 101.1 76.6 114.8
131 103.8 72.6 108.8



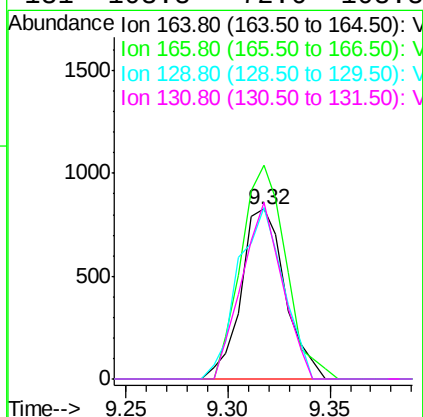





#70
Stvrene
Concen: 1.665 ug/l
RT: 10.70 min Scan# 1576
Delta R.T. 0.00 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17




Instrument :
MSVOA_X
ClientSampled :
358


Tot Ion:104 Resp: 218
Ion Ratio Lower Upper
104 100
78 10.1 39.5 59.3#
103 8.7 43.6 65.4#

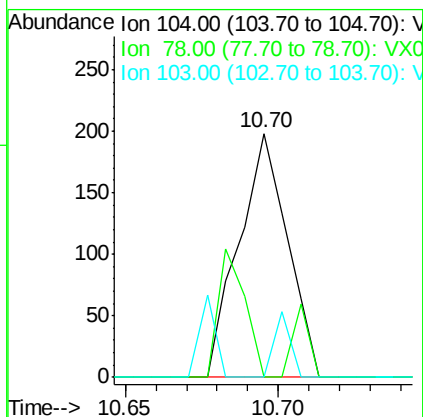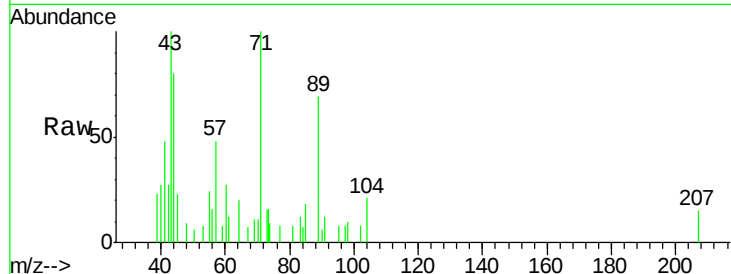

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX019530.D
Acq: 21 Nov 2020 06:17

Tgt Ion:152 Resp: 209262
Ion Ratio Lower Upper
152 100
115 60.4 41.8 125.4
150 157.5 0.0 348.2

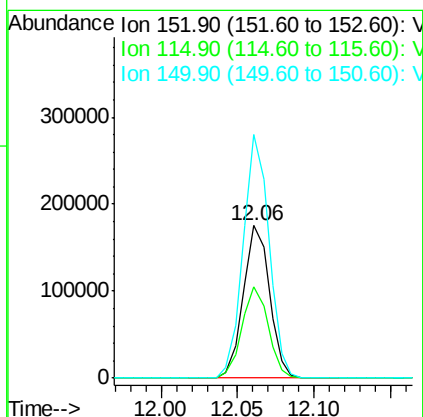

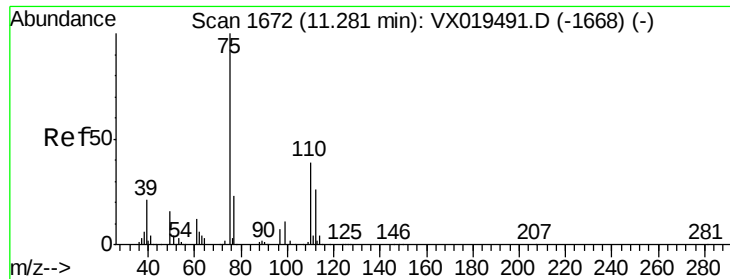

#76

1,2,3-Trichloropropane

Concen: 23.551 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :





358

Tot Ion: 75 Resp: 107555

Ion Ratio Lower Upper

75 100

77 1.3 20.0 60.0#

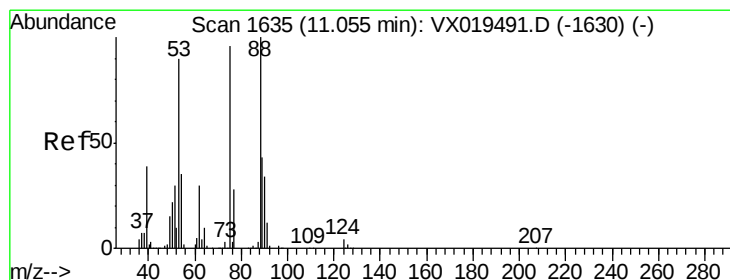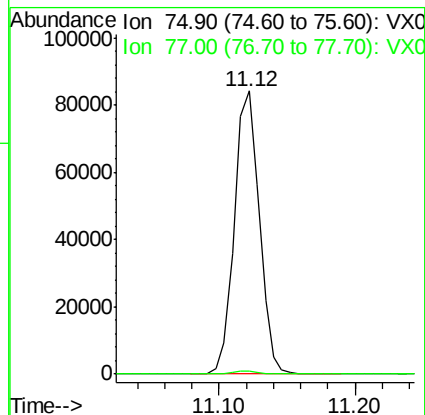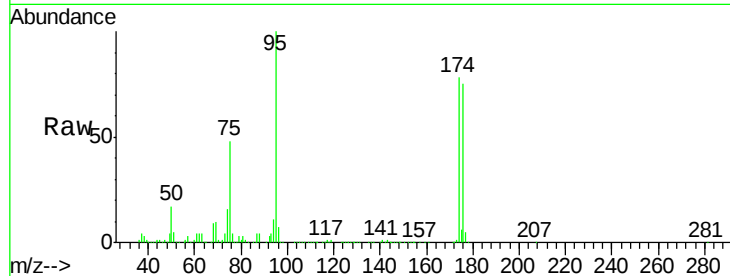

#81

trans-1,4-Dichloro-2-butene

Concen: 62.458 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17




Tgt Ion: 75 Resp: 107555


Ion Ratio Lower Upper

75 100

53 0.2 73.9 110.9#

89 0.0 37.3 55.9#

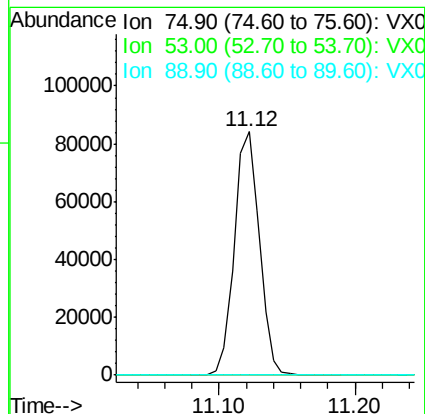

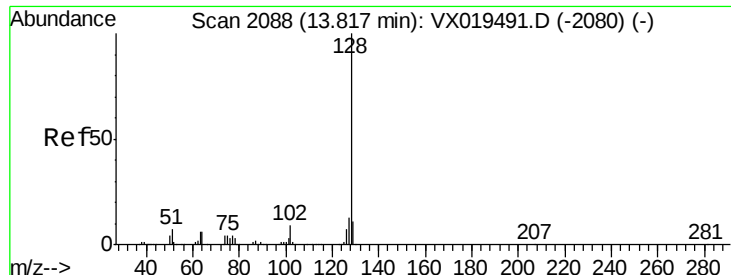

#95

Naphthalene

Concen: 2.255 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. 0.00 min

Lab File: VX019530.D

Acq: 21 Nov 2020 06:17

Instrument :

MSVOA_X

ClientSampleId :

358


Tot Ion:128 Resp: 1239

Ion Ratio Lower Upper

128 100

127 30.0 10.3 15.5#

129 12.4 8.7 13.1



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

