

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112120\
 Data File : VX019527.D
 Acq On : 21 Nov 2020 05:07
 Operator : JC/MD
 Sample : L4788-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW181S-GW-20201117

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	46	rBV	296346	656009	38.92%	2.917%
2	2.343	202	206	216	rVB2	19300	45253	2.69%	0.201%
3	2.624	245	252	265	rVB	13804	32149	1.91%	0.143%
4	3.666	416	423	430	rVB2	7496	17225	1.02%	0.077%
5	4.562	556	570	581	rBV	12306	38367	2.28%	0.171%
6	5.465	706	718	732	rBV	191597	551467	32.72%	2.452%
7	5.623	732	744	760	rBV	356214	996423	59.12%	4.430%
8	6.025	797	810	827	rBV	212613	562871	33.40%	2.503%
9	6.830	930	942	953	rBV	538438	1323950	78.56%	5.887%
10	7.184	994	1000	1010	rVB3	29124	68049	4.04%	0.303%
11	7.287	1010	1017	1035	rBV	56368	143701	8.53%	0.639%
12	8.696	1240	1248	1261	rBV	1066343	1685319	100.00%	7.493%
13	9.318	1344	1350	1359	rVB	13637	20028	1.19%	0.089%
14	10.025	1460	1466	1472	rBV3	25461	75301	4.47%	0.335%
15	10.098	1472	1478	1494	rVB	999902	1422466	84.40%	6.325%
16	11.031	1623	1631	1641	rBV	293274	519719	30.84%	2.311%
17	11.122	1641	1646	1657	rVB	904881	1140879	67.70%	5.073%
18	11.512	1707	1710	1715	rVB	24723	28894	1.71%	0.128%
19	11.787	1752	1755	1760	rBV2	11730	16977	1.01%	0.075%
20	12.012	1789	1792	1795	rVV	21044	23623	1.40%	0.105%
21	12.061	1795	1800	1806	rVV	1166808	1428391	84.75%	6.351%
22	12.140	1810	1813	1816	rVB3	16182	19676	1.17%	0.087%
23	12.207	1822	1824	1828	rVB	16732	18903	1.12%	0.084%
24	12.354	1844	1848	1854	rVB3	23074	41646	2.47%	0.185%
25	12.457	1854	1865	1870	rBV	172361	225940	13.41%	1.005%
26	12.506	1870	1873	1879	rVB4	14011	26301	1.56%	0.117%
27	12.573	1879	1884	1885	rBV3	17282	24193	1.44%	0.108%
28	12.616	1885	1891	1895	rBV2	97380	125374	7.44%	0.557%
29	12.719	1904	1908	1911	rBV	25127	30818	1.83%	0.137%
30	12.768	1911	1916	1920	rVB4	16946	24727	1.47%	0.110%
31	12.860	1924	1931	1935	rBV4	37127	56877	3.37%	0.253%
32	12.933	1937	1943	1944	rBV4	51638	81250	4.82%	0.361%
33	12.981	1949	1951	1953	rVV	27873	33082	1.96%	0.147%
34	13.012	1953	1956	1960	rVB3	71042	92621	5.50%	0.412%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112120\
 Data File : VX019527.D
 Acq On : 21 Nov 2020 05:07
 Operator : JC/MD
 Sample : L4788-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-MW181S-GW-20201117

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Title : SW846 8260

35	13.079	1961	1967	1970	rBV3	75915	98208	5.83%	0.437%
36	13.195	1980	1986	1991	rBV4	45868	84667	5.02%	0.376%
37	13.250	1991	1995	1998	rBV2	44274	51415	3.05%	0.229%
38	13.305	1998	2004	2007	rBV	475791	563906	33.46%	2.507%
39	13.335	2007	2009	2013	rVV3	119915	140124	8.31%	0.623%
40	13.384	2013	2017	2019	rVV3	32117	42670	2.53%	0.190%
41	13.420	2019	2023	2026	rVV2	99949	133349	7.91%	0.593%
42	13.457	2026	2029	2038	rVB5	102585	256866	15.24%	1.142%
43	13.542	2038	2043	2046	rBV5	46826	79300	4.71%	0.353%
44	13.585	2047	2050	2052	rBV3	23624	29565	1.75%	0.131%
45	13.622	2052	2056	2061	rBV4	46737	95392	5.66%	0.424%
46	13.719	2067	2072	2073	rBV3	86422	114410	6.79%	0.509%
47	13.774	2078	2081	2084	rVV2	105770	132699	7.87%	0.590%
48	13.805	2084	2086	2089	rVV2	67401	63174	3.75%	0.281%
49	13.835	2089	2091	2094	rVV2	38645	39125	2.32%	0.174%
50	13.878	2094	2098	2106	rVB5	189777	387563	23.00%	1.723%
51	13.981	2106	2115	2118	rVB5	86247	224415	13.32%	0.998%
52	14.042	2118	2125	2126	rBV5	58244	99389	5.90%	0.442%
53	14.073	2126	2130	2134	rVB	657953	747462	44.35%	3.323%
54	14.115	2134	2137	2139	rBV3	71037	90570	5.37%	0.403%
55	14.201	2149	2151	2153	rBV	40798	45767	2.72%	0.203%
56	14.225	2153	2155	2157	rVV2	63967	70744	4.20%	0.315%
57	14.262	2157	2161	2166	rVB3	161293	289834	17.20%	1.289%
58	14.359	2175	2177	2182	rVB3	48632	62299	3.70%	0.277%
59	14.414	2182	2186	2188	rBV	89125	104888	6.22%	0.466%
60	14.451	2189	2192	2194	rVV2	87182	126203	7.49%	0.561%
61	14.512	2198	2202	2204	rVV3	167799	241979	14.36%	1.076%
62	14.536	2204	2206	2212	rVV3	208716	302243	17.93%	1.344%
63	14.603	2212	2217	2222	rVV4	153507	278506	16.53%	1.238%
64	14.652	2222	2225	2228	rVV2	426604	553988	32.87%	2.463%
65	14.713	2232	2235	2239	rVB2	109918	161018	9.55%	0.716%
66	14.792	2244	2248	2251	rVV	1058126	1073272	63.68%	4.772%
67	14.829	2251	2254	2257	rVB4	103338	123026	7.30%	0.547%
68	14.884	2261	2263	2266	rVB2	120785	127504	7.57%	0.567%
69	14.951	2271	2274	2276	rBV3	77909	111423	6.61%	0.495%
70	15.146	2301	2306	2309	rBV4	134710	264502	15.69%	1.176%
71	15.225	2315	2319	2321	rBV2	187716	263033	15.61%	1.170%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX112120\
Data File : VX019527.D
Acq On : 21 Nov 2020 05:07
Operator : JC/MD
Sample : L4788-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW181S-GW-20201117

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Title : SW846 8260

72	15.255	2321	2324	2327	rVV	387376	457356	27.14%	2.034%
73	15.323	2331	2335	2338	rVB2	185018	229000	13.59%	1.018%
74	15.420	2347	2351	2355	rBV4	136929	223957	13.29%	0.996%
75	15.536	2365	2370	2376	rBV	935806	1320635	78.36%	5.872%
76	15.664	2388	2391	2395	rBV4	107200	139645	8.29%	0.621%
77	16.146	2465	2470	2476	rBV6	153368	371424	22.04%	1.651%
78	16.432	2513	2517	2523	rVB	282596	475446	28.21%	2.114%


Sum of corrected areas: 22490430

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX112120\
Data File : VX019527.D
Acq On : 21 Nov 2020 05:07
Operator : JC/MD
Sample : L4788-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW181S-GW-20201117

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

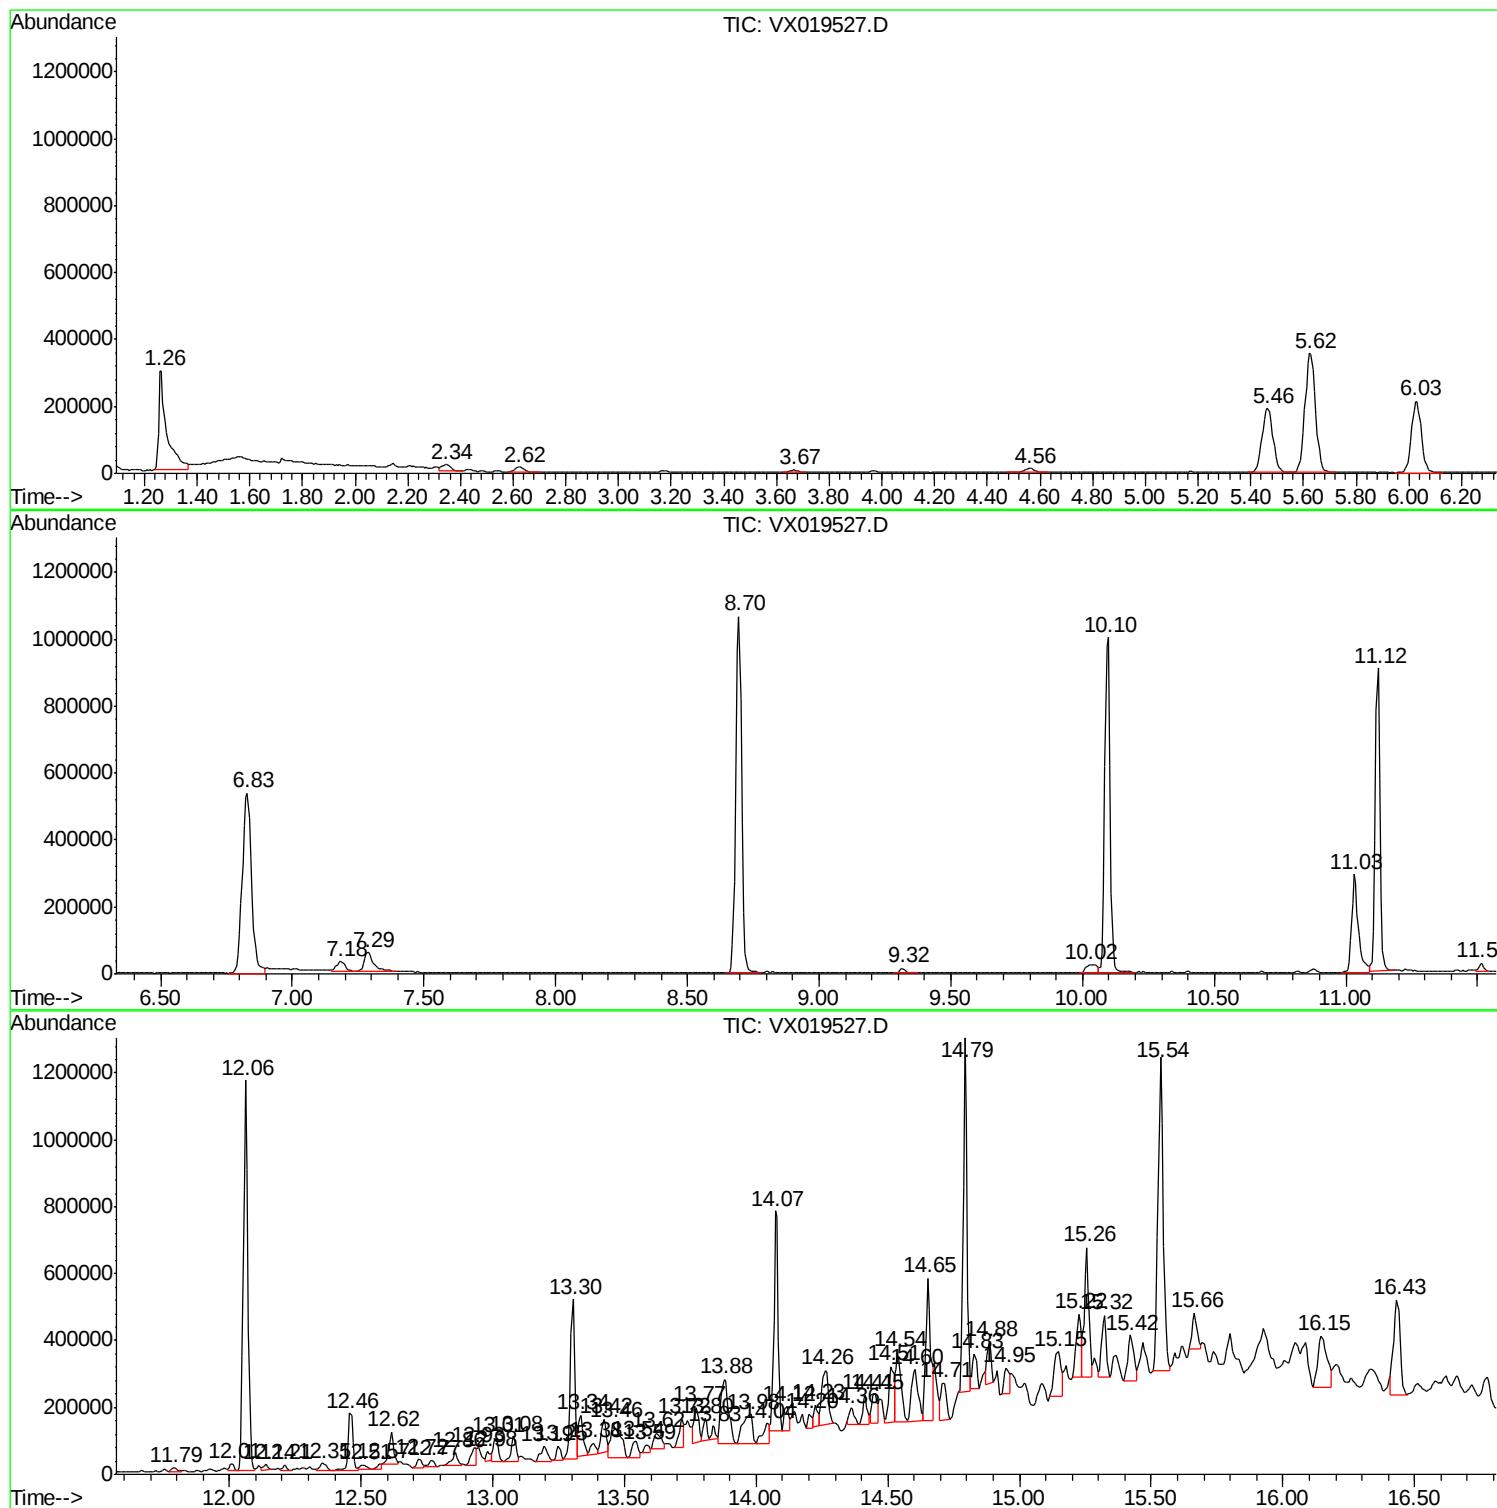

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX112120\
Data File : VX019527.D
Acq On : 21 Nov 2020 05:07
Operator : JC/MD
Sample : L4788-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW181S-GW-20201117

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX112120\
Data File : VX019527.D
Acq On : 21 Nov 2020 05:07
Operator : JC/MD
Sample : L4788-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-MW181S-GW-20201117

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc