


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX112120\
 Data File : VX019533.D
 Acq On : 21 Nov 2020 07:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112120W.M
 Title : SW846 8260
 Last Update : Sat Nov 21 01:57:45 2020

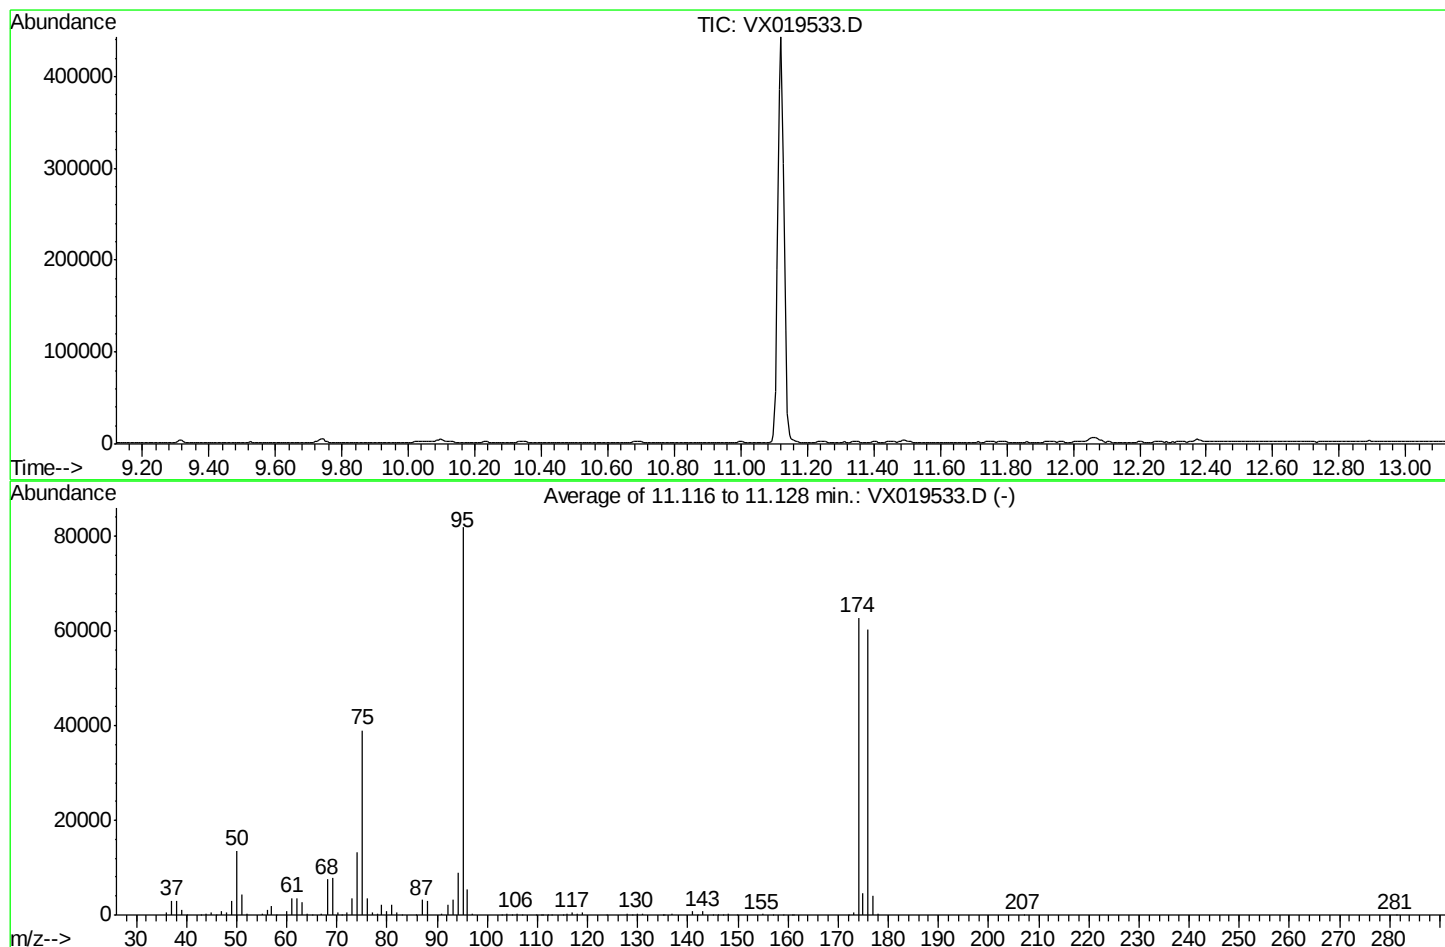

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	13568	PASS
75	95	30	60	47.6	39024	PASS
95	95	100	100	100.0	81922	PASS
96	95	5	9	6.7	5467	PASS
173	174	0.00	2	0.7	453	PASS
174	95	50	100	76.7	62842	PASS
175	174	5	9	7.4	4655	PASS
176	174	95	101	96.2	60456	PASS
177	176	5	9	6.5	3945	PASS