

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
Data File : VX038976.D
Acq On : 21 Nov 2023 11:57
Operator : JC/MD
Sample : VX1121WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1121WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX038976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.520	229	235	245	rBV	7419	14267	1.93%	0.346%
2	5.385	692	705	720	rBV	78391	231411	31.28%	5.608%
3	5.550	720	732	748	rVB	119051	341868	46.21%	8.284%
4	5.952	788	798	812	rBV	90175	242787	32.81%	5.883%
5	6.757	921	930	945	rBV	214579	521447	70.48%	12.636%
6	8.647	1234	1240	1258	rBV	470085	739871	100.00%	17.929%
7	9.275	1336	1343	1348	rBV2	10906	16722	2.26%	0.405%
8	10.055	1465	1471	1489	rBV	503072	714231	96.53%	17.307%
9	11.079	1634	1639	1652	rBV	428239	554518	74.95%	13.437%
10	11.311	1672	1677	1683	rBV	13595	17955	2.43%	0.435%
11	12.018	1788	1793	1807	rBV	568031	731701	98.90%	17.731%




Sum of corrected areas: 4126778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
Data File : VX038976.D
Acq On : 21 Nov 2023 11:57
Operator : JC/MD
Sample : VX1121WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1121WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

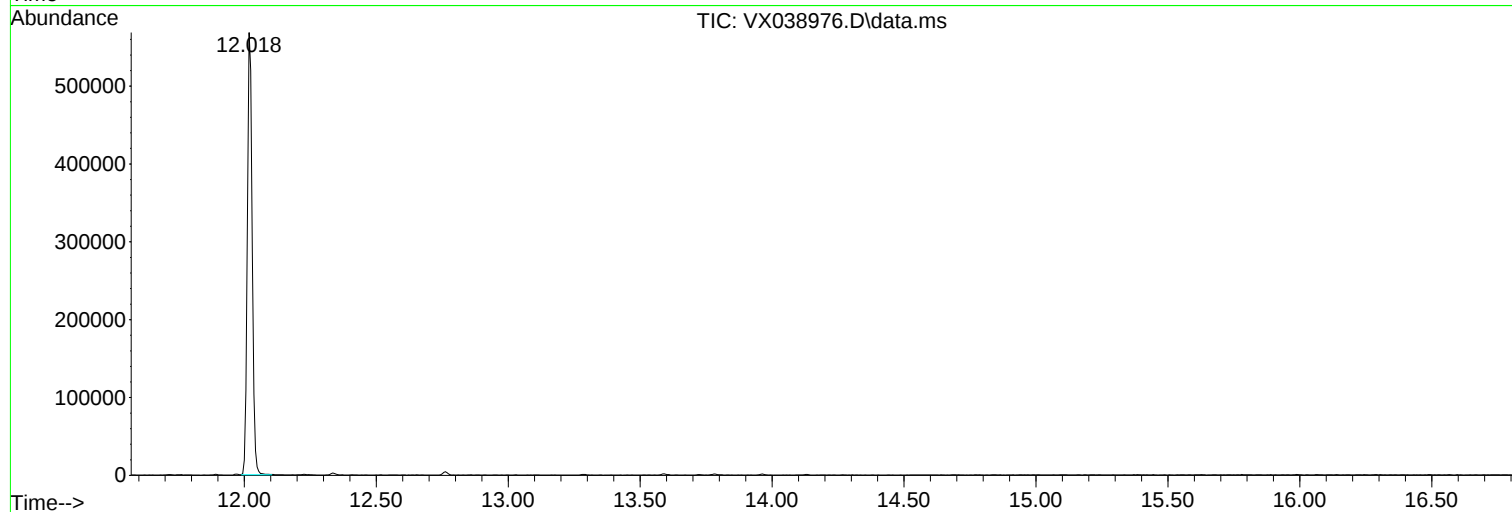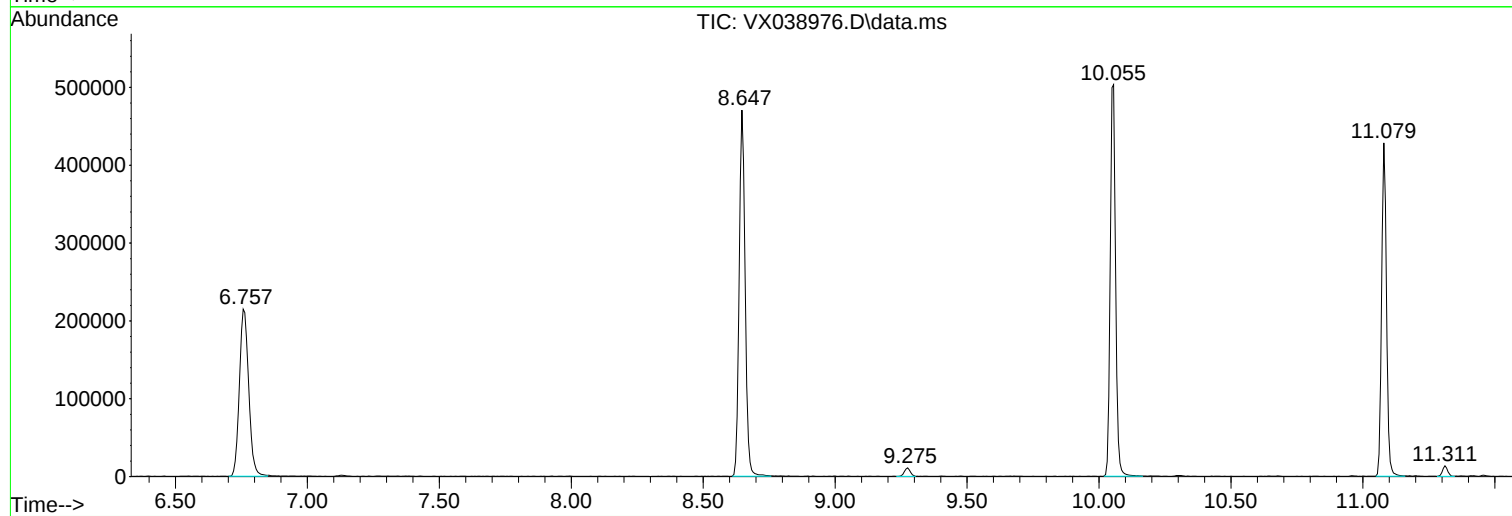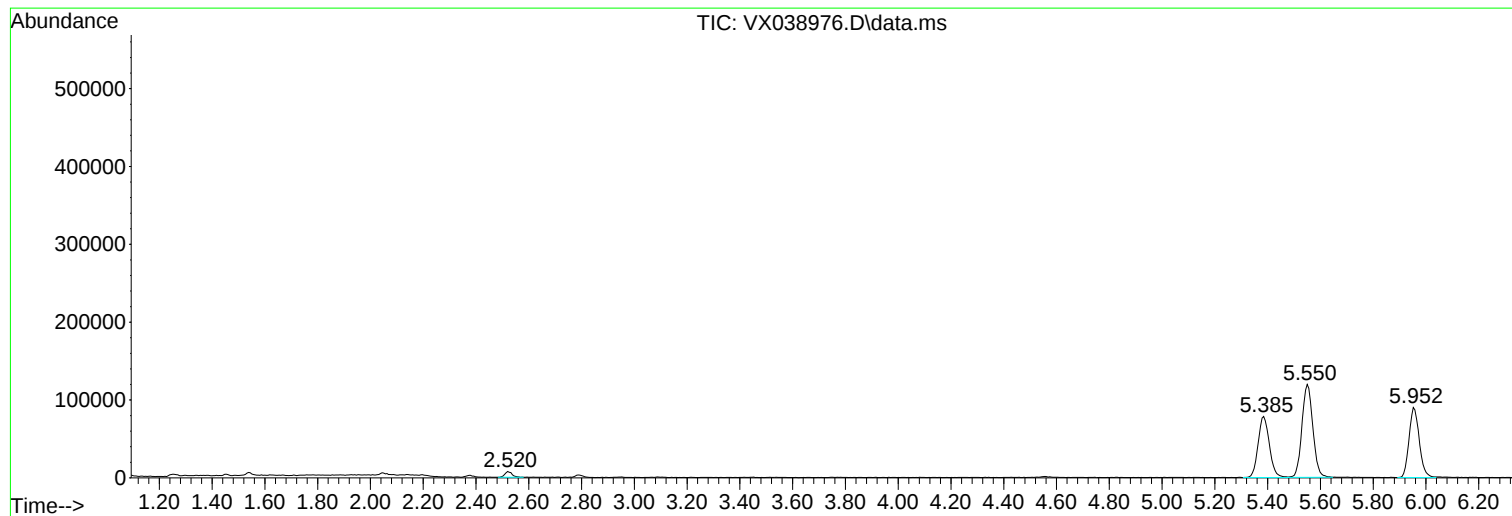

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
Data File : VX038976.D
Acq On : 21 Nov 2023 11:57
Operator : JC/MD
Sample : VX1121WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1121WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
Data File : VX038976.D
Acq On : 21 Nov 2023 11:57
Operator : JC/MD
Sample : VX1121WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1121WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------