

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
 Data File : VX038986.D
 Acq On : 21 Nov 2023 15:50
 Operator : JC/MD
 Sample : 05407-08 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 INTERCEPTOR-SUMP-20231114

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
 Title : SW846 8260

Signal : TIC: VX038986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.794	274	280	286	rBV	6941	13193	1.91%	0.327%
2	4.489	550	558	567	rBV2	17851	49434	7.17%	1.226%
3	5.385	693	705	721	rBV2	71663	212010	30.77%	5.257%
4	5.550	721	732	747	rVV	108020	305402	44.32%	7.573%
5	5.952	788	798	814	rBV	82955	223840	32.49%	5.551%
6	6.763	920	931	955	rBV	196466	482935	70.09%	11.976%
7	7.129	981	991	1000	rBV	92649	205960	29.89%	5.107%
8	8.647	1233	1240	1262	rBV	430829	682042	98.99%	16.913%
9	10.055	1465	1471	1488	rVB	464230	655244	95.10%	16.249%
10	11.079	1634	1639	1653	rVB	397790	513496	74.52%	12.734%
11	12.024	1788	1794	1804	rBV	514859	689031	100.00%	17.087%




Sum of corrected areas: 4032587

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
Data File : VX038986.D
Acq On : 21 Nov 2023 15:50
Operator : JC/MD
Sample : 05407-08 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-SUMP-20231114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

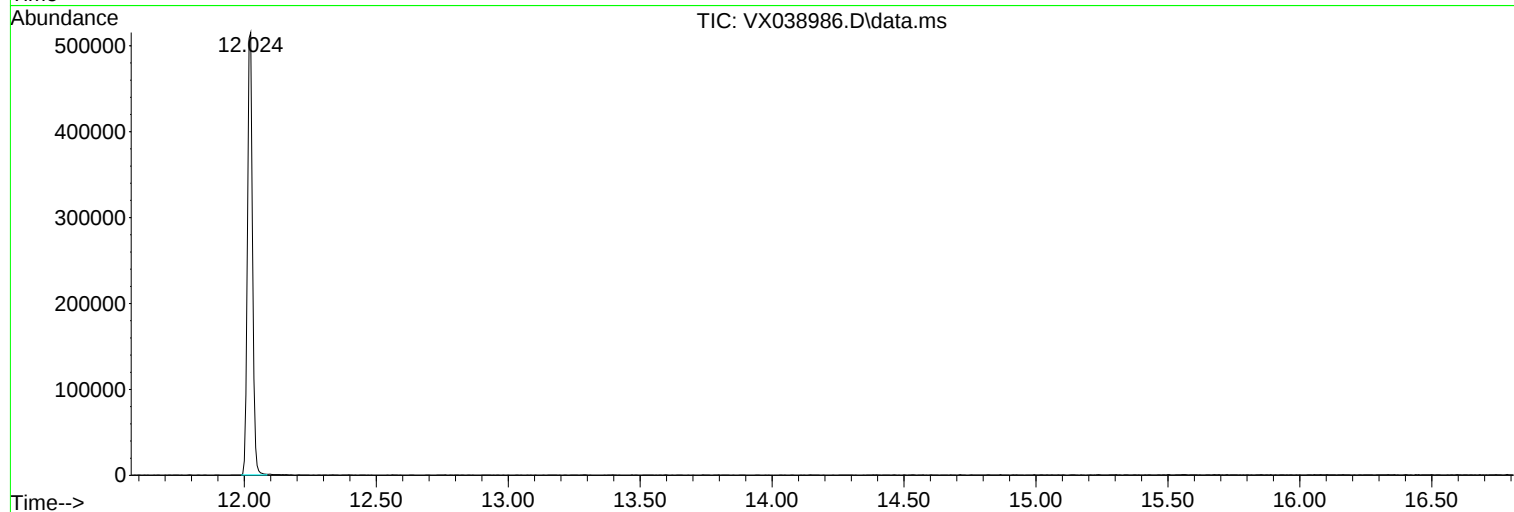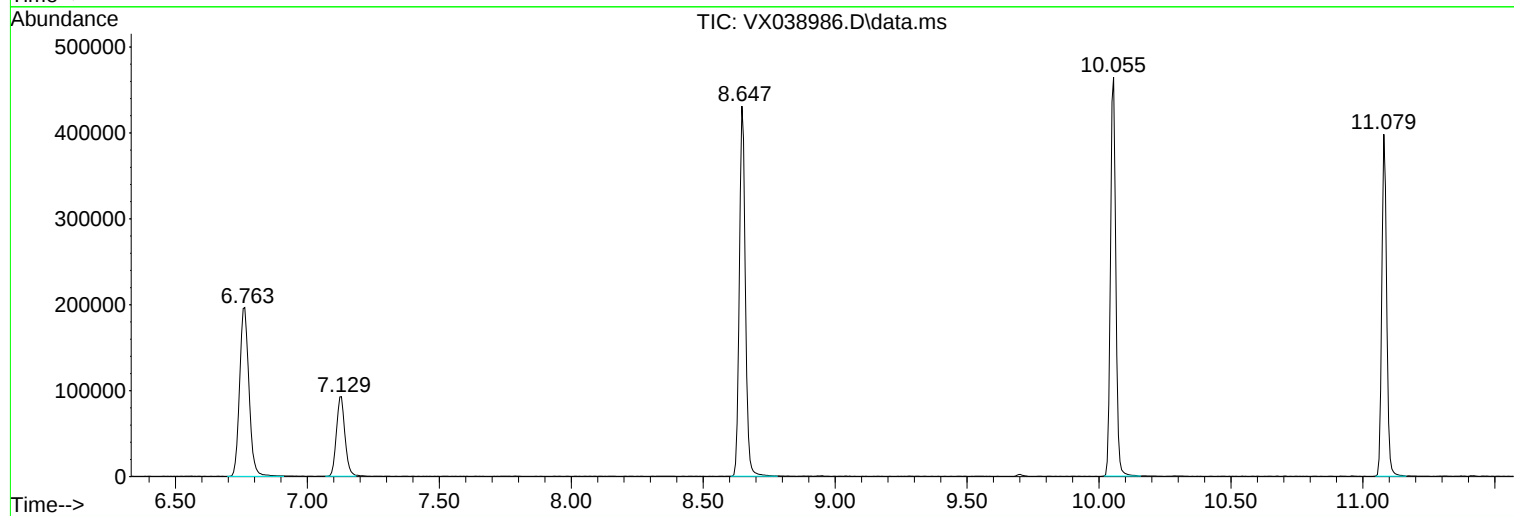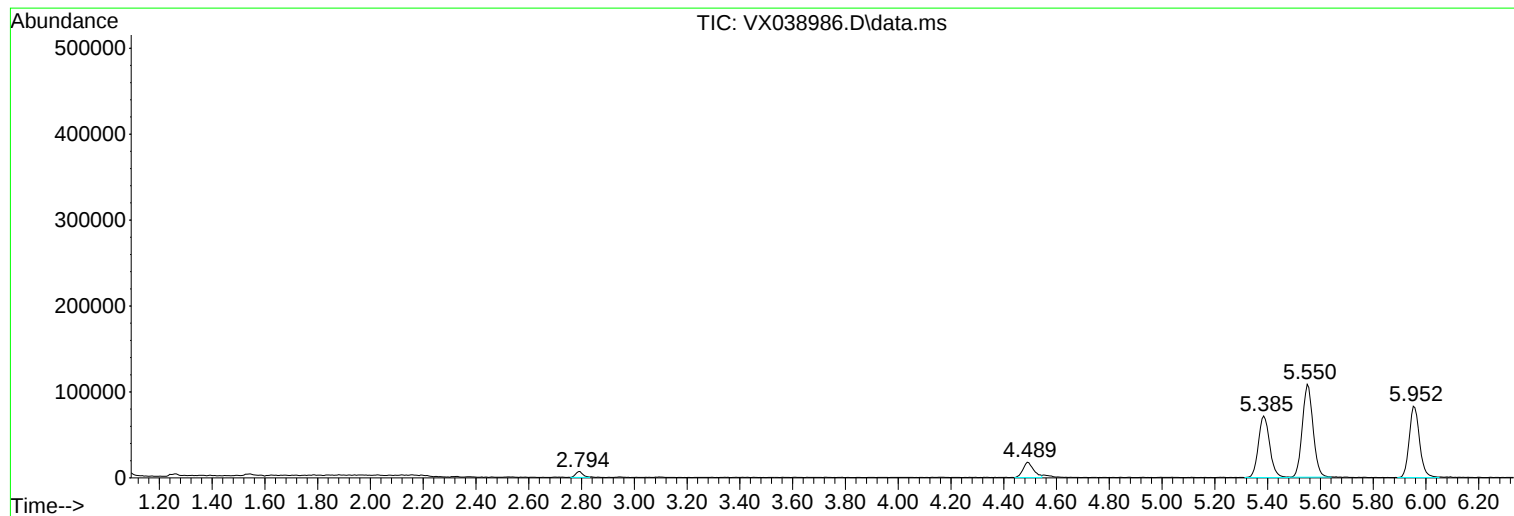

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
Data File : VX038986.D
Acq On : 21 Nov 2023 15:50
Operator : JC/MD
Sample : 05407-08 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-SUMP-20231114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX112123\
Data File : VX038986.D
Acq On : 21 Nov 2023 15:50
Operator : JC/MD
Sample : 05407-08 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
INTERCEPTOR-SUMP-20231114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc